

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
 Data File : FF008779.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jul 2021 10:29
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 16 01:44:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.519	3162544	23.253 ug/ml
12) N-OCTACOSANE	16.920	2748690	22.223 ug/ml
13) N-TRIACONTANE	17.803	191001	1.594 ug/ml
14) N-DOTRIACONTANE	18.633	294115	2.510 ug/ml
15) N-TETRATRIACONTANE	19.414	224377	2.146 ug/ml
16) N-HEXATRIACONTANE	20.150	120872	1.287 ug/ml
17) N-OCTATRIACONTANE	20.895	124372	1.509 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008779.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2021 10:29
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 01:44:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

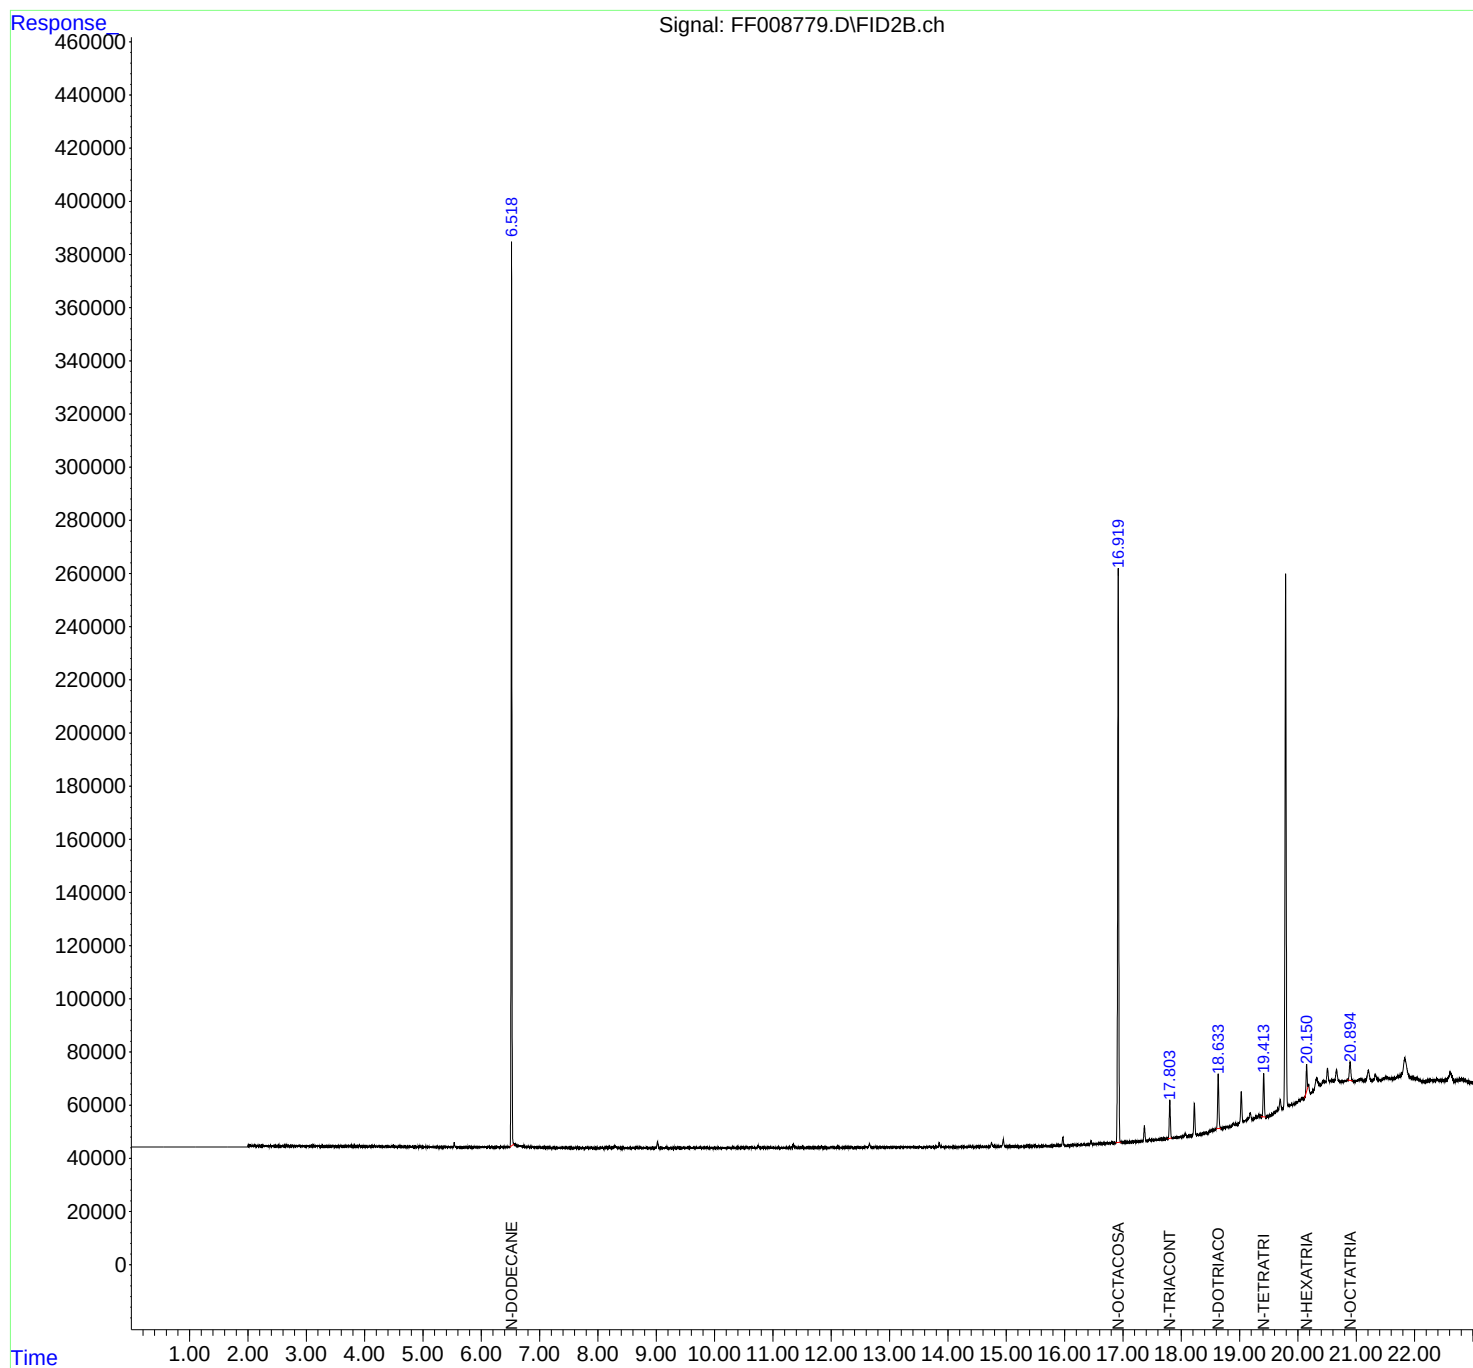


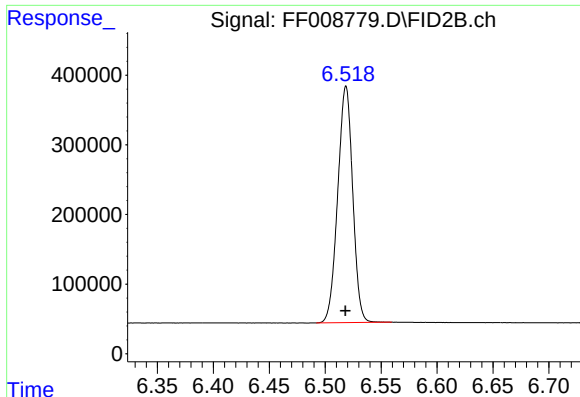

#3 N-DODECANE


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 3162544
Conc: 23.25 ug/ml

Instrument :
FID_F
ClientSampleId :

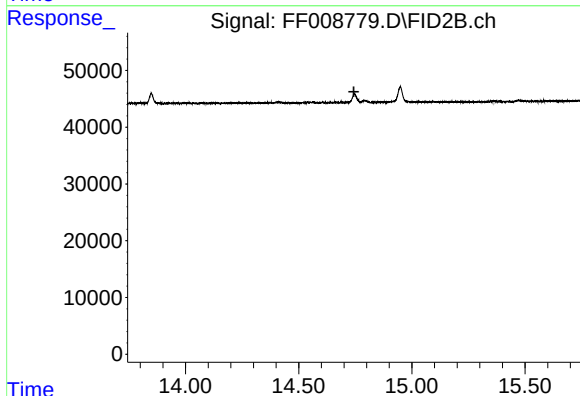


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.744 min
Response: 0
Conc: N.D.

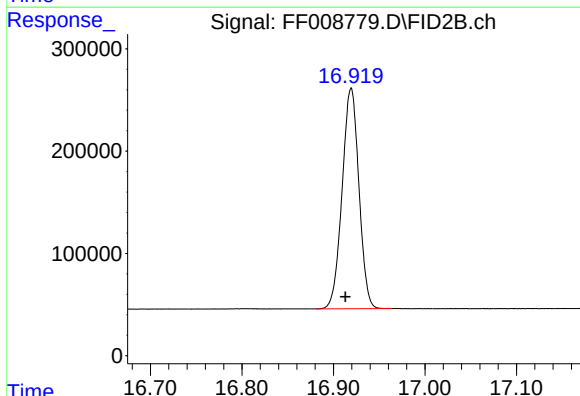


#12 N-OCTACOSANE

R.T.: 16.920 min
Delta R.T.: 0.006 min
Response: 2748690
Conc: 22.22 ug/ml

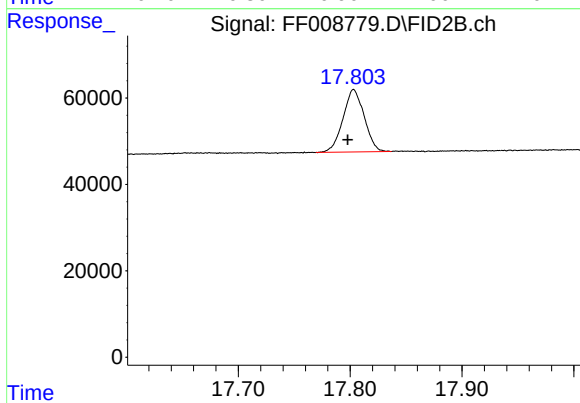

#13 N-TRIACONTANE


R.T.: 17.803 min
Delta R.T.: 0.005 min
Response: 191001
Conc: 1.59 ug/ml

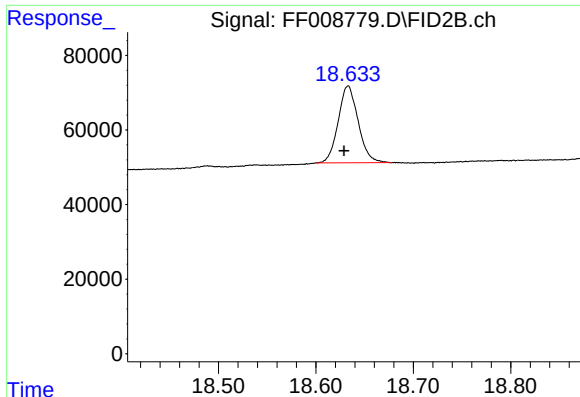

#14 N-DOTRIACONTANE


R.T.: 18.633 min
Delta R.T.: 0.005 min
Response: 294115
Conc: 2.51 ug/ml

Instrument :
FID_F
ClientSampleId :

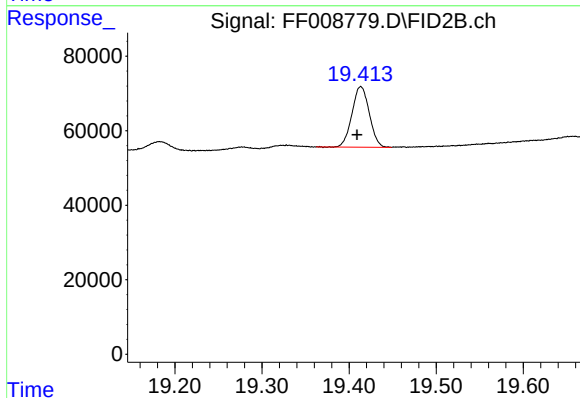


#15 N-TETRATRIACONTANE

R.T.: 19.414 min
Delta R.T.: 0.004 min
Response: 224377
Conc: 2.15 ug/ml

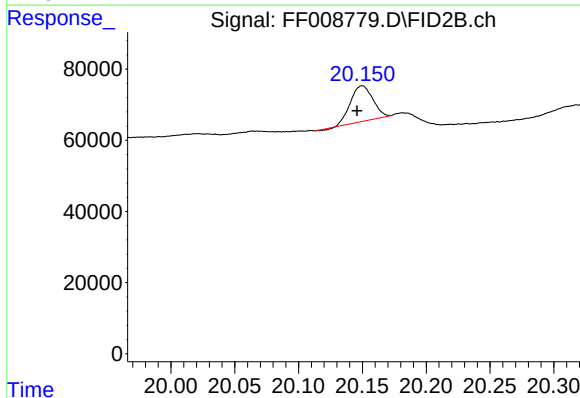

#16 N-HEXATRIACONTANE

R.T.: 20.150 min
Delta R.T.: 0.005 min
Response: 120872
Conc: 1.29 ug/ml

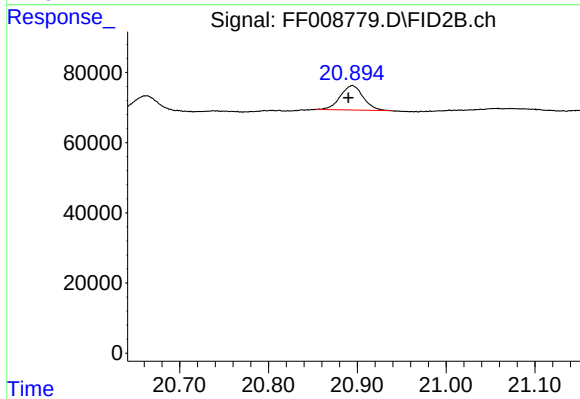

#17 N-OCTATRIACONTANE

R.T.: 20.895 min
Delta R.T.: 0.005 min
Response: 124372
Conc: 1.51 ug/ml