

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
 Data File : FF008783.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jul 2021 12:33
 Operator : DD\AJ
 Sample : M3026-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 16 01:44:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.748	1434374	12.586 ug/ml
Target Compounds			
4) N-TETRADECANE	8.311	164494	1.219 ug/ml
10) N-TETRACOSANE	14.945	295783	2.245 ug/ml
13) N-TRIACONTANE	17.802	119154	0.994 ug/ml
14) N-DOTRIACONTANE	18.631	127379	1.087 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008783.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2021 12:33
Operator : DD\AJ
Sample : M3026-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 01:44:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

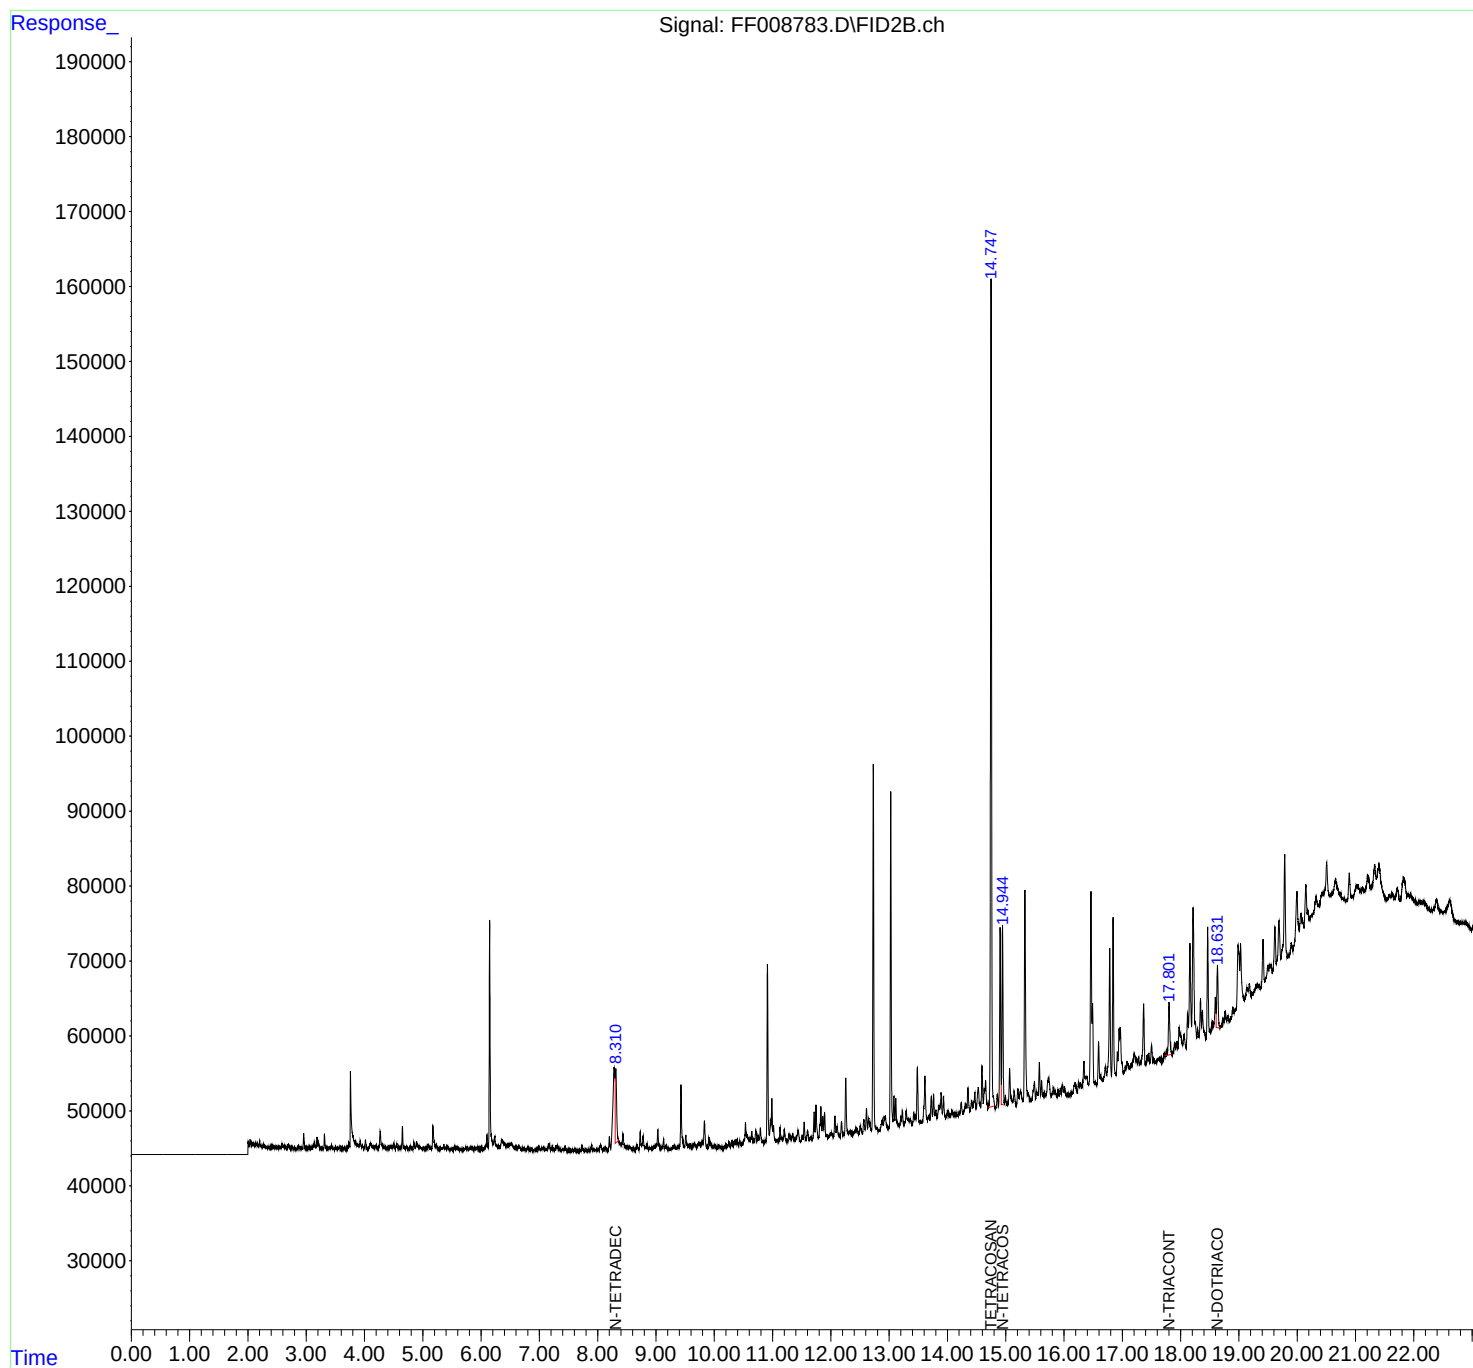


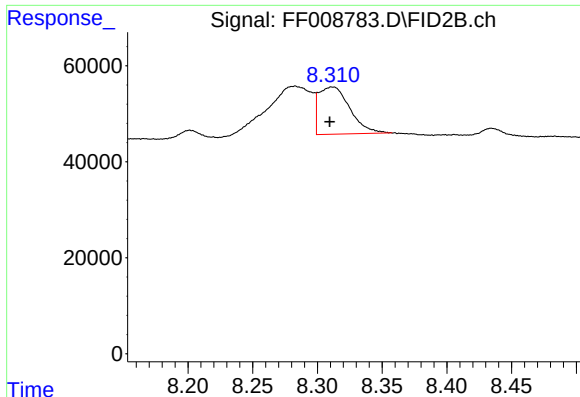

#4 N-TETRADECANE


R.T.: 8.311 min
Delta R.T.: 0.001 min
Response: 164494
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :

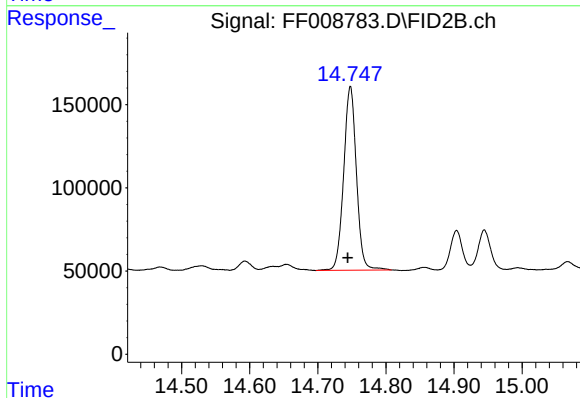


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.748 min
Delta R.T.: 0.004 min
Response: 1434374
Conc: 12.59 ug/ml

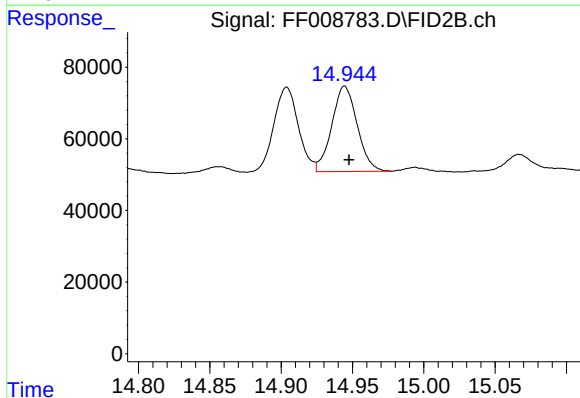


#10 N-TETRACOSANE

R.T.: 14.945 min
Delta R.T.: -0.003 min
Response: 295783
Conc: 2.24 ug/ml

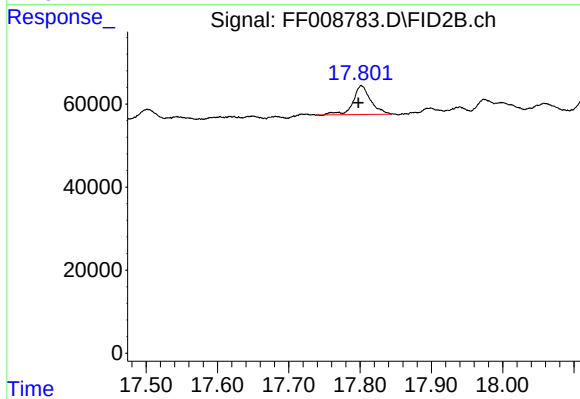

#13 N-TRIACONTANE

R.T.: 17.802 min
Delta R.T.: 0.004 min
Response: 119154
Conc: 0.99 ug/ml

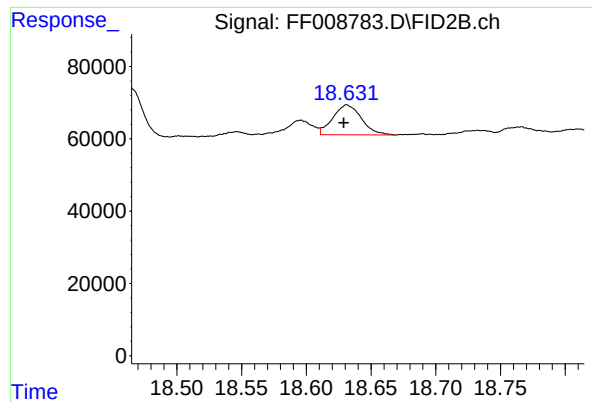

#14 N-DOTRIACONTANE

R.T.: 18.631 min
Delta R.T.: 0.002 min
Response: 127379
Conc: 1.09 ug/ml

Instrument :
FID_F
ClientSampleId :