

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF071521\  
 Data File : FF008784.D  
 Signal(s) : FID2B.ch  
 Acq On : 15 Jul 2021 13:05  
 Operator : DD\AJ  
 Sample : M3026-08  
 Misc :  
 ALS Vial : 59 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jul 16 01:44:42 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062321.M  
 Quant Title :  
 QLast Update : Thu Jun 24 08:07:11 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units   |
|-------------------------------|---------|----------|--------------|
| -----                         |         |          |              |
| System Monitoring Compounds   |         |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.749  | 1820603  | 15.975 ug/ml |
| Target Compounds              |         |          |              |
| 4) N-TETRADECANE              | 8.269   | 829827   | 6.151 ug/ml  |
| 10) N-TETRACOSANE             | 14.946  | 359271   | 2.727 ug/ml  |
| 12) N-OCTACOSANE              | 16.843f | 295777   | 2.391 ug/ml  |
| -----                         |         |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF071521\  
Data File : FF008784.D  
Signal(s) : FID2B.ch  
Acq On : 15 Jul 2021 13:05  
Operator : DD\AJ  
Sample : M3026-08  
Misc :  
ALS Vial : 59 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 16 01:44:42 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062321.M  
Quant Title :  
QLast Update : Thu Jun 24 08:07:11 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

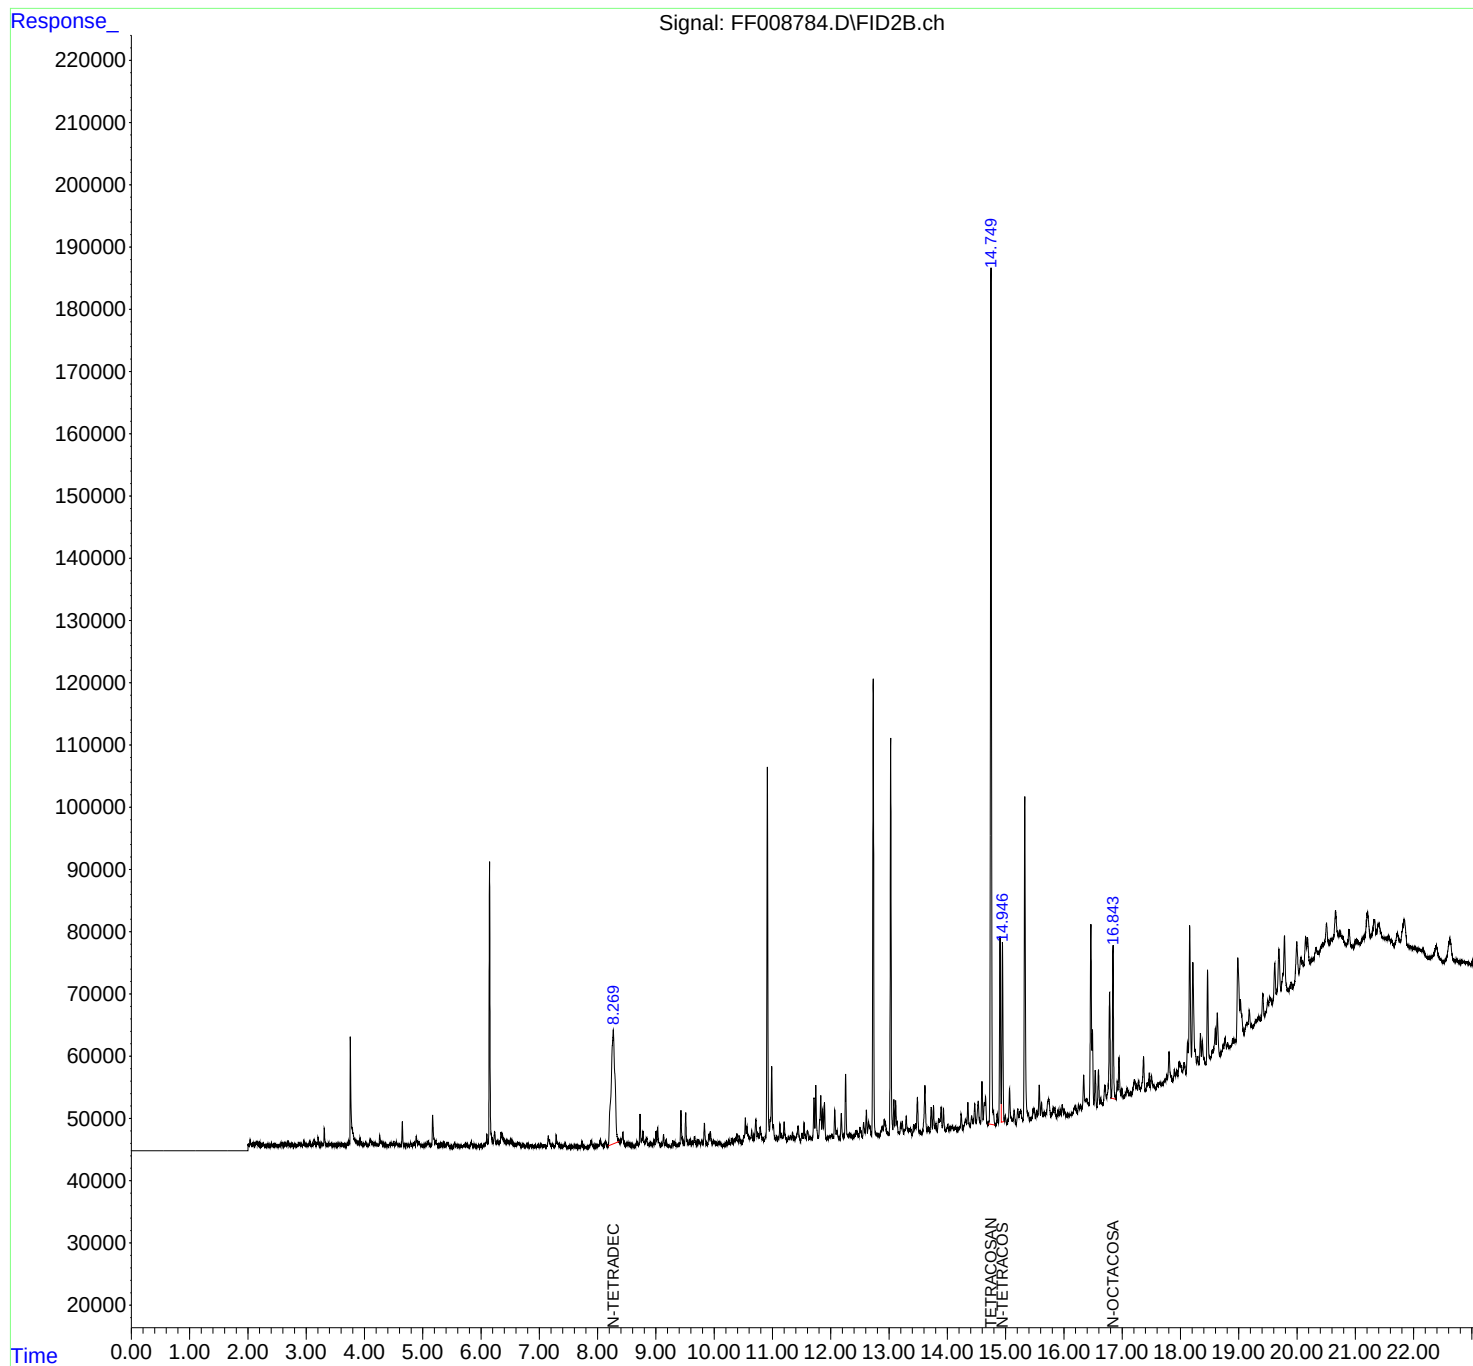


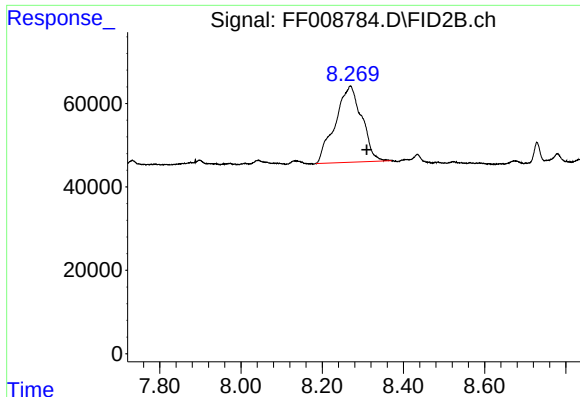

#4 N-TETRADECANE


R.T.: 8.269 min  
Delta R.T.: -0.040 min  
Response: 829827  
Conc: 6.15 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

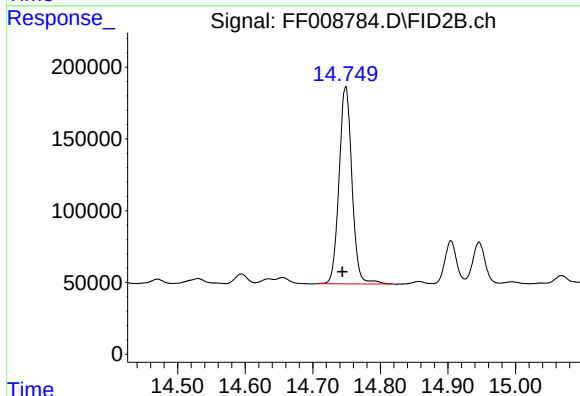


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.749 min  
Delta R.T.: 0.005 min  
Response: 1820603  
Conc: 15.97 ug/ml

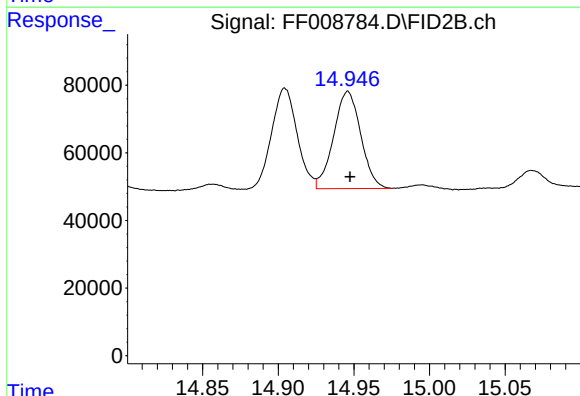

#10 N-TETRACOSANE

R.T.: 14.946 min  
Delta R.T.: -0.001 min  
Response: 359271  
Conc: 2.73 ug/ml

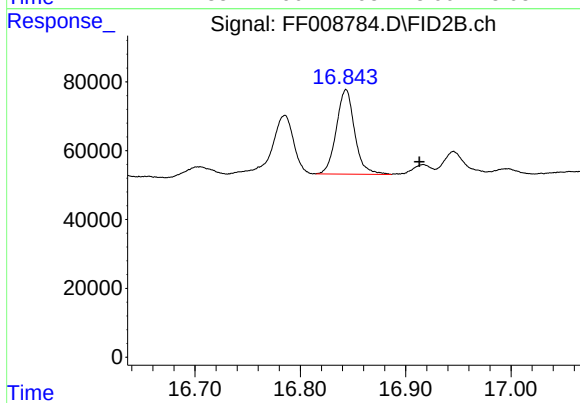

#12 N-OCTACOSANE

R.T.: 16.843 min  
Delta R.T.: -0.070 min  
Response: 295777  
Conc: 2.39 ug/ml