

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008785.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2021 13:36
Operator : DD\AJ
Sample : M3026-11
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 01:44:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.748	1434578	12.587 ug/ml
Target Compounds			
4) N-TETRADECANE	8.255f	350357	2.597 ug/ml
10) N-TETRACOSANE	14.946	166618	1.264 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008785.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2021 13:36
Operator : DD\AJ
Sample : M3026-11
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 01:44:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

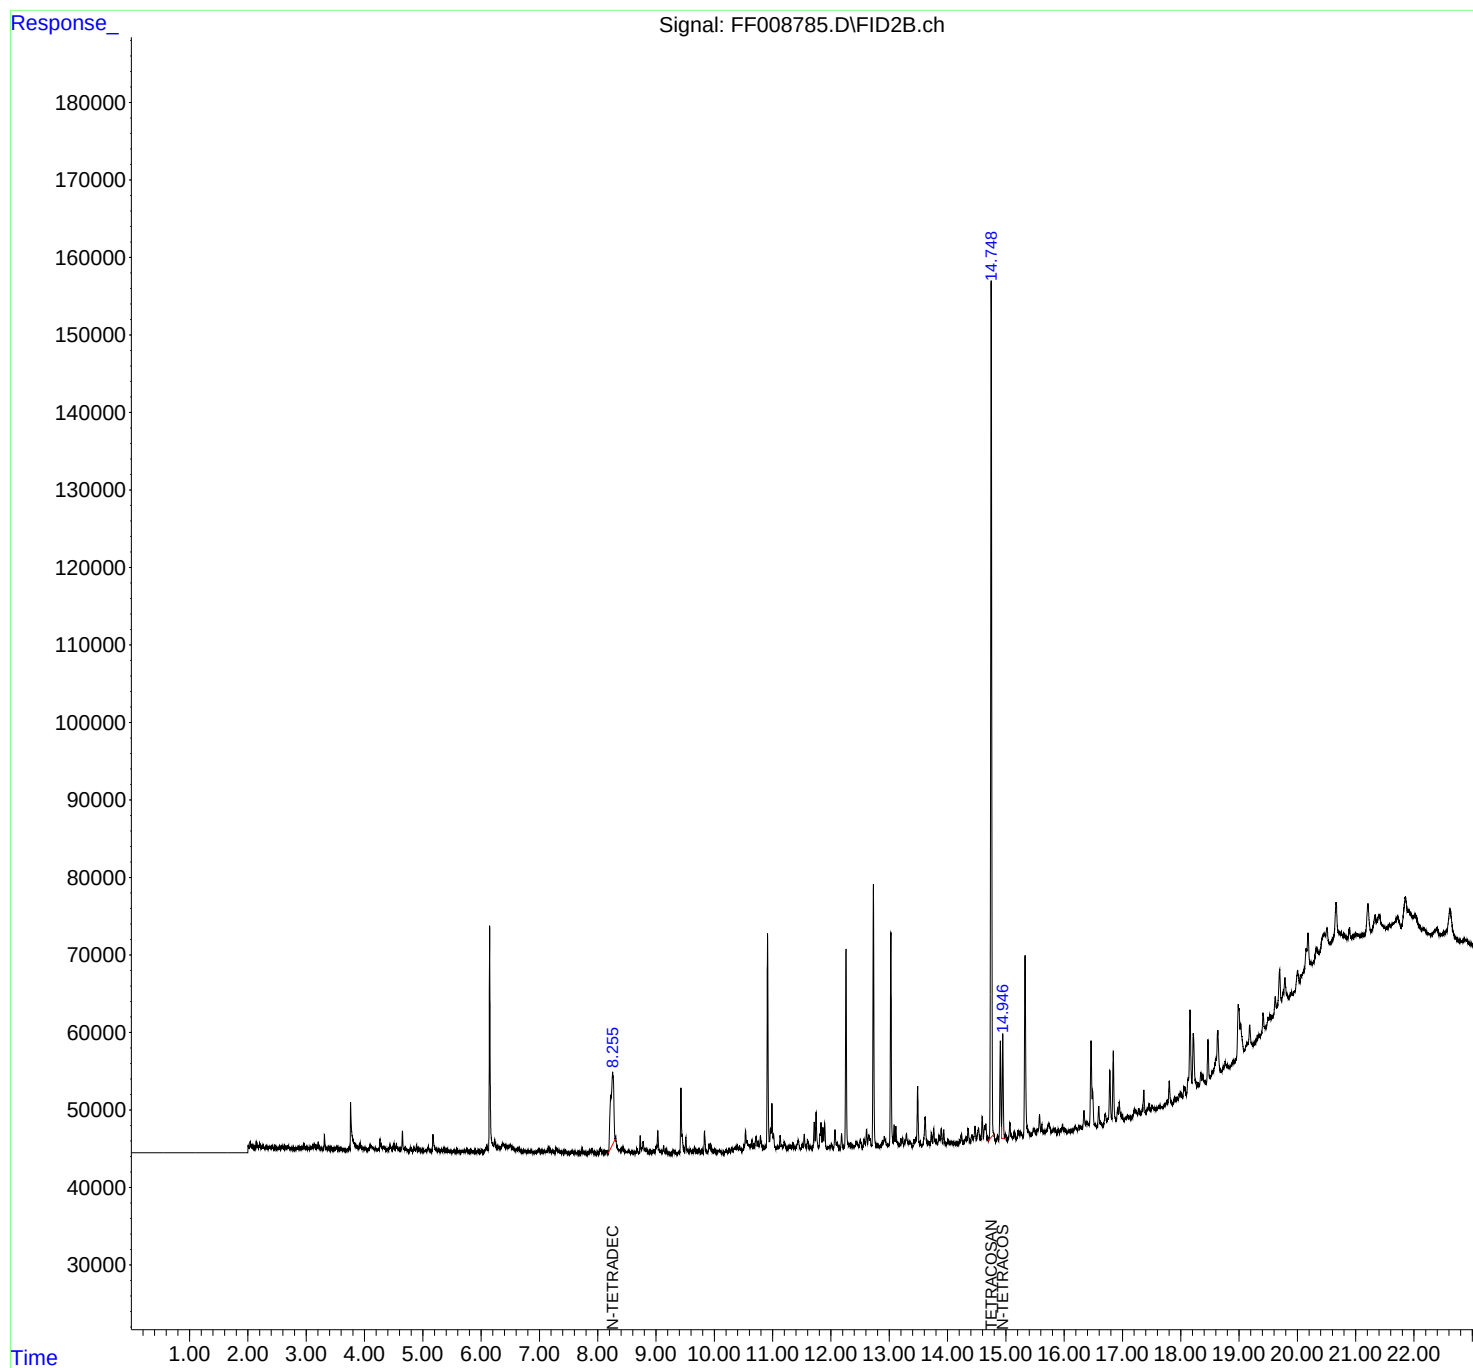


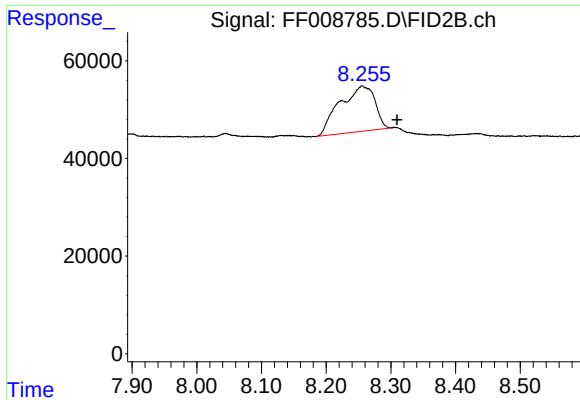

#4 N-TETRADECANE


R.T.: 8.255 min
Delta R.T.: -0.054 min
Response: 350357
Conc: 2.60 ug/ml

Instrument :
FID_F
ClientSampleId :

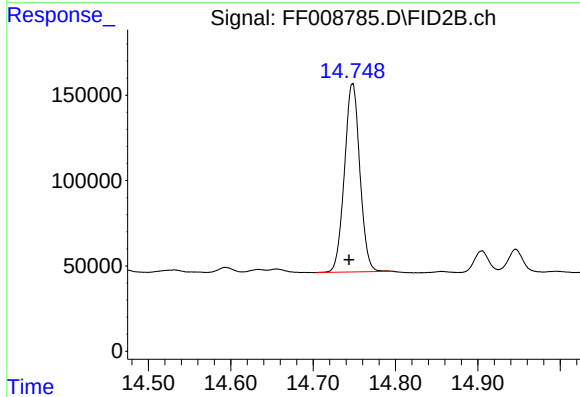

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.748 min
Delta R.T.: 0.004 min
Response: 1434578
Conc: 12.59 ug/ml

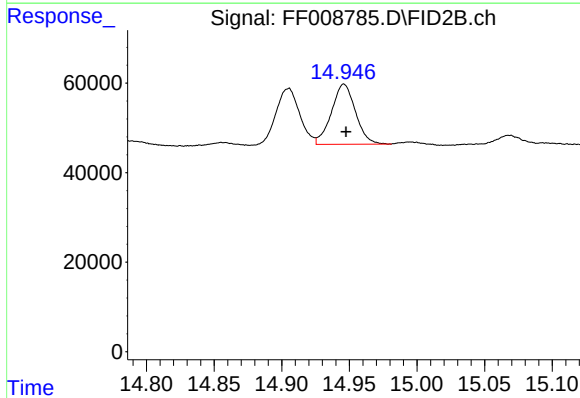

#10 N-TETRACOSANE

R.T.: 14.946 min
Delta R.T.: -0.002 min
Response: 166618
Conc: 1.26 ug/ml