

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008806.D
Signal(s) : FID2B.ch
Acq On : 16 Jul 2021 00:42
Operator : DD\AJ
Sample : M3039-02
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 01:47:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	2103247	18.455 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.942	214532	1.628 ug/ml
13) N-TRIACONTANE	17.804	172082	1.436 ug/ml
14) N-DOTRIACONTANE	18.627	236767	2.021 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008806.D
Signal(s) : FID2B.ch
Acq On : 16 Jul 2021 00:42
Operator : DD\AJ
Sample : M3039-02
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 01:47:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

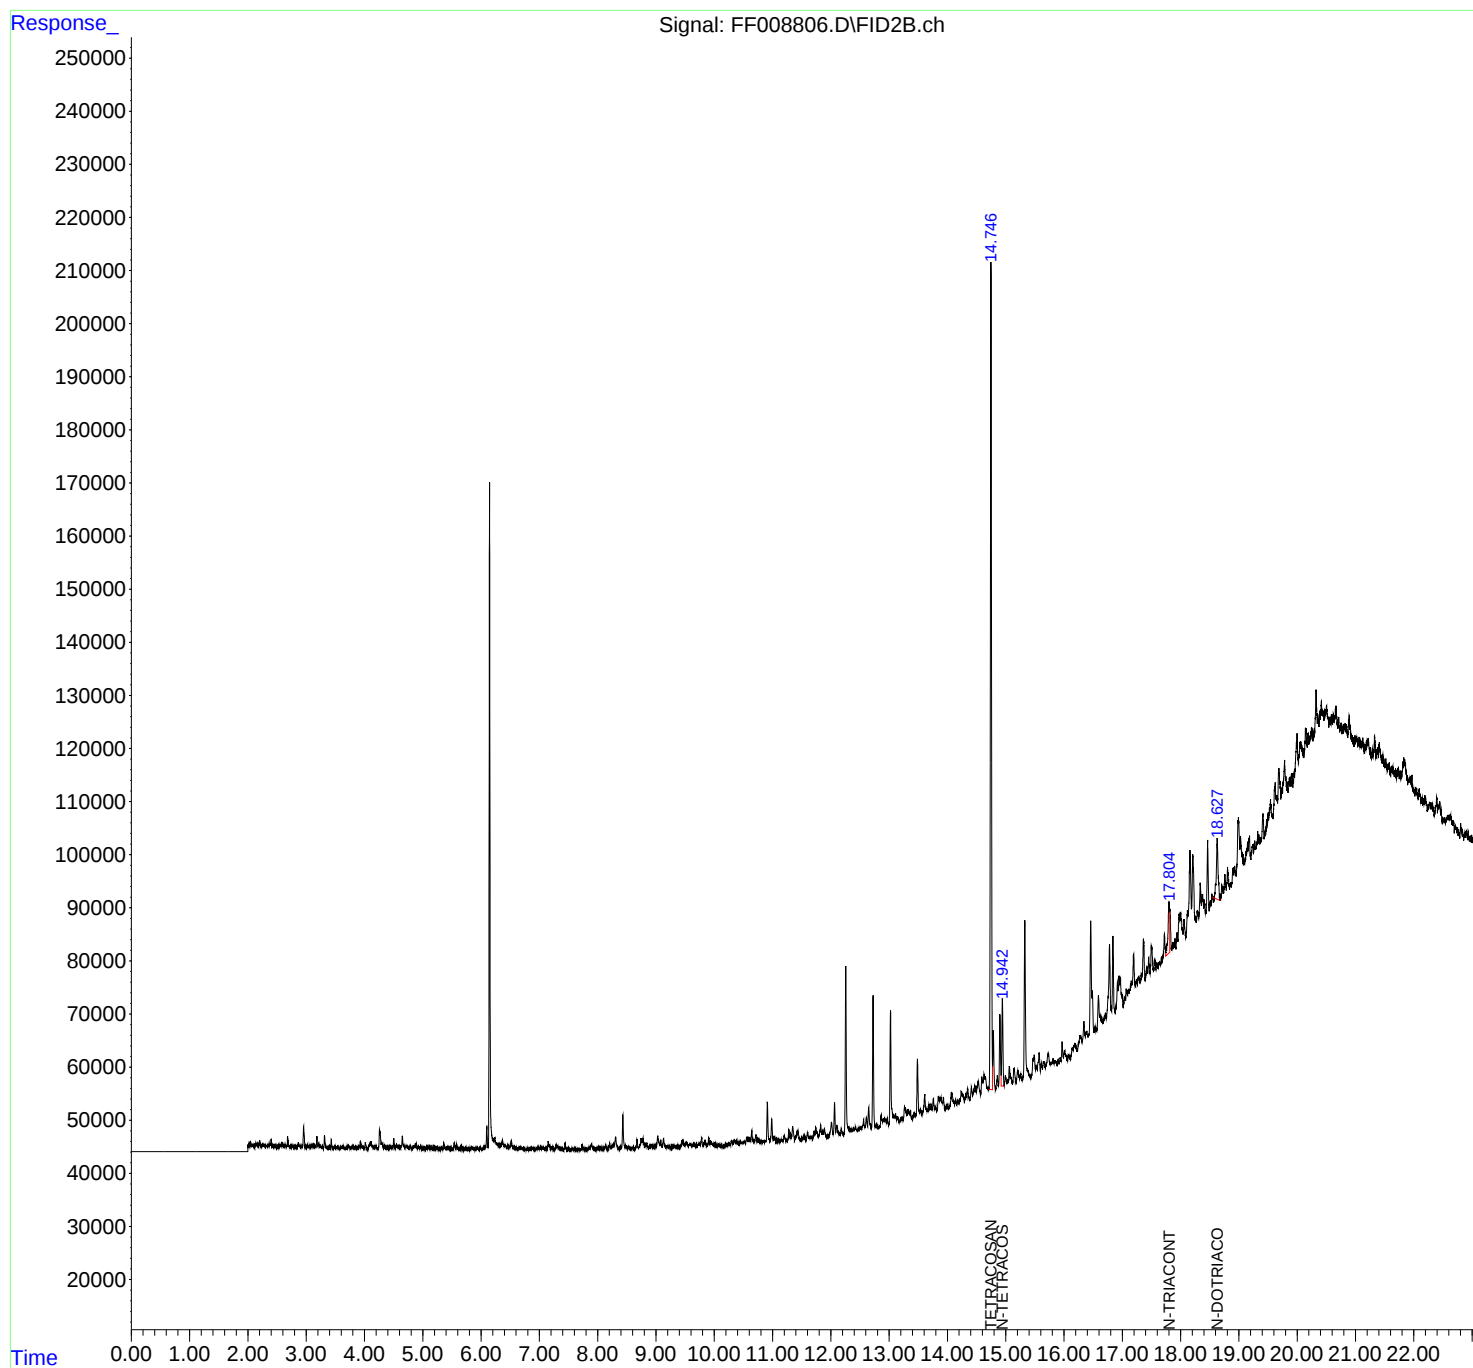


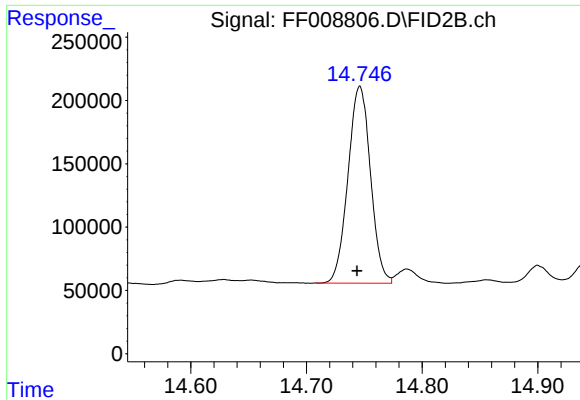

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.746 min
Delta R.T.: 0.002 min
Response: 2103247
Conc: 18.45 ug/ml

Instrument :
FID_F
ClientSampleId :

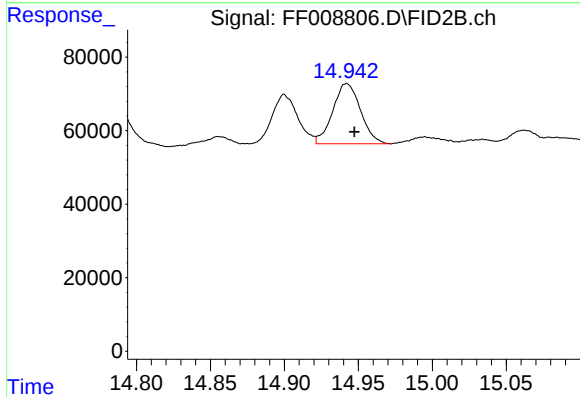


#10 N-TETRACOSANE

R.T.: 14.942 min
Delta R.T.: -0.005 min
Response: 214532
Conc: 1.63 ug/ml

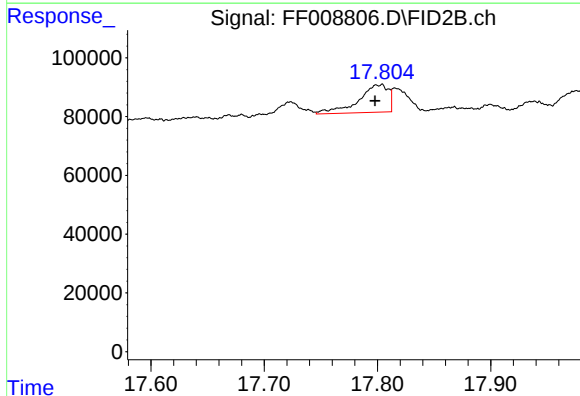

#13 N-TRIACONTANE

R.T.: 17.804 min
Delta R.T.: 0.006 min
Response: 172082
Conc: 1.44 ug/ml

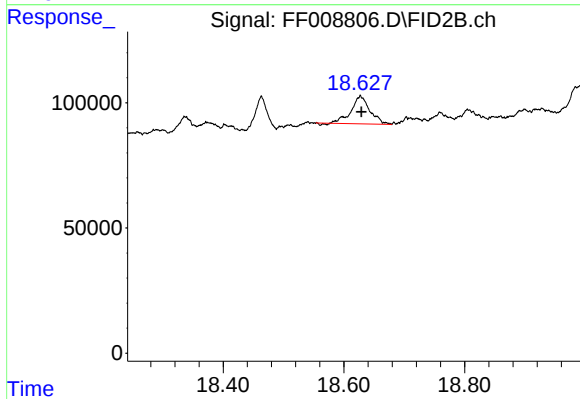

#14 N-DOTRIACONTANE

R.T.: 18.627 min
Delta R.T.: -0.002 min
Response: 236767
Conc: 2.02 ug/ml