

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008807.D
Signal(s) : FID2B.ch
Acq On : 16 Jul 2021 09:32
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 11:31:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.741	1861227	16.331 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.629	258992	2.211 ug/ml
16) N-HEXATRIACONTANE	20.180	127977	1.362 ug/ml
18) N-TETRACONTANE	21.847	123594	1.335 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071521\
Data File : FF008807.D
Signal(s) : FID2B.ch
Acq On : 16 Jul 2021 09:32
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 11:31:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

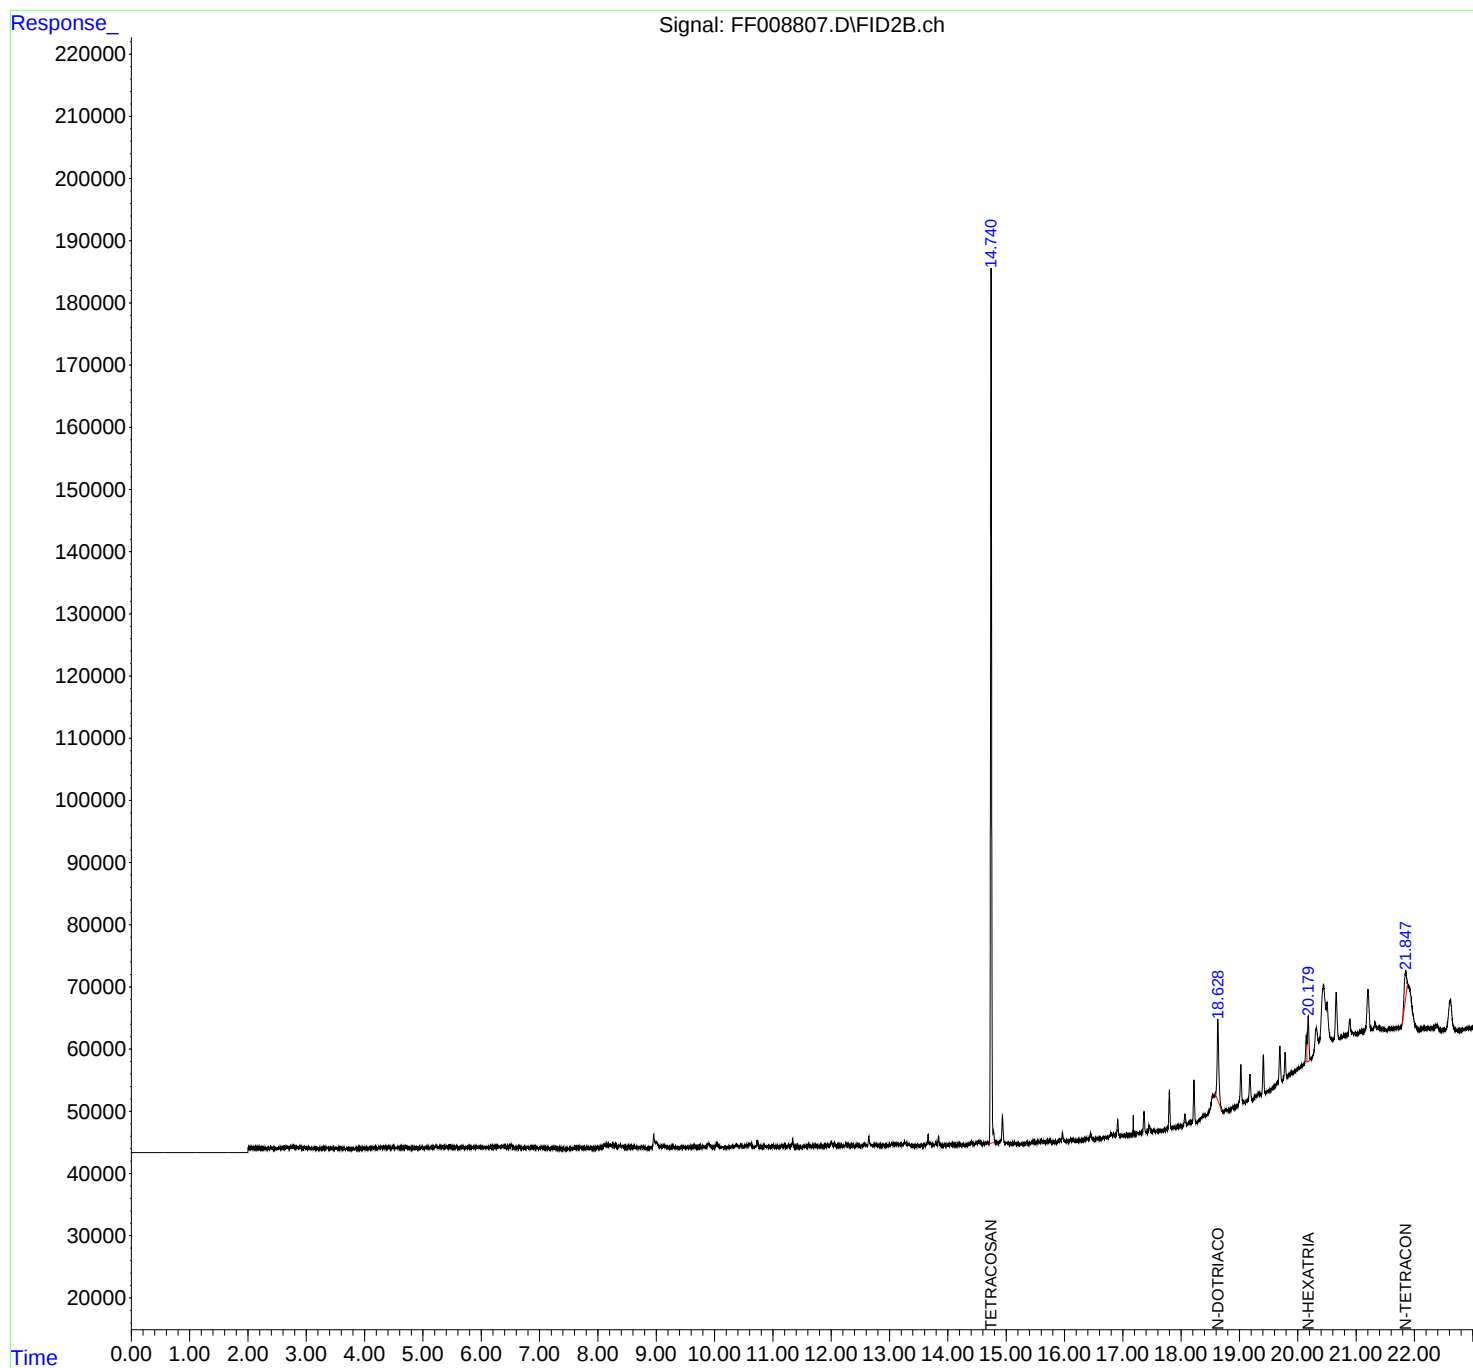


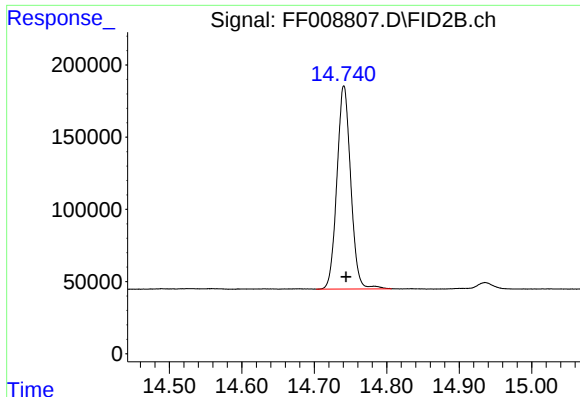

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.741 min
Delta R.T.: -0.003 min
Response: 1861227
Conc: 16.33 ug/ml

Instrument :
FID_F
ClientSampleId :

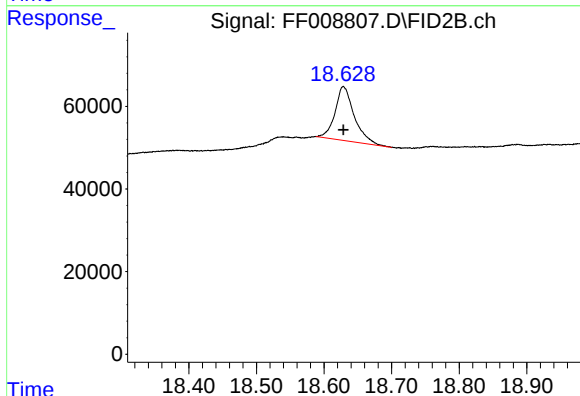


#14 N-DOTRIACONTANE

R.T.: 18.629 min
Delta R.T.: 0.000 min
Response: 258992
Conc: 2.21 ug/ml

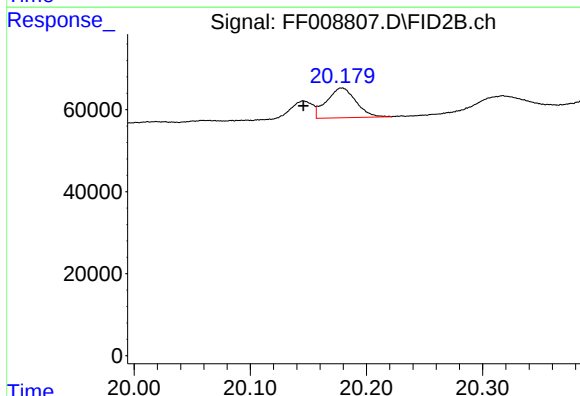

#16 N-HEXATRIACONTANE

R.T.: 20.180 min
Delta R.T.: 0.034 min
Response: 127977
Conc: 1.36 ug/ml

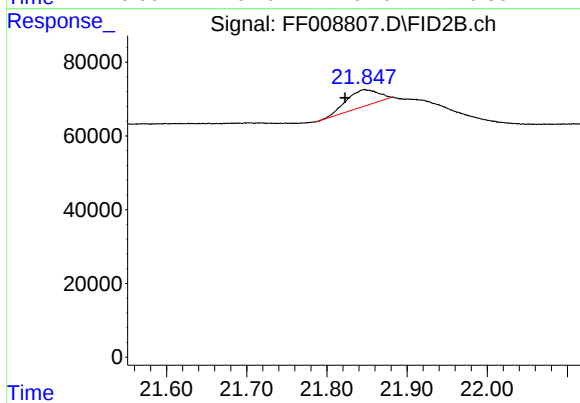

#18 N-TETRACONTANE

R.T.: 21.847 min
Delta R.T.: 0.024 min
Response: 123594
Conc: 1.34 ug/ml