

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071522\
Data File : FF011046.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2022 16:57
Operator : AJ\MA
Sample : I,BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 15 23:29:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.810	1871470	19.950 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.698	69096	0.644 ug/ml
16) N-HEXATRIACONTANE	20.289f	168653	1.961 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071522\
Data File : FF011046.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2022 16:57
Operator : AJ\MA
Sample : I,BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 15 23:29:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

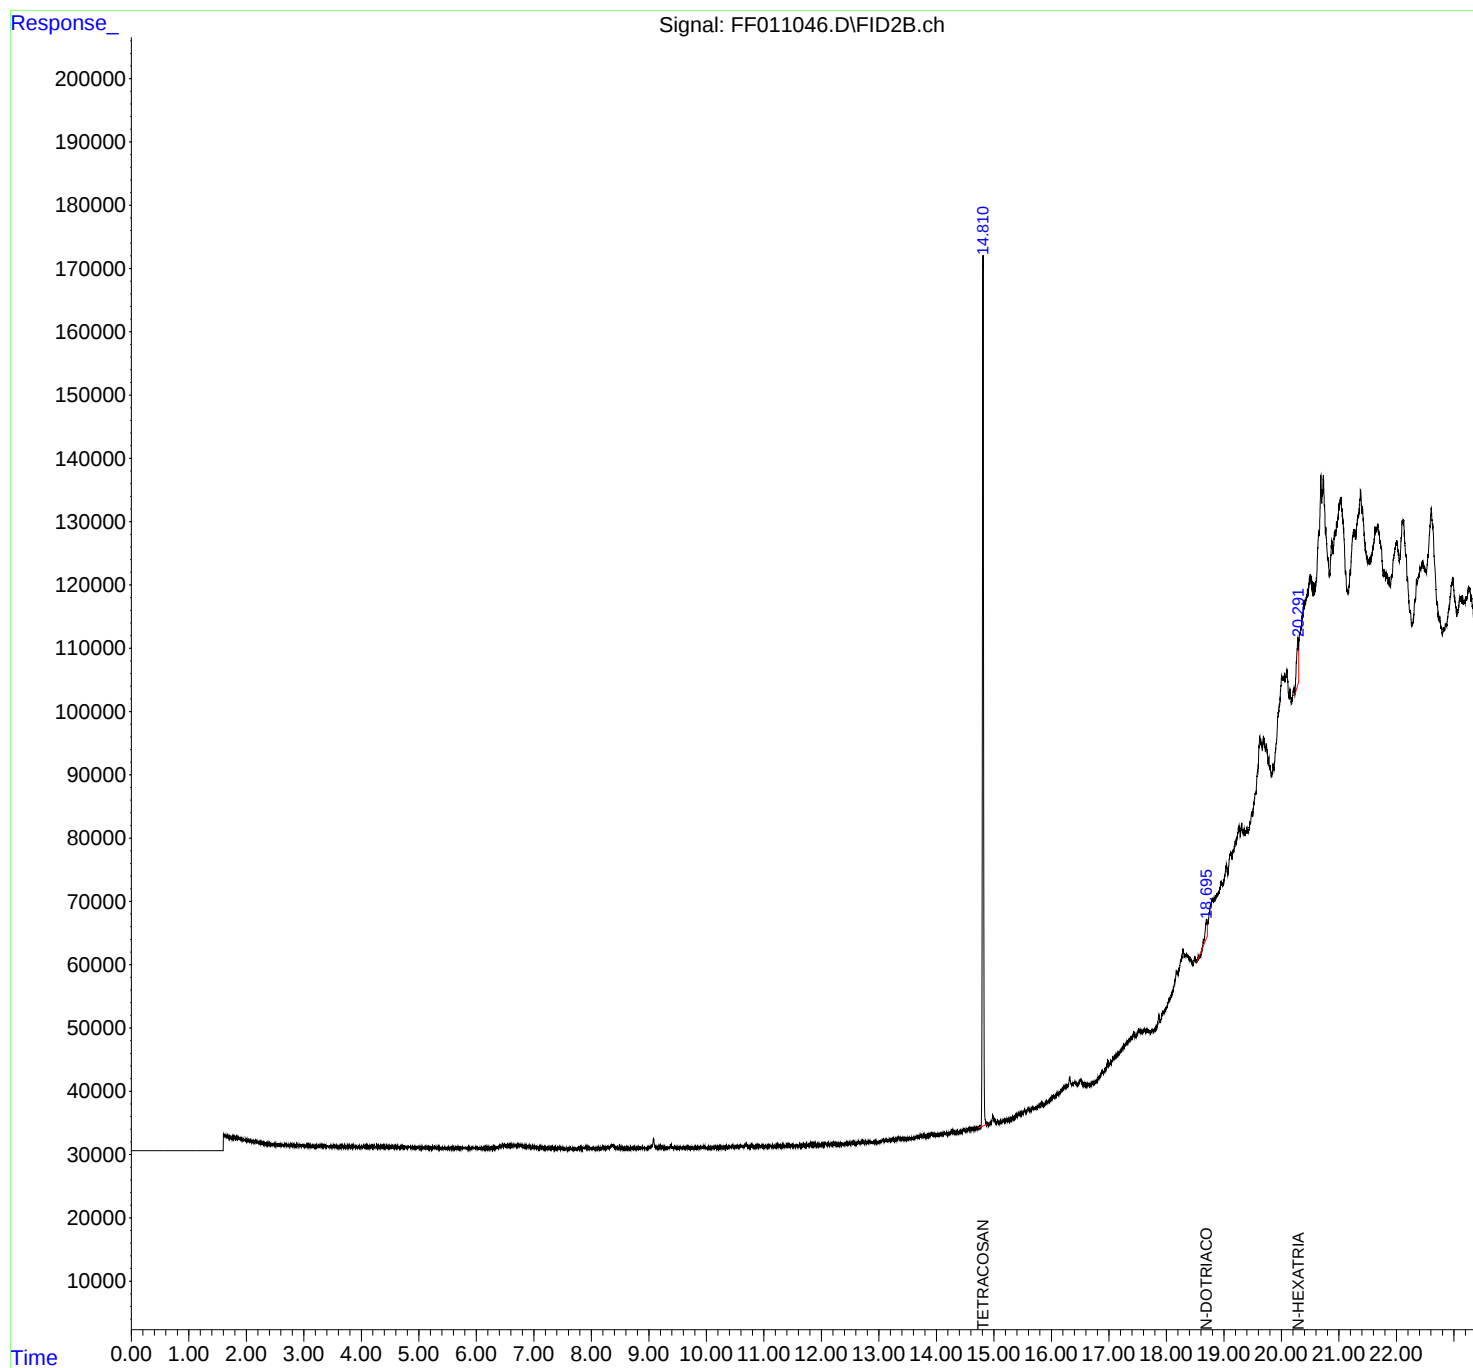

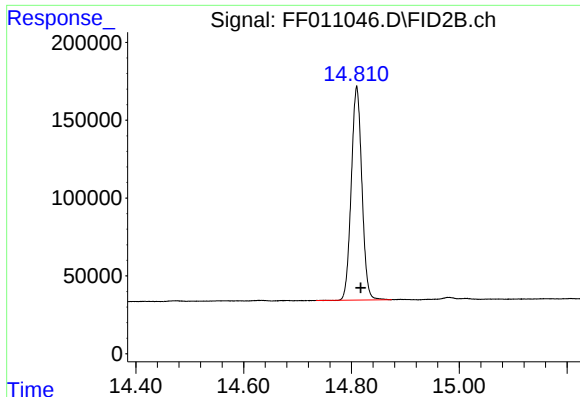


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.810 min
Delta R.T.: -0.007 min
Response: 1871470
Conc: 19.95 ug/ml

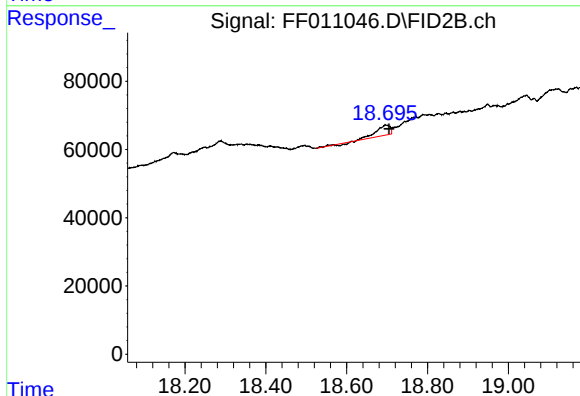

#14 N-DOTRIACONTANE

R.T.: 18.698 min
Delta R.T.: -0.007 min
Response: 69096
Conc: 0.64 ug/ml

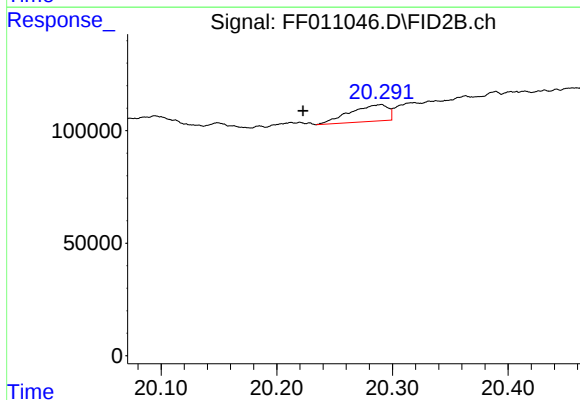

#16 N-HEXATRIACONTANE

R.T.: 20.289 min
Delta R.T.: 0.066 min
Response: 168653
Conc: 1.96 ug/ml