

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071522\
 Data File : FF011051.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jul 2022 19:56
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 15 23:31:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
 Quant Title :
 QLast Update : Fri Jul 01 01:40:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.811	1903928	20.296 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.866	14093	0.134 ug/ml
14) N-DOTRIACONTANE	18.699	249186	2.322 ug/ml
15) N-TETRATRIACONTANE	19.487	191490	1.964 ug/ml
17) N-OCTATRIACONTANE	21.000f	452864	6.040 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071522\
Data File : FF011051.D
Signal(s) : FID2B.ch
Acq On : 15 Jul 2022 19:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 15 23:31:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

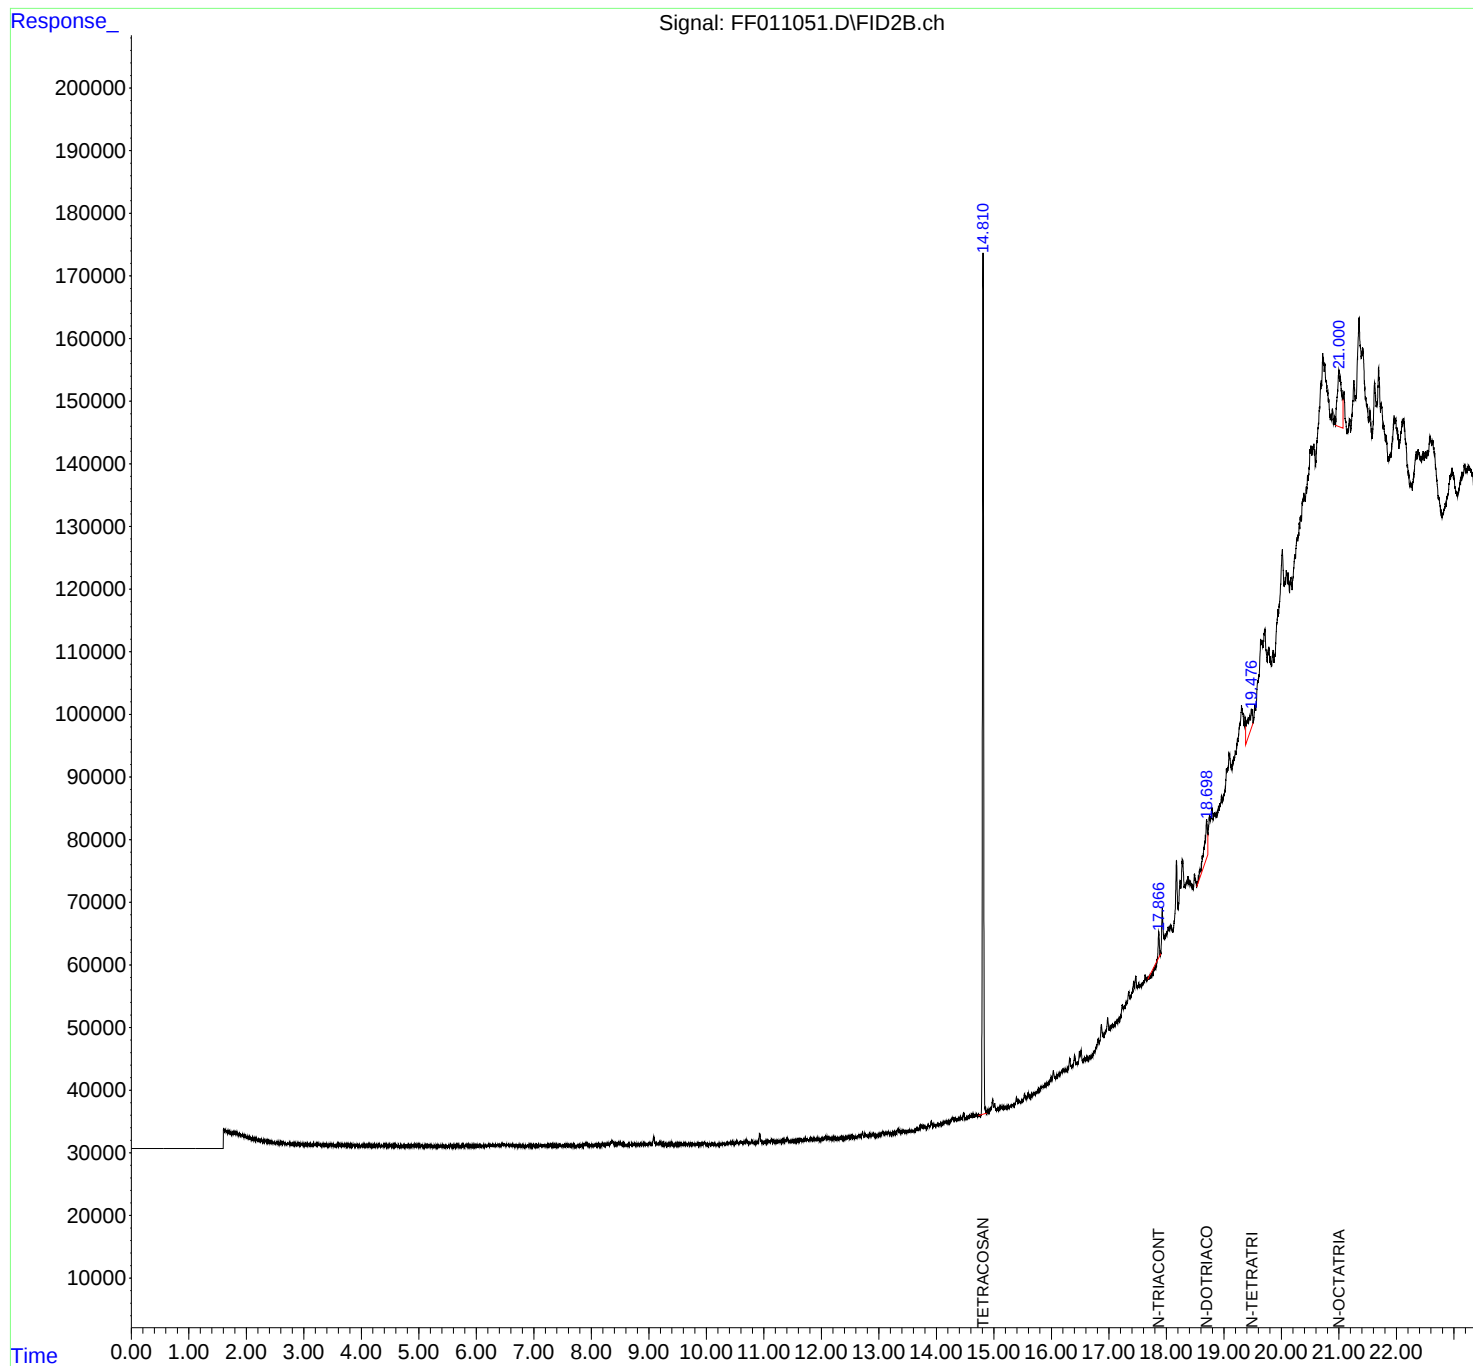

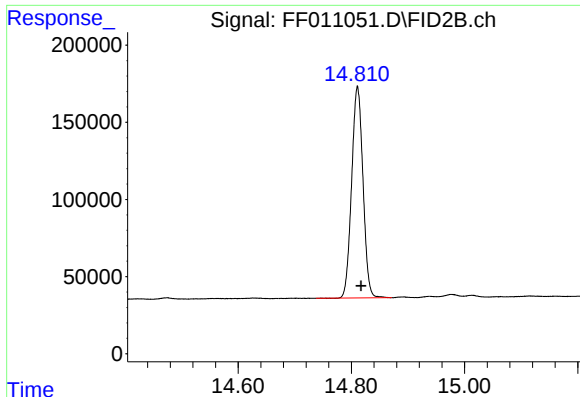


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.811 min
Delta R.T.: -0.006 min
Response: 1903928
Conc: 20.30 ug/ml

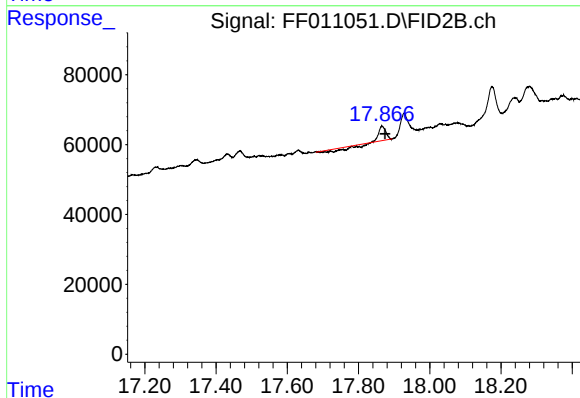


#13 N-TRIACONTANE

R.T.: 17.866 min
Delta R.T.: -0.008 min
Response: 14093
Conc: 0.13 ug/ml

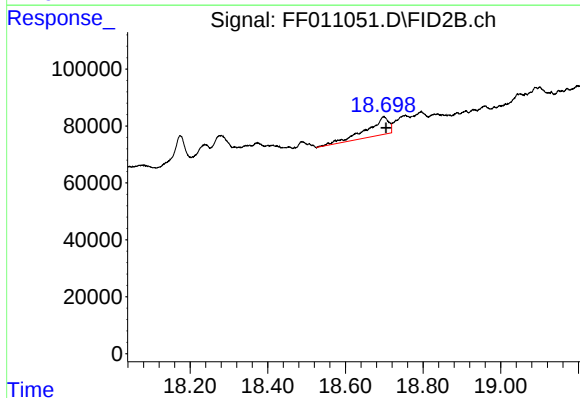


#14 N-DOTRIACONTANE

R.T.: 18.699 min
Delta R.T.: -0.006 min
Response: 249186
Conc: 2.32 ug/ml

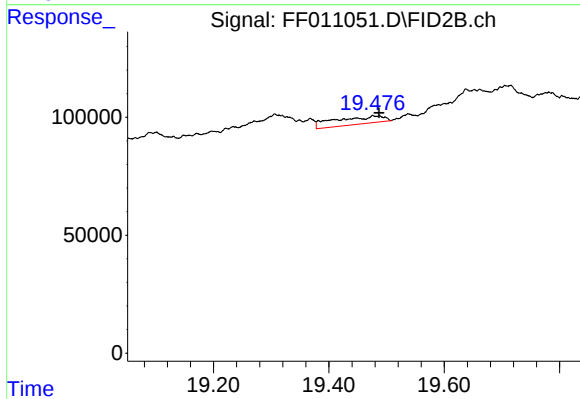

#15 N-TETRATRIACONTANE

R.T.: 19.487 min
Delta R.T.: 0.000 min
Response: 191490
Conc: 1.96 ug/ml

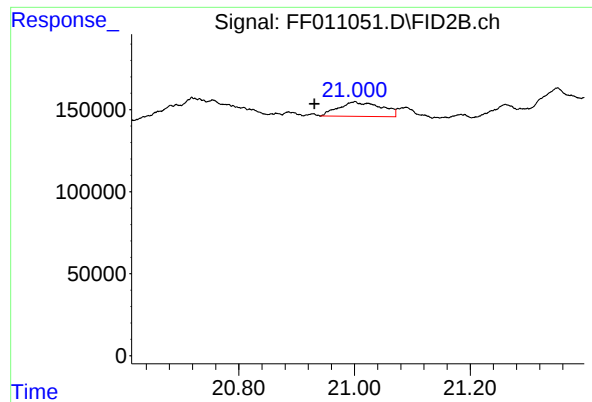

#17 N-OCTATRIACONTANE

R.T.: 21.000 min
Delta R.T.: 0.069 min
Response: 452864
Conc: 6.04 ug/ml