

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071618\
 Data File : FF001373.D
 Signal(s) : FID2B.ch
 Acq On : 16 Jul 2018 16:39
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 17 03:27:27 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	5229526	48.546 ug/ml
Target Compounds			
2) N-DECANE	4.222	6885981	55.462 ug/ml
3) N-DODECANE	6.234	6684661	53.348 ug/ml
4) N-TETRADECANE	8.022	6506517	51.734 ug/ml
5) N-HEXADECANE	9.619	6366458	50.955 ug/ml
6) N-OCTADECANE	11.056	6262816	49.974 ug/ml
7) N-EICOSANE	12.363	6126672	49.253 ug/ml
8) N-DOCOSANE	13.559	6019629	48.817 ug/ml
10) N-TETRACOSANE	14.660	5970836	48.978 ug/ml
11) N-HEXACOSANE	15.680	5909097	48.749 ug/ml
12) N-OCTACOSANE	16.629	5995391	49.766 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071618\
Data File : FF001373.D
Signal(s) : FID2B.ch
Acq On : 16 Jul 2018 16:39
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 17 03:27:27 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

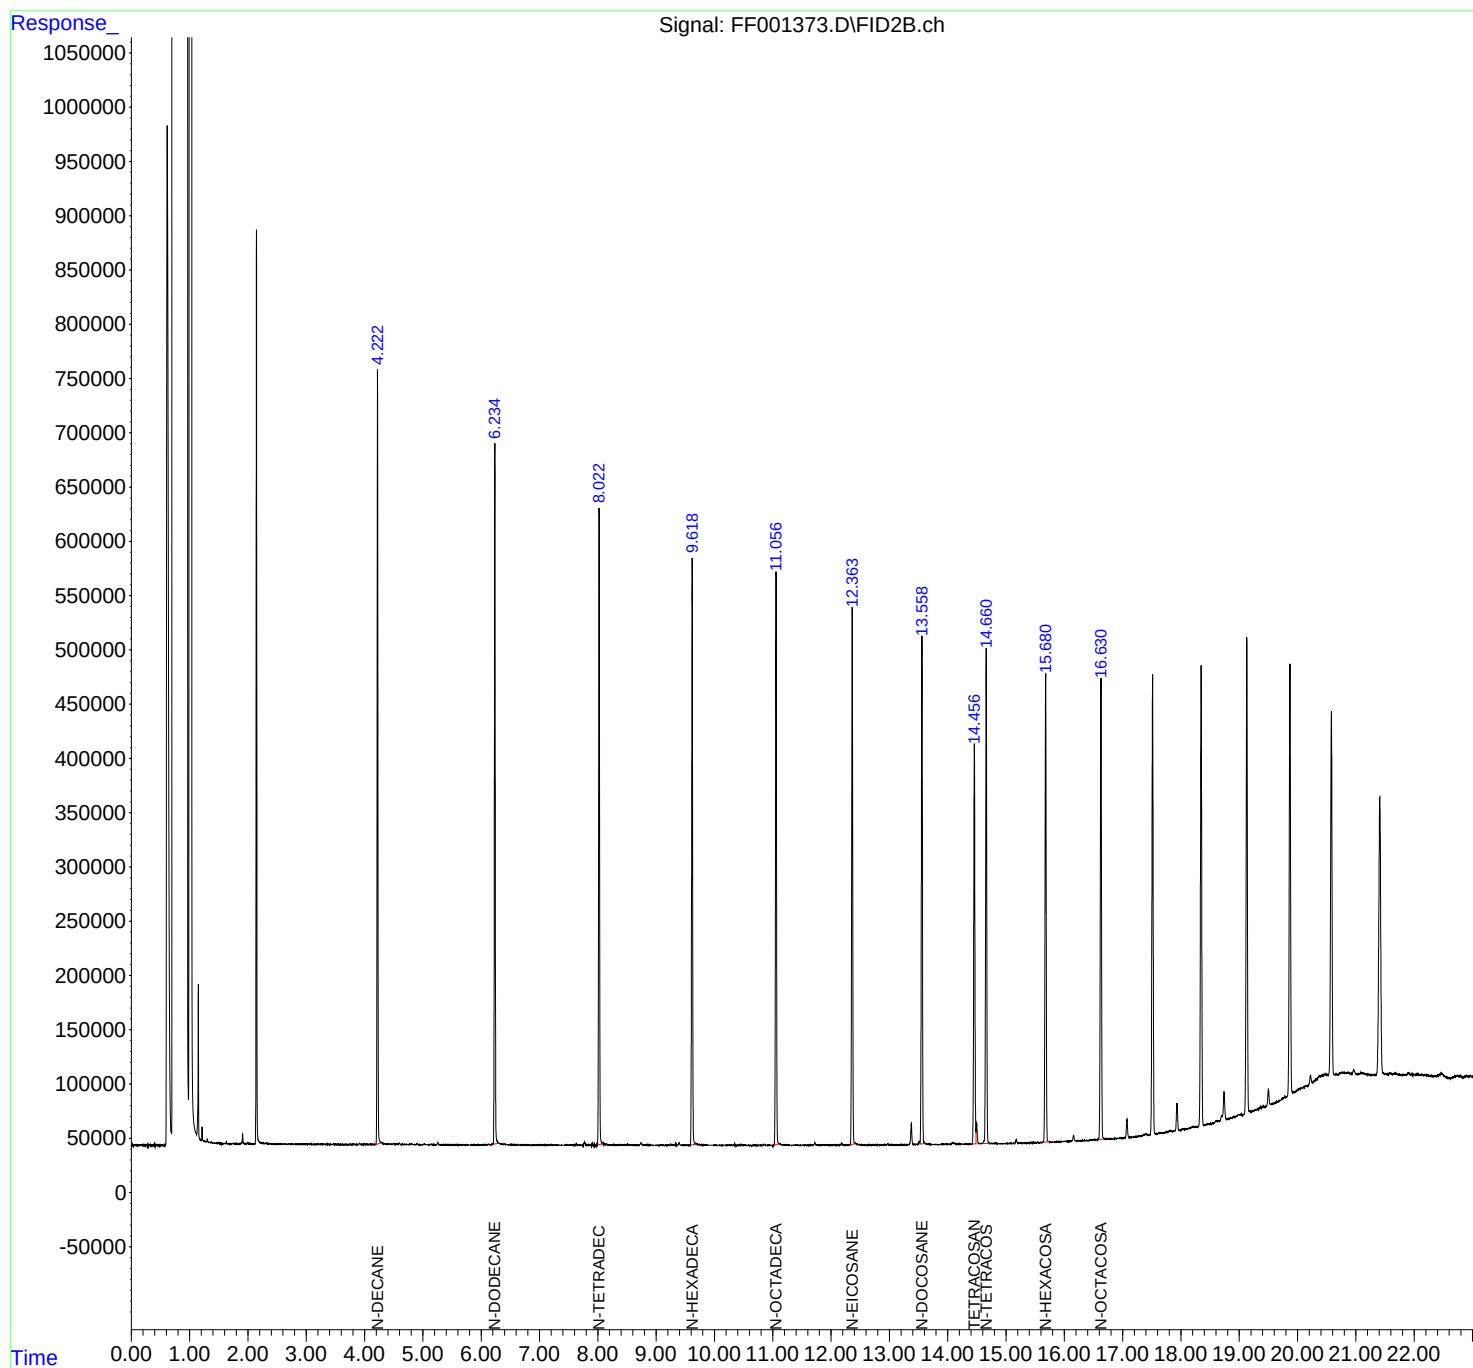

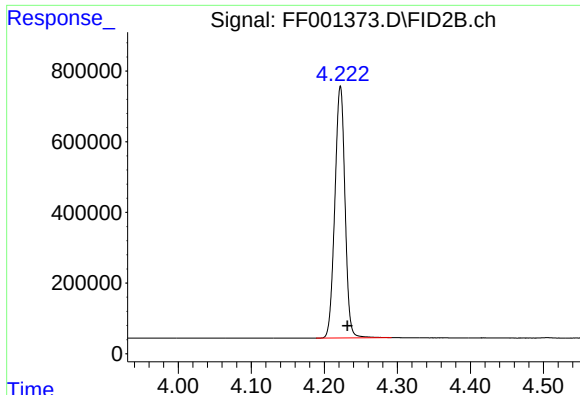


#2 N-DECANE

R.T.: 4.222 min
Delta R.T.: -0.009 min
Response: 6885981
Conc: 55.46 ug/ml

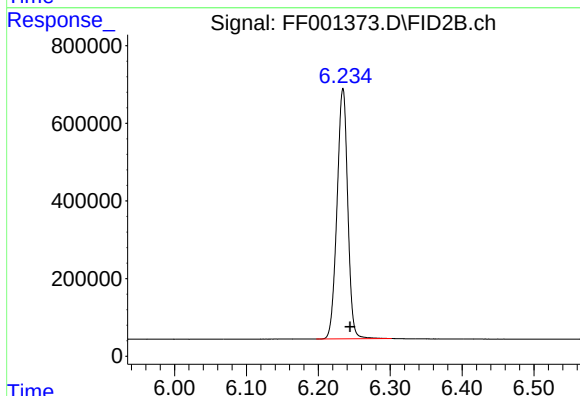


#3 N-DODECANE

R.T.: 6.234 min
Delta R.T.: -0.010 min
Response: 6684661
Conc: 53.35 ug/ml

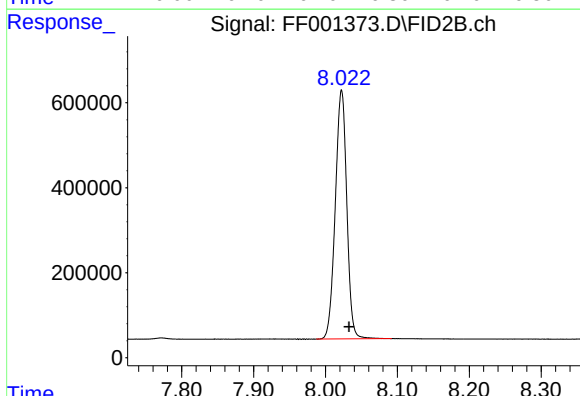


#4 N-TETRADECANE

R.T.: 8.022 min
Delta R.T.: -0.010 min
Response: 6506517
Conc: 51.73 ug/ml

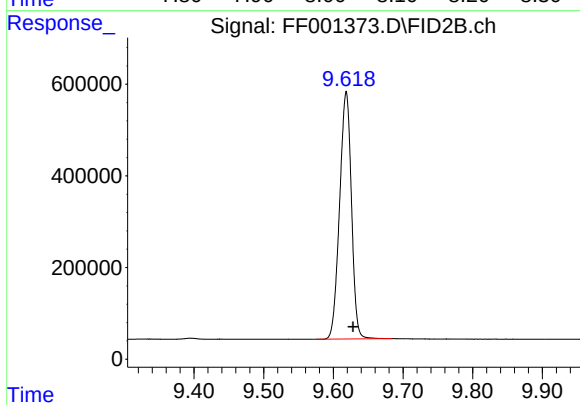


#5 N-HEXADECANE

R.T.: 9.619 min
Delta R.T.: -0.010 min
Response: 6366458
Conc: 50.95 ug/ml

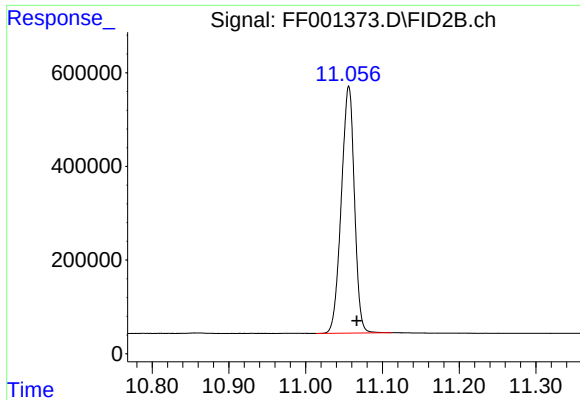


#6 N-OCTADECANE

R.T.: 11.056 min
Delta R.T.: -0.010 min
Response: 6262816
Conc: 49.97 ug/ml

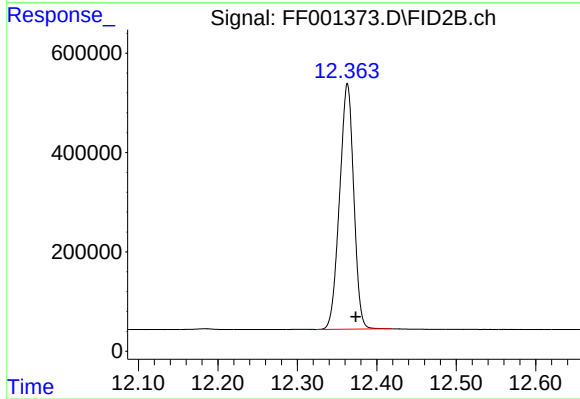


#7 N-EICOSANE

R.T.: 12.363 min
Delta R.T.: -0.010 min
Response: 6126672
Conc: 49.25 ug/ml

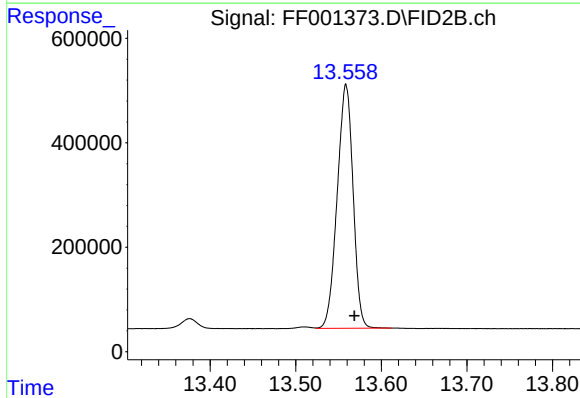


#8 N-DOCOSANE

R.T.: 13.559 min
Delta R.T.: -0.010 min
Response: 6019629
Conc: 48.82 ug/ml

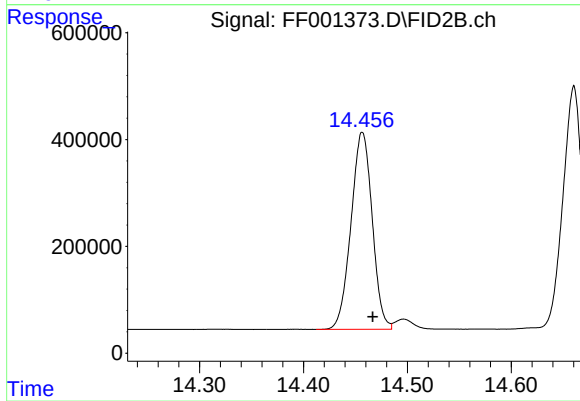


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.457 min
Delta R.T.: -0.010 min
Response: 5229526
Conc: 48.55 ug/ml

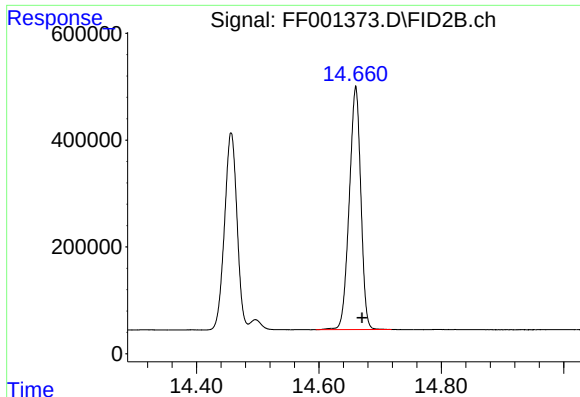


#10 N-TETRACOSANE

R.T.: 14.660 min
Delta R.T.: -0.010 min
Response: 5970836
Conc: 48.98 ug/ml

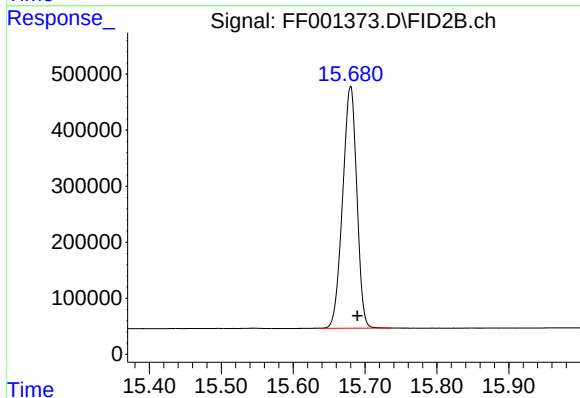

#11 N-HEXACOSANE

R.T.: 15.680 min
Delta R.T.: -0.009 min
Response: 5909097
Conc: 48.75 ug/ml

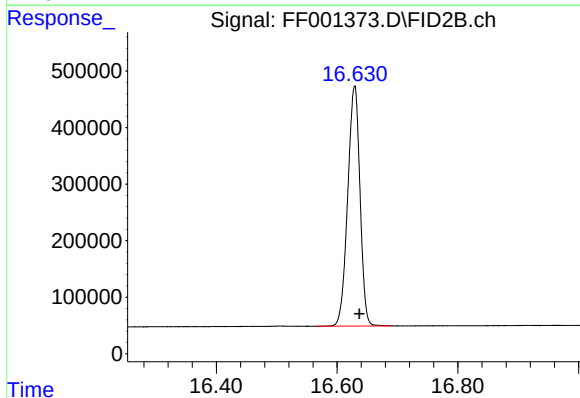

#12 N-OCTACOSANE

R.T.: 16.629 min
Delta R.T.: -0.008 min
Response: 5995391
Conc: 49.77 ug/ml