

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071619\
 Data File : FF005074.D
 Signal(s) : FID2B.ch
 Acq On : 16 Jul 2019 15:29
 Operator : DD\AJ
 Sample : K3622-07 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 17 00:34:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.677	104938	1.079 ug/ml
Target Compounds				
6)	N-OCTADECANE	11.256	71350	0.602 ug/ml
7)	N-EICOSANE	12.570	125957	1.086 ug/ml
8)	N-DOCOSANE	13.775	36051	0.320 ug/ml
10)	N-TETRACOSANE	14.862	278109	2.498 ug/ml
12)	N-OCTACOSANE	16.866	127662	1.145 ug/ml
13)	N-TRIACONTANE	17.755	242047	2.155 ug/ml
14)	N-DOTRIACONTANE	18.599	160603	1.410 ug/ml
15)	N-TETRATRIACONTANE	19.384	75582	0.696 ug/ml
16)	N-HEXATRIACONTANE	20.140	285127	2.753 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071619\
Data File : FF005074.D
Signal(s) : FID2B.ch
Acq On : 16 Jul 2019 15:29
Operator : DD\AJ
Sample : K3622-07 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 17 00:34:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

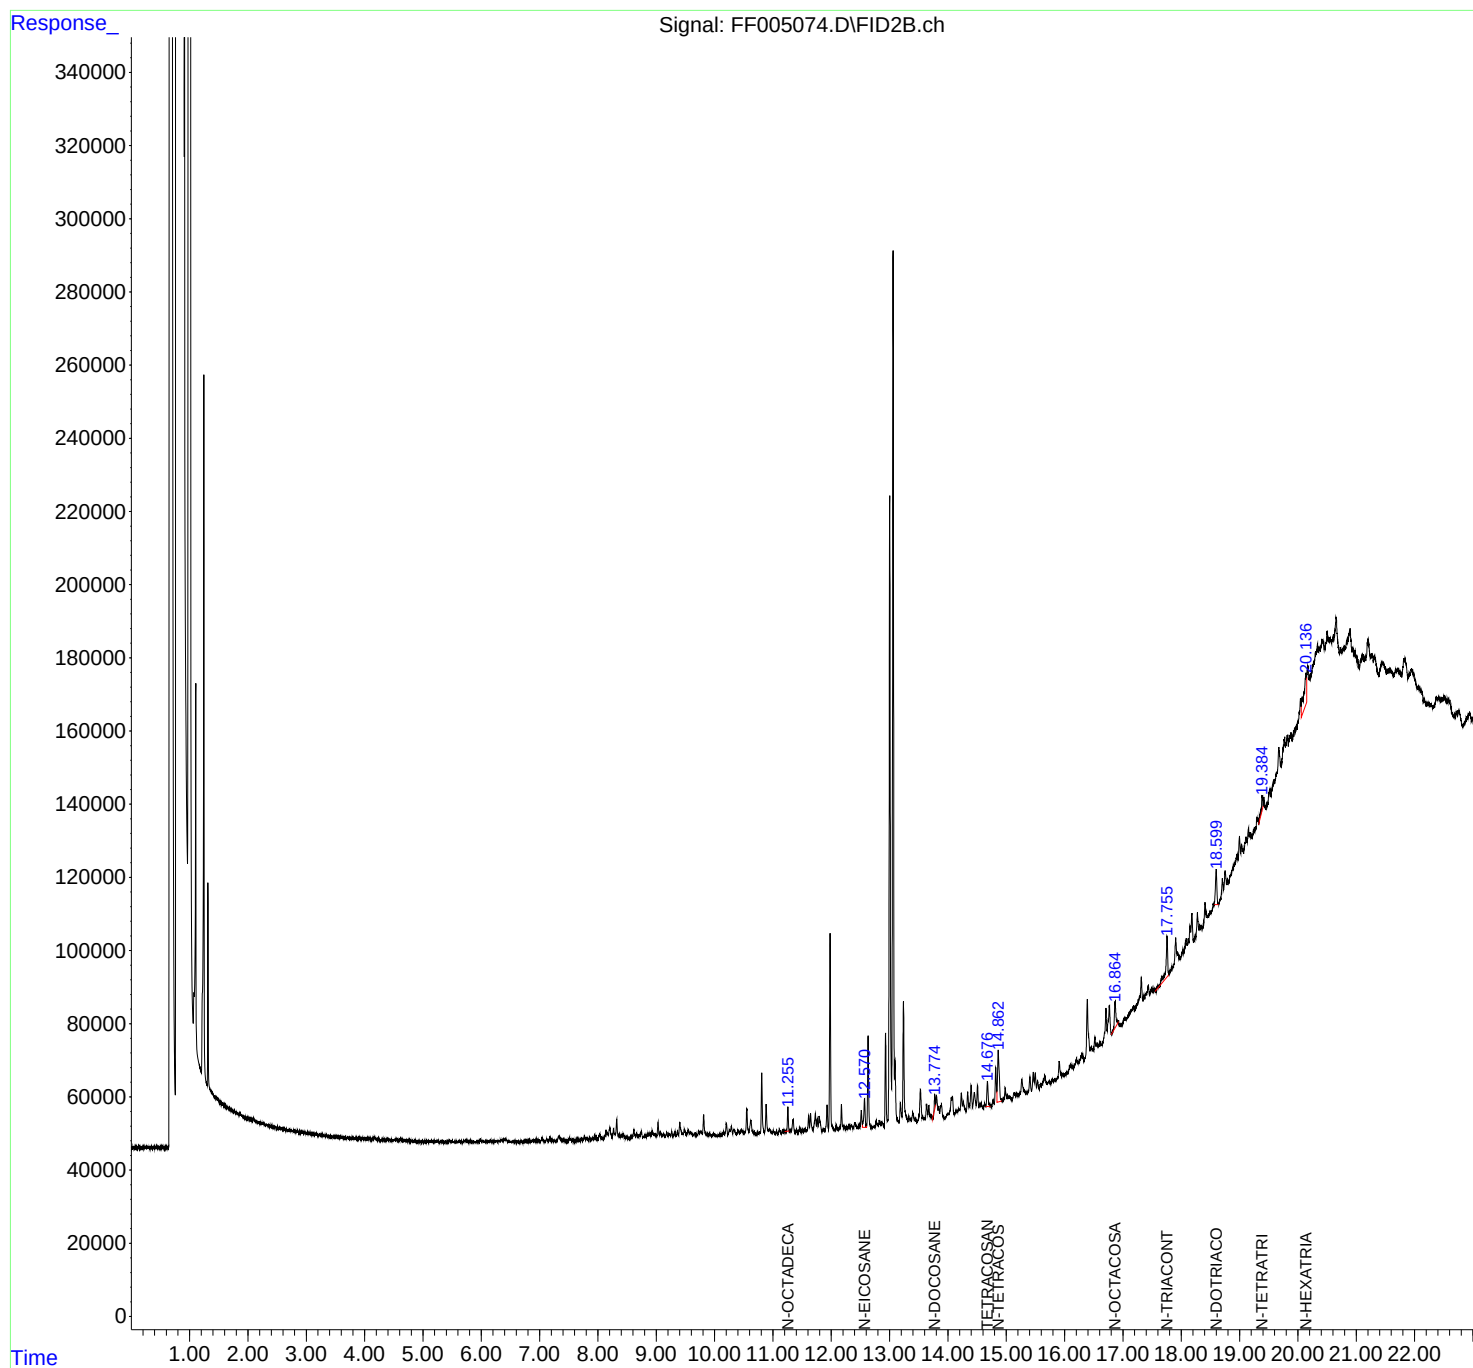

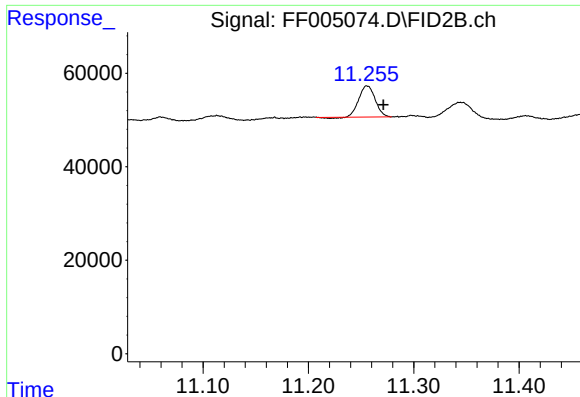


#6 N-OCTADECANE

R.T.: 11.256 min
Delta R.T.: -0.015 min
Response: 71350
Conc: 0.60 ug/ml

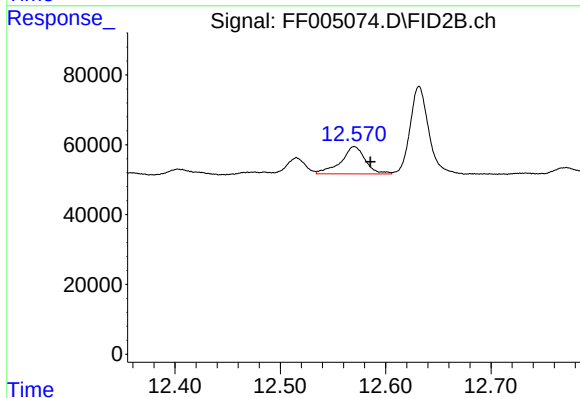


#7 N-EICOSANE

R.T.: 12.570 min
Delta R.T.: -0.015 min
Response: 125957
Conc: 1.09 ug/ml

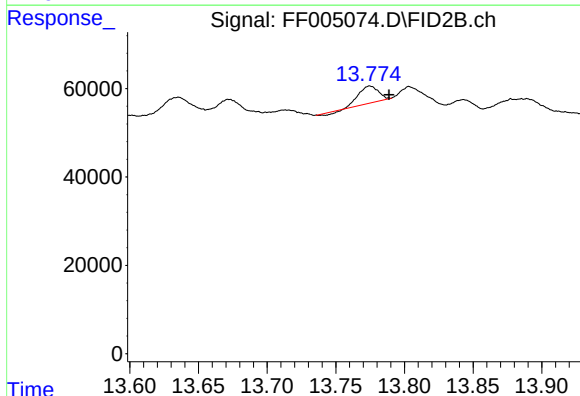


#8 N-DOCOSANE

R.T.: 13.775 min
Delta R.T.: -0.014 min
Response: 36051
Conc: 0.32 ug/ml

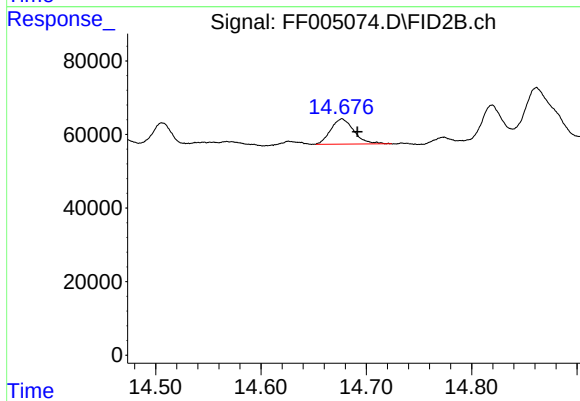


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.677 min
Delta R.T.: -0.015 min
Response: 104938
Conc: 1.08 ug/ml

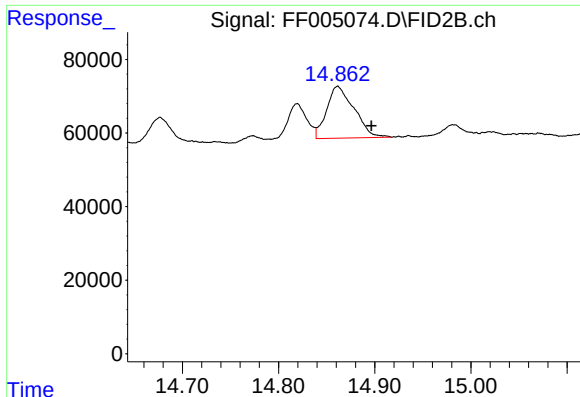


#10 N-TETRACOSANE

R.T.: 14.862 min
Delta R.T.: -0.035 min
Response: 278109
Conc: 2.50 ug/ml

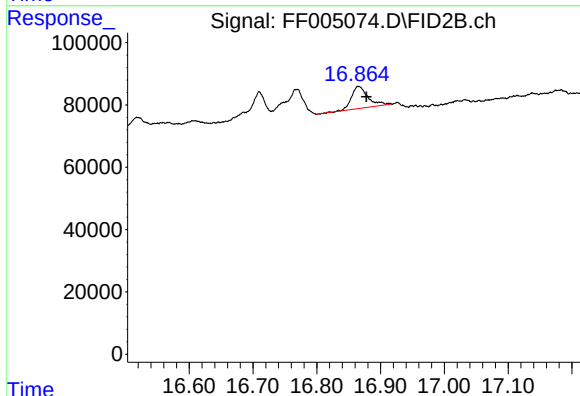


#12 N-OCTACOSANE

R.T.: 16.866 min
Delta R.T.: -0.012 min
Response: 127662
Conc: 1.14 ug/ml

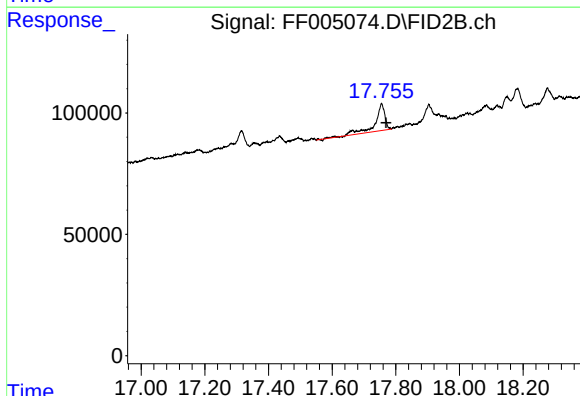


#13 N-TRIACONTANE

R.T.: 17.755 min
Delta R.T.: -0.014 min
Response: 242047
Conc: 2.15 ug/ml

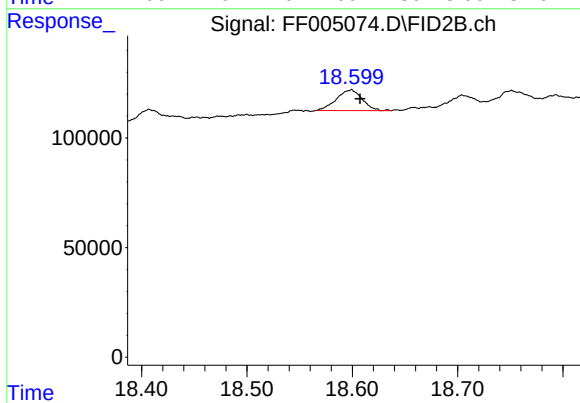

#14 N-DOTRIACONTANE

R.T.: 18.599 min
Delta R.T.: -0.008 min
Response: 160603
Conc: 1.41 ug/ml

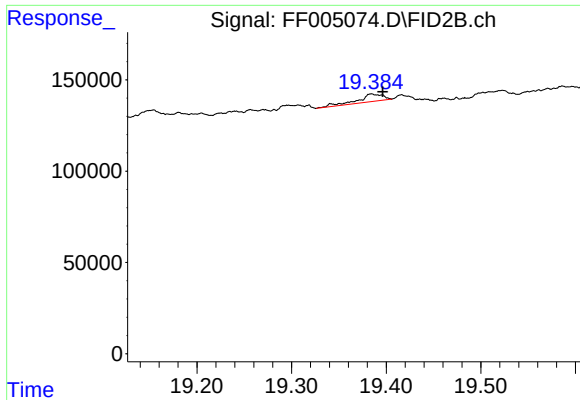


#15 N-TETRATRIACONTANE

R.T.: 19.384 min

Delta R.T.: -0.012 min

Response: 75582

Conc: 0.70 ug/ml

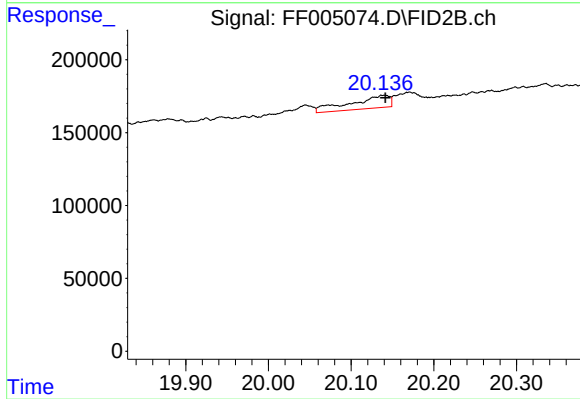

#16 N-HEXATRIACONTANE

R.T.: 20.140 min

Delta R.T.: -0.001 min

Response: 285127

Conc: 2.75 ug/ml