

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071621\
 Data File : FF008812.D
 Signal(s) : FID2B.ch
 Acq On : 16 Jul 2021 12:11
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 16 23:17:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.519	3740846	27.505 ug/ml
12) N-OCTACOSANE	16.918	3188314	25.777 ug/ml
13) N-TRIACONTANE	17.802	325910	2.719 ug/ml
14) N-DOTRIACONTANE	18.631	462209	3.945 ug/ml
15) N-TETRATRIACONTANE	19.412	380691	3.641 ug/ml
16) N-HEXATRIACONTANE	20.150	287884	3.065 ug/ml
17) N-OCTATRIACONTANE	20.891	190336	2.309 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071621\
Data File : FF008812.D
Signal(s) : FID2B.ch
Acq On : 16 Jul 2021 12:11
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 23:17:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

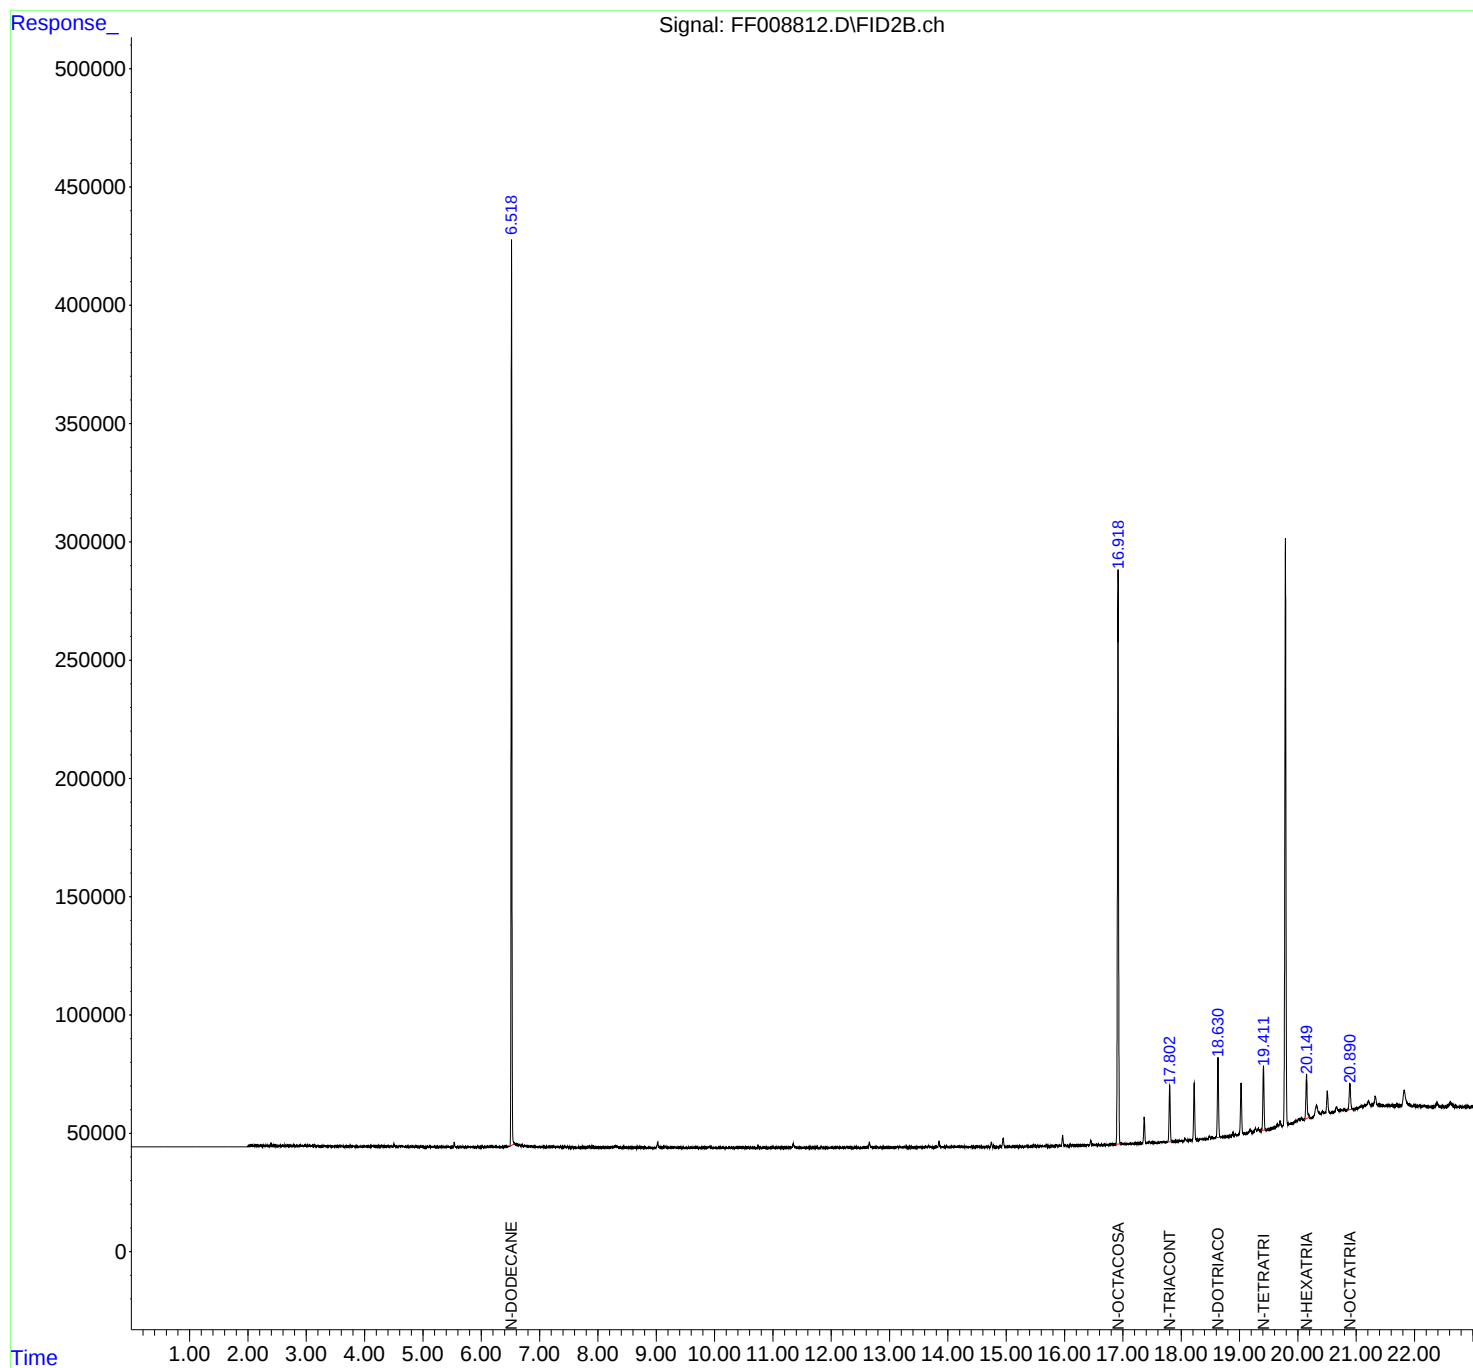


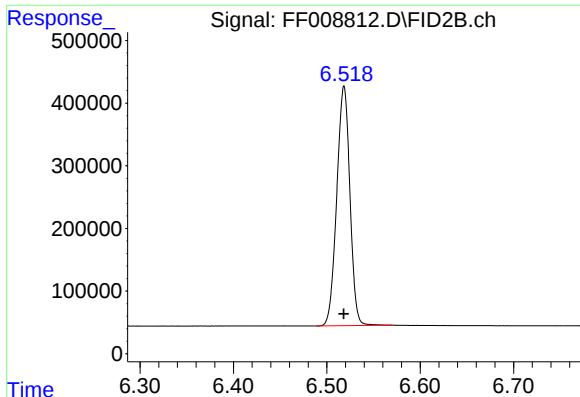

#3 N-DODECANE


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 3740846
Conc: 27.51 ug/ml

Instrument :
FID_F
ClientSampleId :

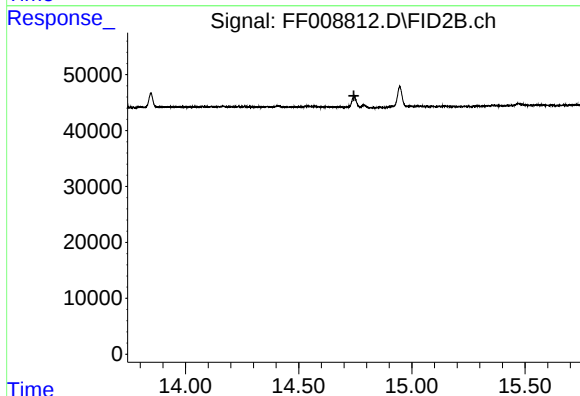


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.744 min
Response: 0
Conc: N.D.

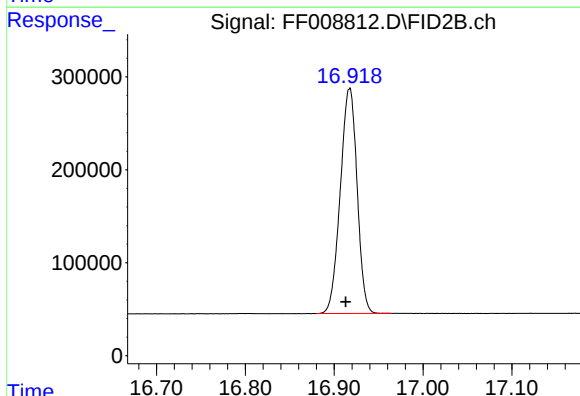


#12 N-OCTACOSANE

R.T.: 16.918 min
Delta R.T.: 0.005 min
Response: 3188314
Conc: 25.78 ug/ml

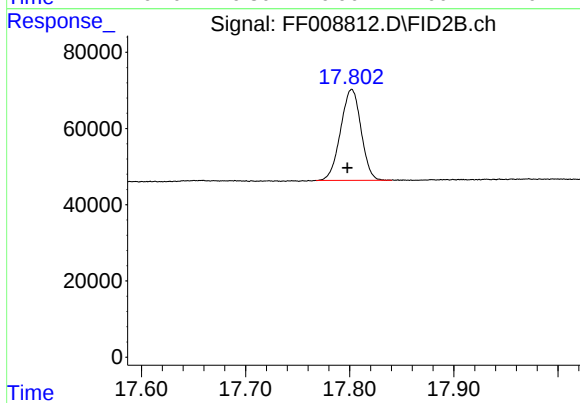

#13 N-TRIACONTANE


R.T.: 17.802 min
Delta R.T.: 0.004 min
Response: 325910
Conc: 2.72 ug/ml

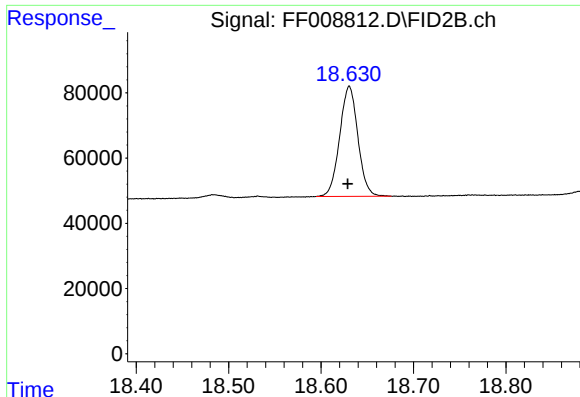

#14 N-DOTRIACONTANE


R.T.: 18.631 min
Delta R.T.: 0.002 min
Response: 462209
Conc: 3.95 ug/ml

Instrument :
FID_F
ClientSampleId :

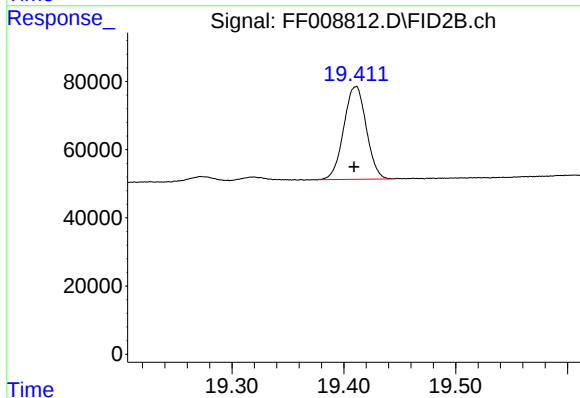


#15 N-TETRATRIACONTANE

R.T.: 19.412 min
Delta R.T.: 0.003 min
Response: 380691
Conc: 3.64 ug/ml

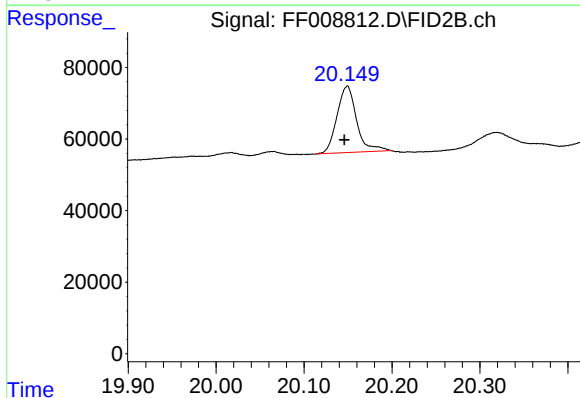

#16 N-HEXATRIACONTANE

R.T.: 20.150 min
Delta R.T.: 0.004 min
Response: 287884
Conc: 3.06 ug/ml

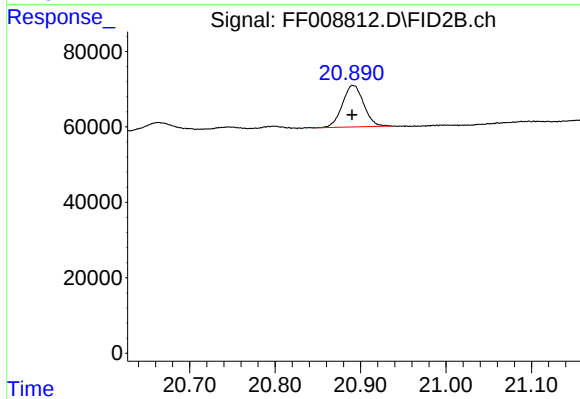

#17 N-OCTATRIACONTANE

R.T.: 20.891 min
Delta R.T.: 0.000 min
Response: 190336
Conc: 2.31 ug/ml