

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071621\
 Data File : FF008821.D
 Signal(s) : FID2B.ch
 Acq On : 16 Jul 2021 16:56
 Operator : DD\AJ
 Sample : PB137706BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 16 23:19:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	2102441	18.448 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.630	149480	1.276 ug/ml
15) N-TETRATRIACONTANE	19.410	95514	0.914 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071621\
Data File : FF008821.D
Signal(s) : FID2B.ch
Acq On : 16 Jul 2021 16:56
Operator : DD\AJ
Sample : PB137706BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 16 23:19:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

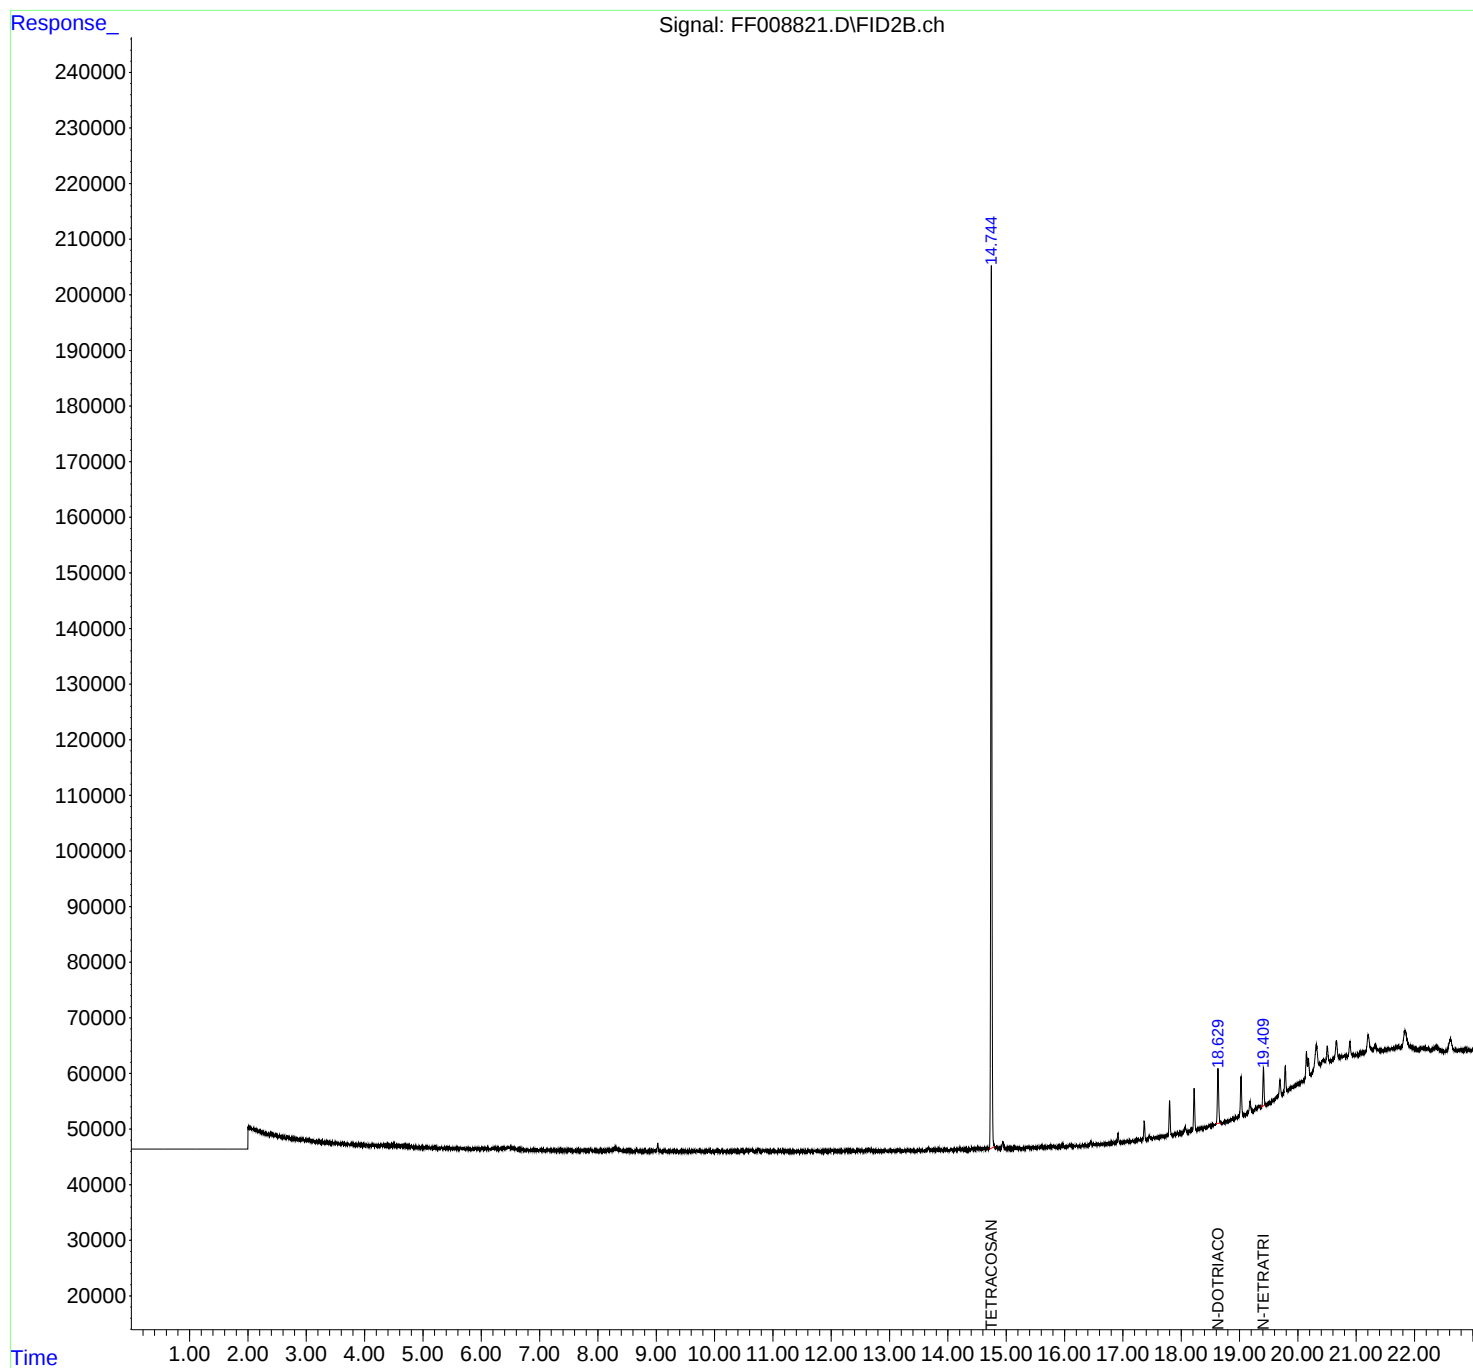


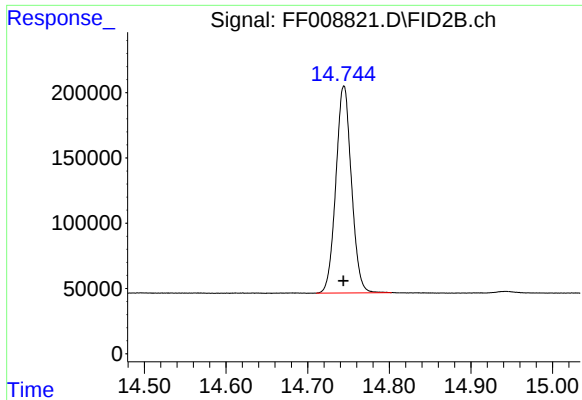

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.745 min
Delta R.T.: 0.000 min
Response: 2102441
Conc: 18.45 ug/ml

Instrument :
FID_F
ClientSampleId :

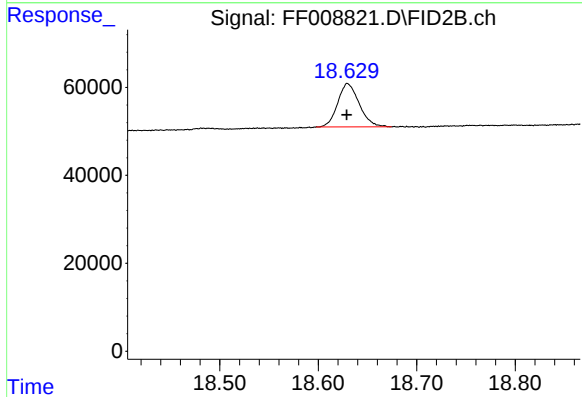

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: 0.000 min
Response: 149480
Conc: 1.28 ug/ml

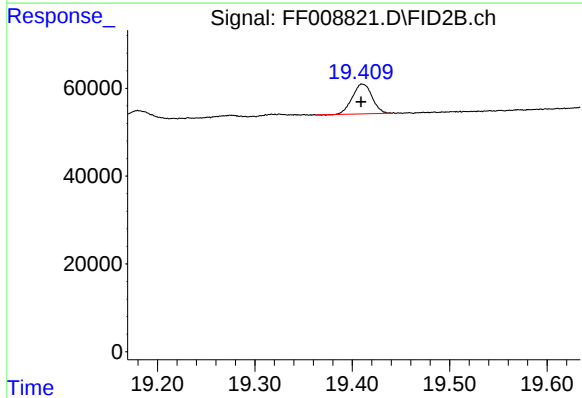

#15 N-TETRATRIACONTANE

R.T.: 19.410 min
Delta R.T.: 0.000 min
Response: 95514
Conc: 0.91 ug/ml