

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071621\
 Data File : FF008833.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jul 2021 02:28
 Operator : DD\AJ
 Sample : PB137737BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 17 03:42:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.744	2550843	22.382 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.916	117697	0.952 ug/ml
13) N-TRIACONTANE	17.800	276064	2.304 ug/ml
14) N-DOTRIACONTANE	18.630	384662	3.283 ug/ml
15) N-TETRATRIACONTANE	19.412	278125	2.660 ug/ml
16) N-HEXATRIACONTANE	20.147	159404	1.697 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071621\
Data File : FF008833.D
Signal(s) : FID2B.ch
Acq On : 17 Jul 2021 02:28
Operator : DD\AJ
Sample : PB137737BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 17 03:42:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

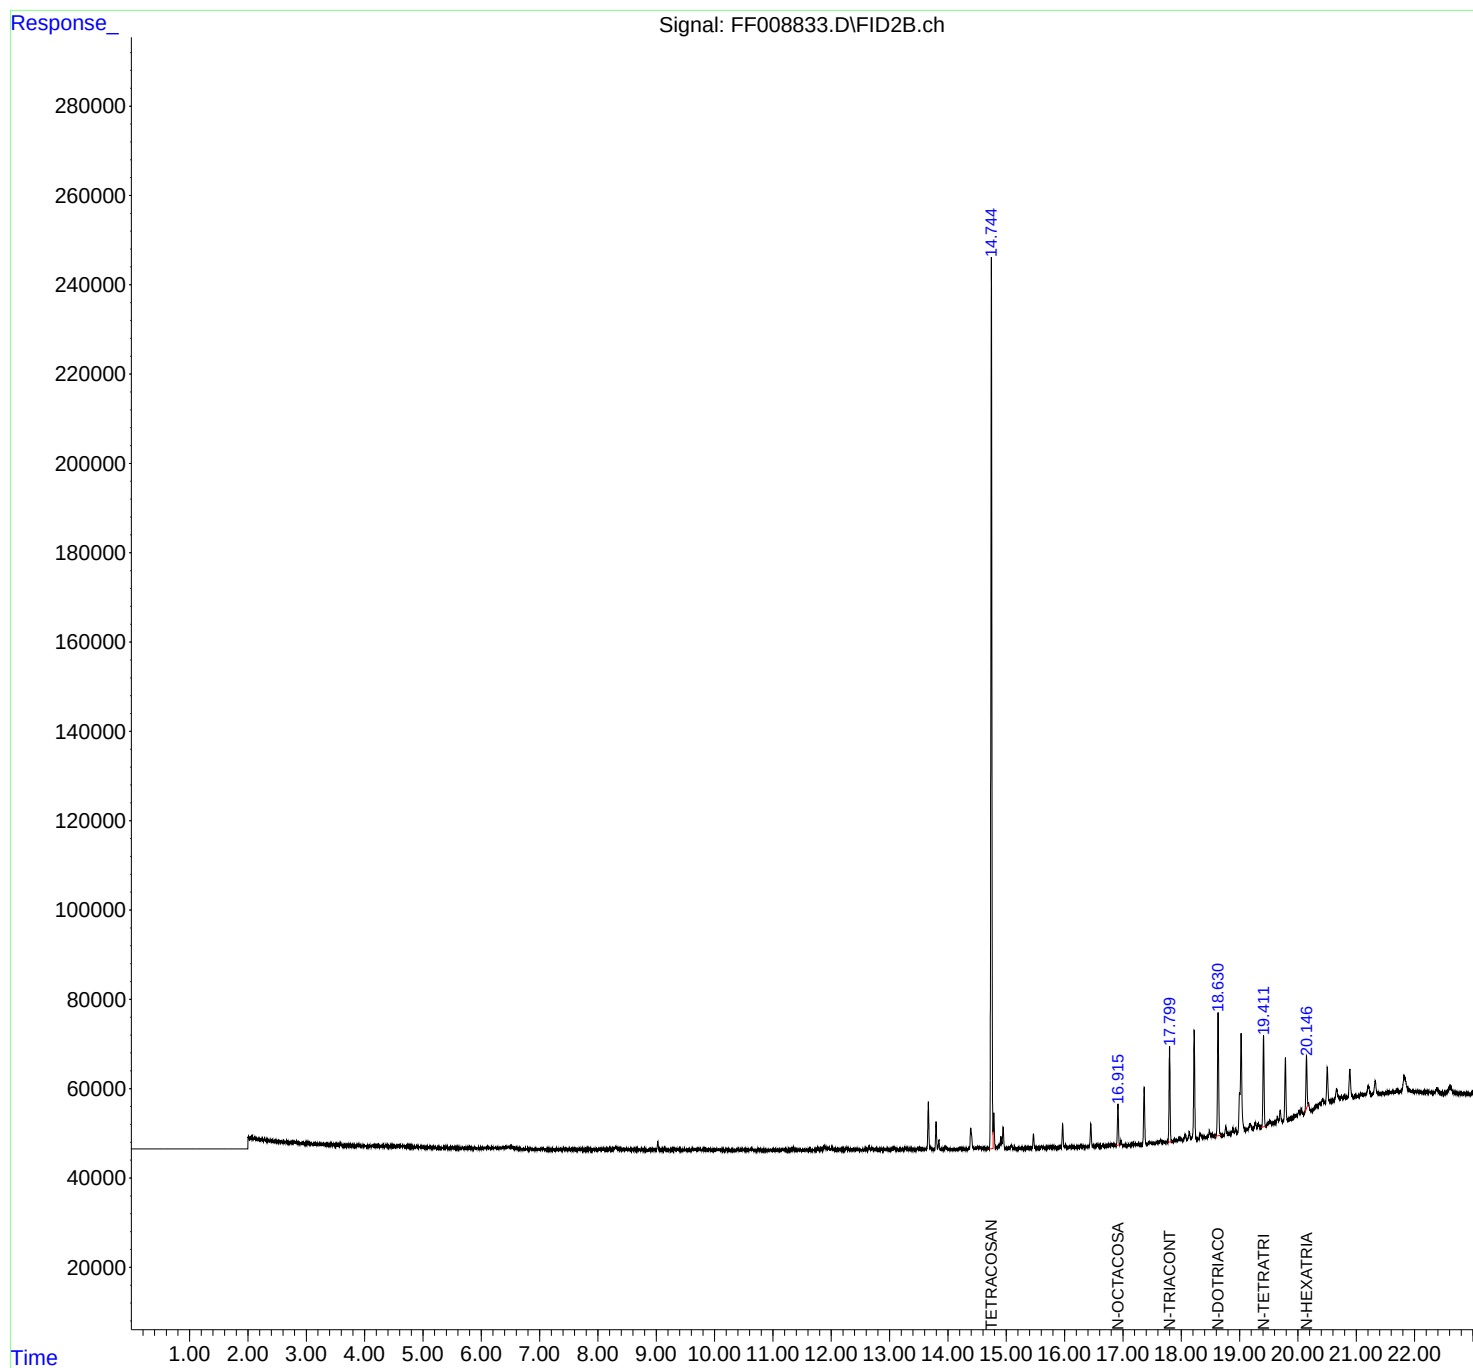


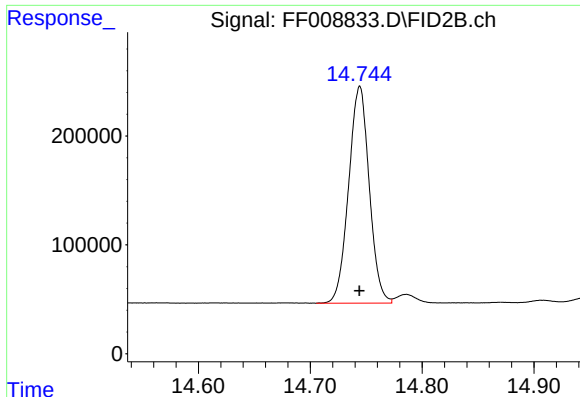

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.744 min
Delta R.T.: 0.000 min
Response: 2550843
Conc: 22.38 ug/ml

Instrument :
FID_F
ClientSampleId :

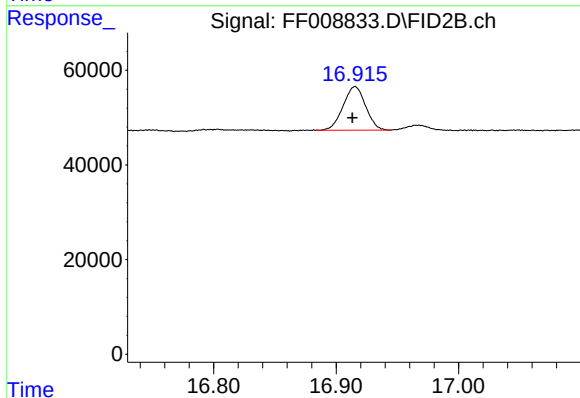


#12 N-OCTACOSANE

R.T.: 16.916 min
Delta R.T.: 0.002 min
Response: 117697
Conc: 0.95 ug/ml

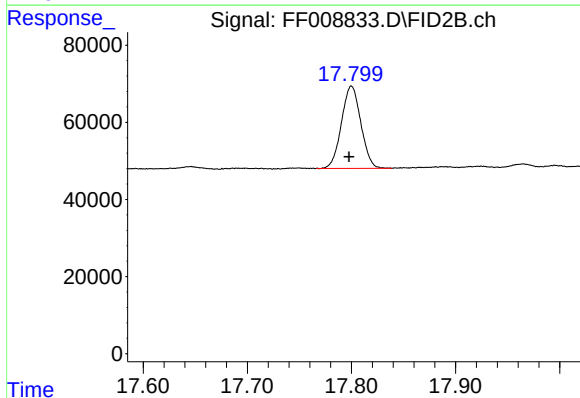


#13 N-TRIACONTANE

R.T.: 17.800 min
Delta R.T.: 0.002 min
Response: 276064
Conc: 2.30 ug/ml

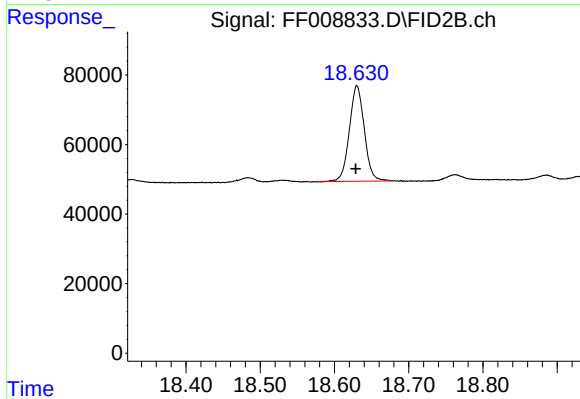

#14 N-DOTRIACONTANE


R.T.: 18.630 min
Delta R.T.: 0.001 min
Response: 384662
Conc: 3.28 ug/ml

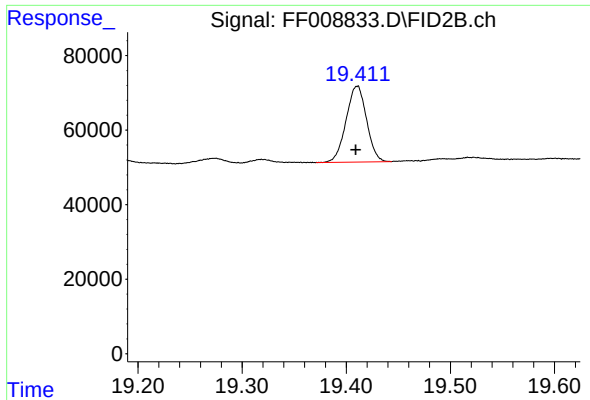

#15 N-TETRATRIACONTANE

R.T.: 19.412 min
Delta R.T.: 0.003 min
Response: 278125
Conc: 2.66 ug/ml

Instrument :
FID_F
ClientSampleId :

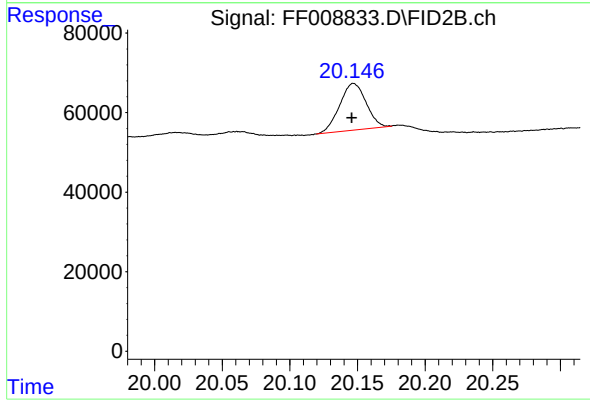

#16 N-HEXATRIACONTANE

R.T.: 20.147 min
Delta R.T.: 0.002 min
Response: 159404
Conc: 1.70 ug/ml