

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071621\
 Data File : FF008836.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jul 2021 04:02
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: Sample.e
 Quant Time: Jul 17 06:18:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	5063914	44.432 ug/ml
Target Compounds			
2) N-DECANE	4.505	7251162	53.781 ug/ml
3) N-DODECANE	6.521	7118947	52.344 ug/ml
4) N-TETRADECANE	8.312	6934984	51.402 ug/ml
5) N-HEXADECANE	9.908	6638470	48.595 ug/ml
6) N-OCTADECANE	11.346	6525654	46.888 ug/ml
7) N-EICOSANE	12.653	6243683	45.537 ug/ml
8) N-DOCOSANE	13.847	5971900	44.634 ug/ml
10) N-TETRACOSANE	14.950	5837869	44.304 ug/ml
11) N-HEXACOSANE	15.970	5693785	44.560 ug/ml
12) N-OCTACOSANE	16.918	5674517	45.878 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071621\
Data File : FF008836.D
Signal(s) : FID2B.ch
Acq On : 17 Jul 2021 04:02
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: Sample.e
Quant Time: Jul 17 06:18:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

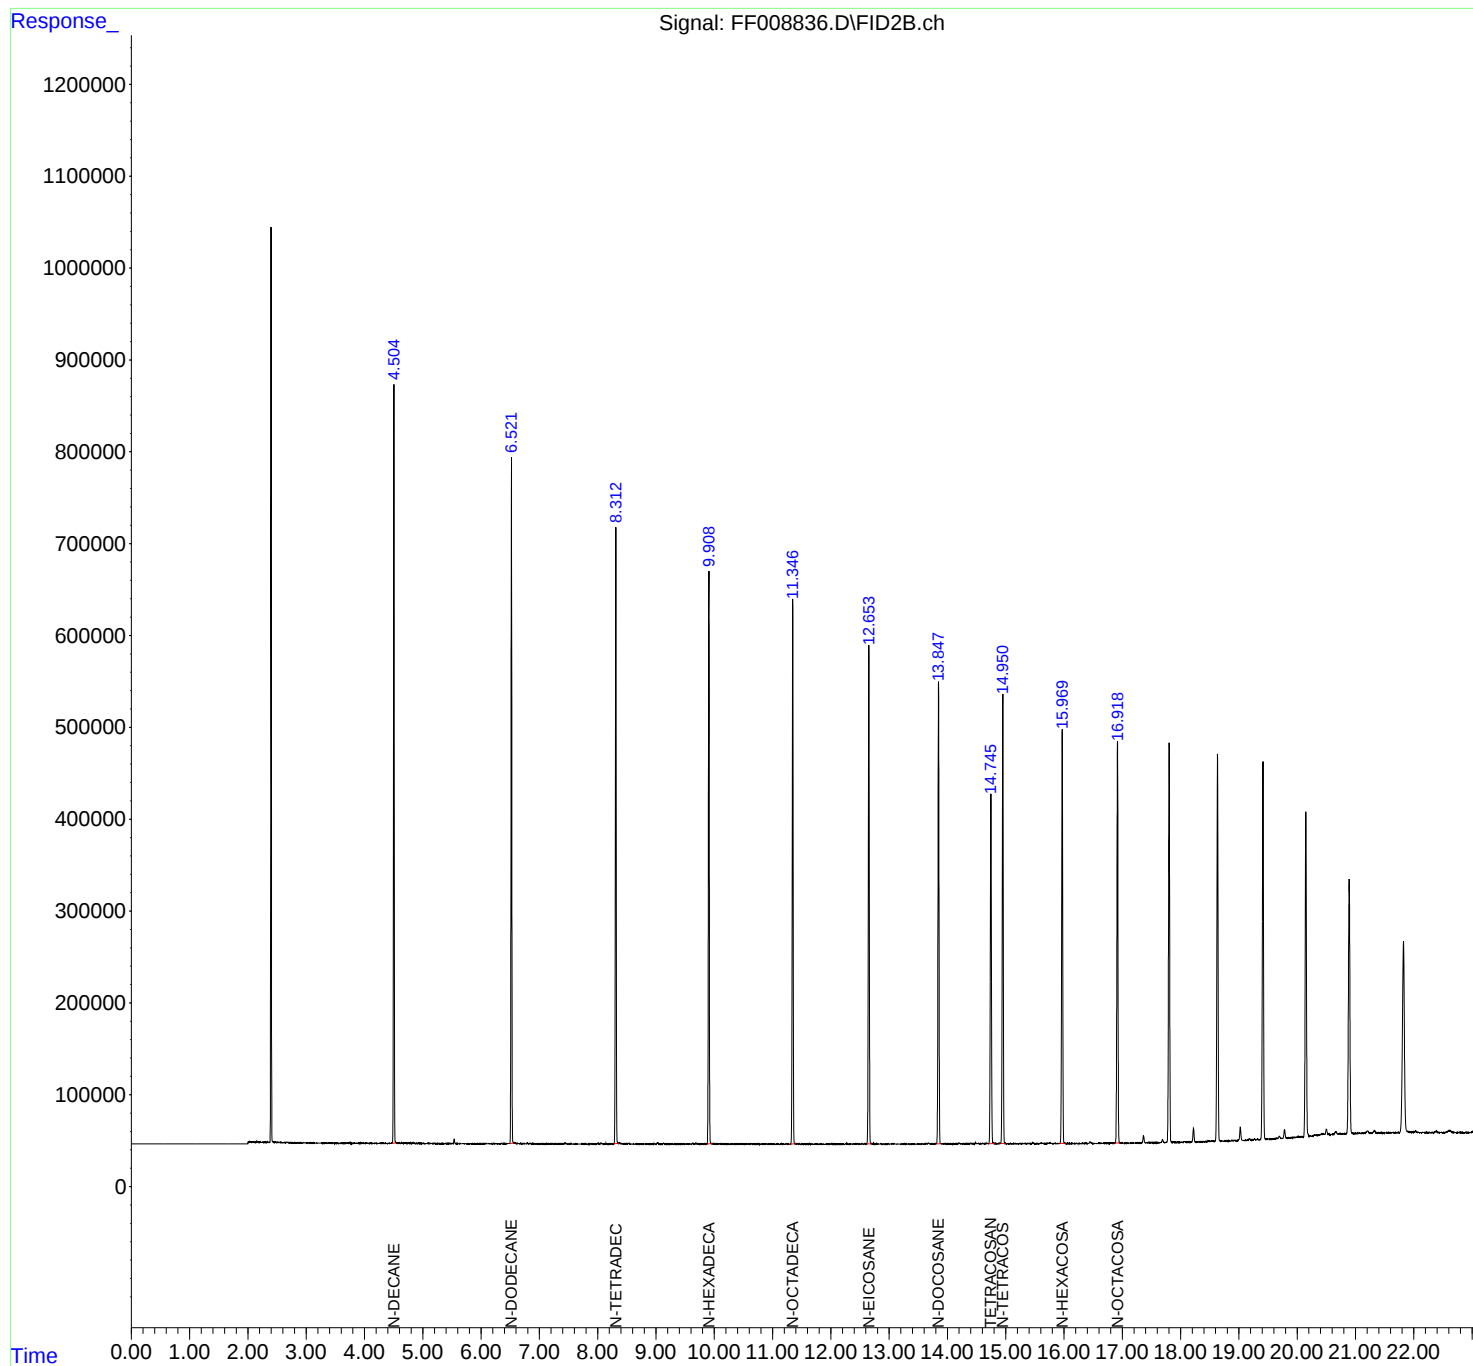


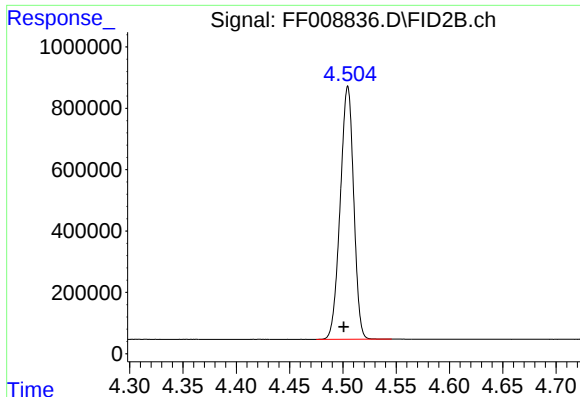

#2 N-DECANE


R.T.: 4.505 min
Delta R.T.: 0.004 min
Response: 7251162
Conc: 53.78 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

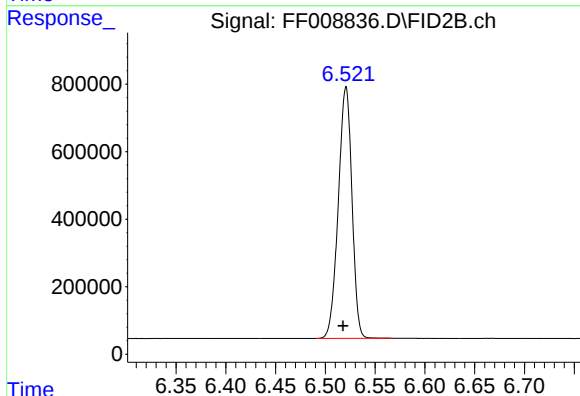


#3 N-DODECANE

R.T.: 6.521 min
Delta R.T.: 0.003 min
Response: 7118947
Conc: 52.34 ug/ml

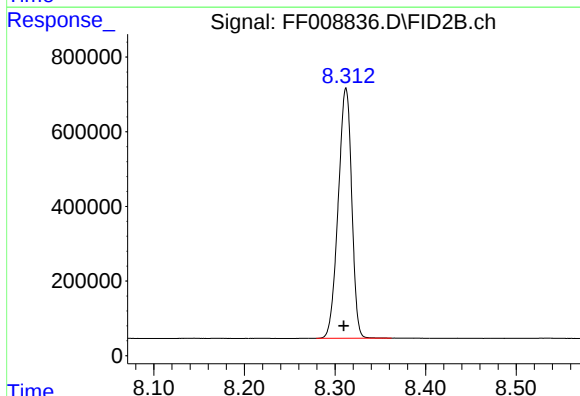


#4 N-TETRADECANE

R.T.: 8.312 min
Delta R.T.: 0.003 min
Response: 6934984
Conc: 51.40 ug/ml

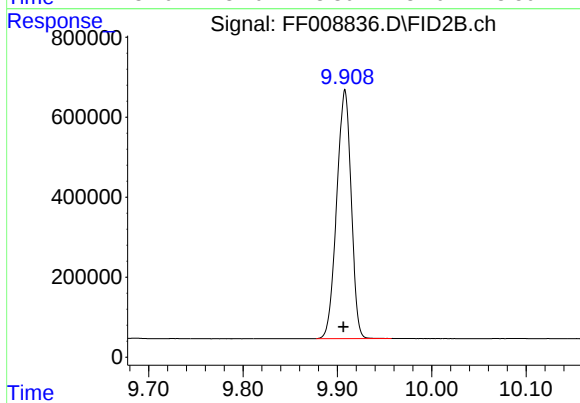

#5 N-HEXADECANE


R.T.: 9.908 min
Delta R.T.: 0.002 min
Response: 6638470
Conc: 48.59 ug/ml

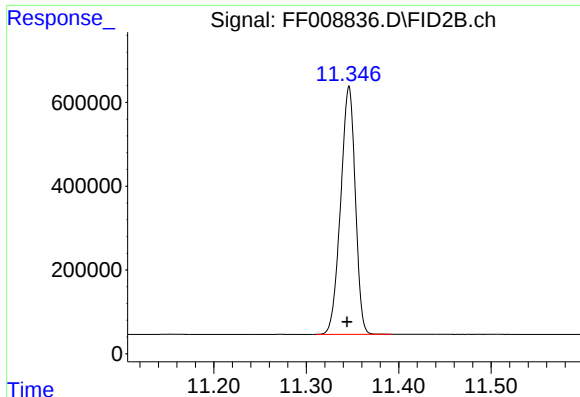

#6 N-OCTADECANE


R.T.: 11.346 min
Delta R.T.: 0.002 min
Response: 6525654
Conc: 46.89 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

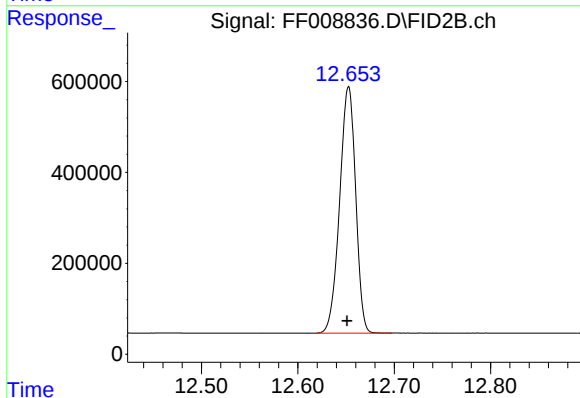


#7 N-EICOSANE

R.T.: 12.653 min
Delta R.T.: 0.002 min
Response: 6243683
Conc: 45.54 ug/ml

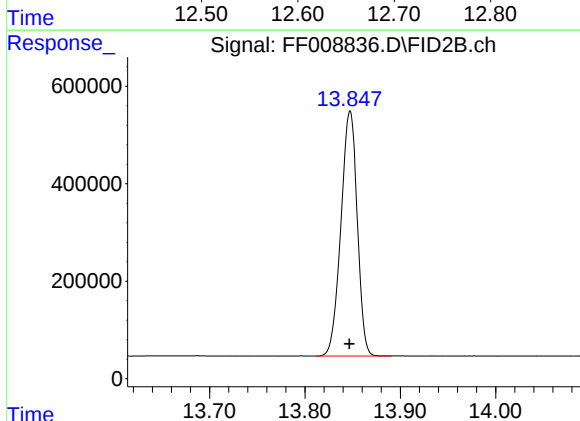


#8 N-DOCOSANE

R.T.: 13.847 min
Delta R.T.: 0.000 min
Response: 5971900
Conc: 44.63 ug/ml

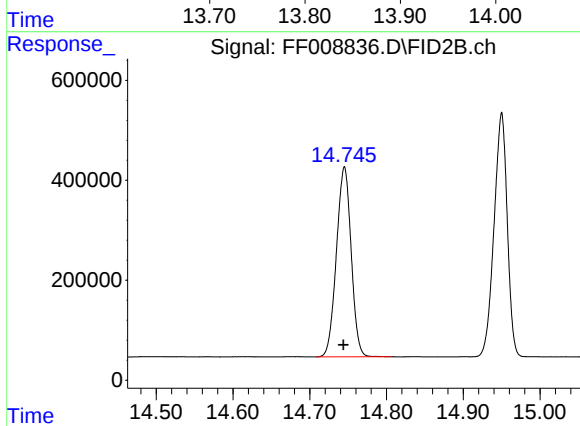

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.745 min
Delta R.T.: 0.001 min
Response: 5063914
Conc: 44.43 ug/ml

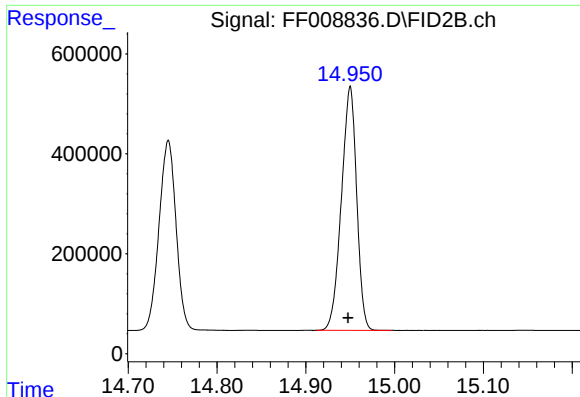

#10 N-TETRACOSANE


R.T.: 14.950 min
Delta R.T.: 0.003 min
Response: 5837869
Conc: 44.30 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

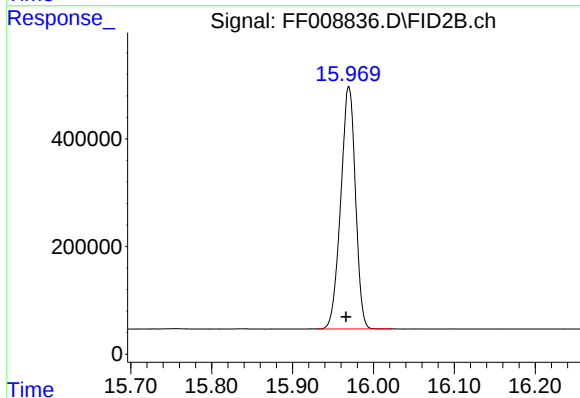

#11 N-HEXACOSANE

R.T.: 15.970 min
Delta R.T.: 0.003 min
Response: 5693785
Conc: 44.56 ug/ml

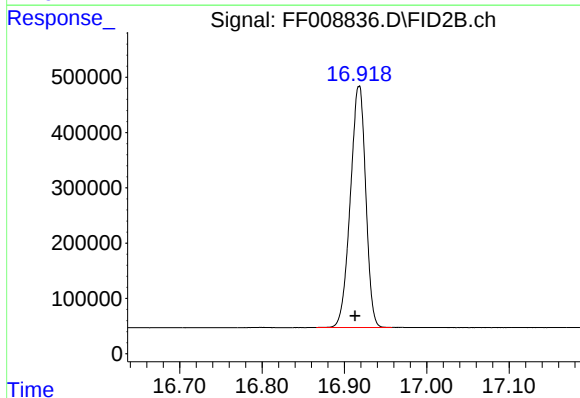

#12 N-OCTACOSANE

R.T.: 16.918 min
Delta R.T.: 0.005 min
Response: 5674517
Conc: 45.88 ug/ml