

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071818\
Data File : FF001407.D
Signal(s) : FID2B.ch
Acq On : 18 Jul 2018 15:03
Operator : AJ\SJ
Sample : J4035-16
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 19 02:09:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	1653463	15.349 ug/ml
Target Compounds			
4) N-TETRADECANE	8.080	497350	3.954 ug/ml
13) N-TRIACONTANE	17.508	269478	2.242 ug/ml
14) N-DOTRIACONTANE	18.344	425942	3.613 ug/ml
15) N-TETRATRIACONTANE	19.136	143568	1.222 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071818\
Data File : FF001407.D
Signal(s) : FID2B.ch
Acq On : 18 Jul 2018 15:03
Operator : AJ\SJ
Sample : J4035-16
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 19 02:09:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

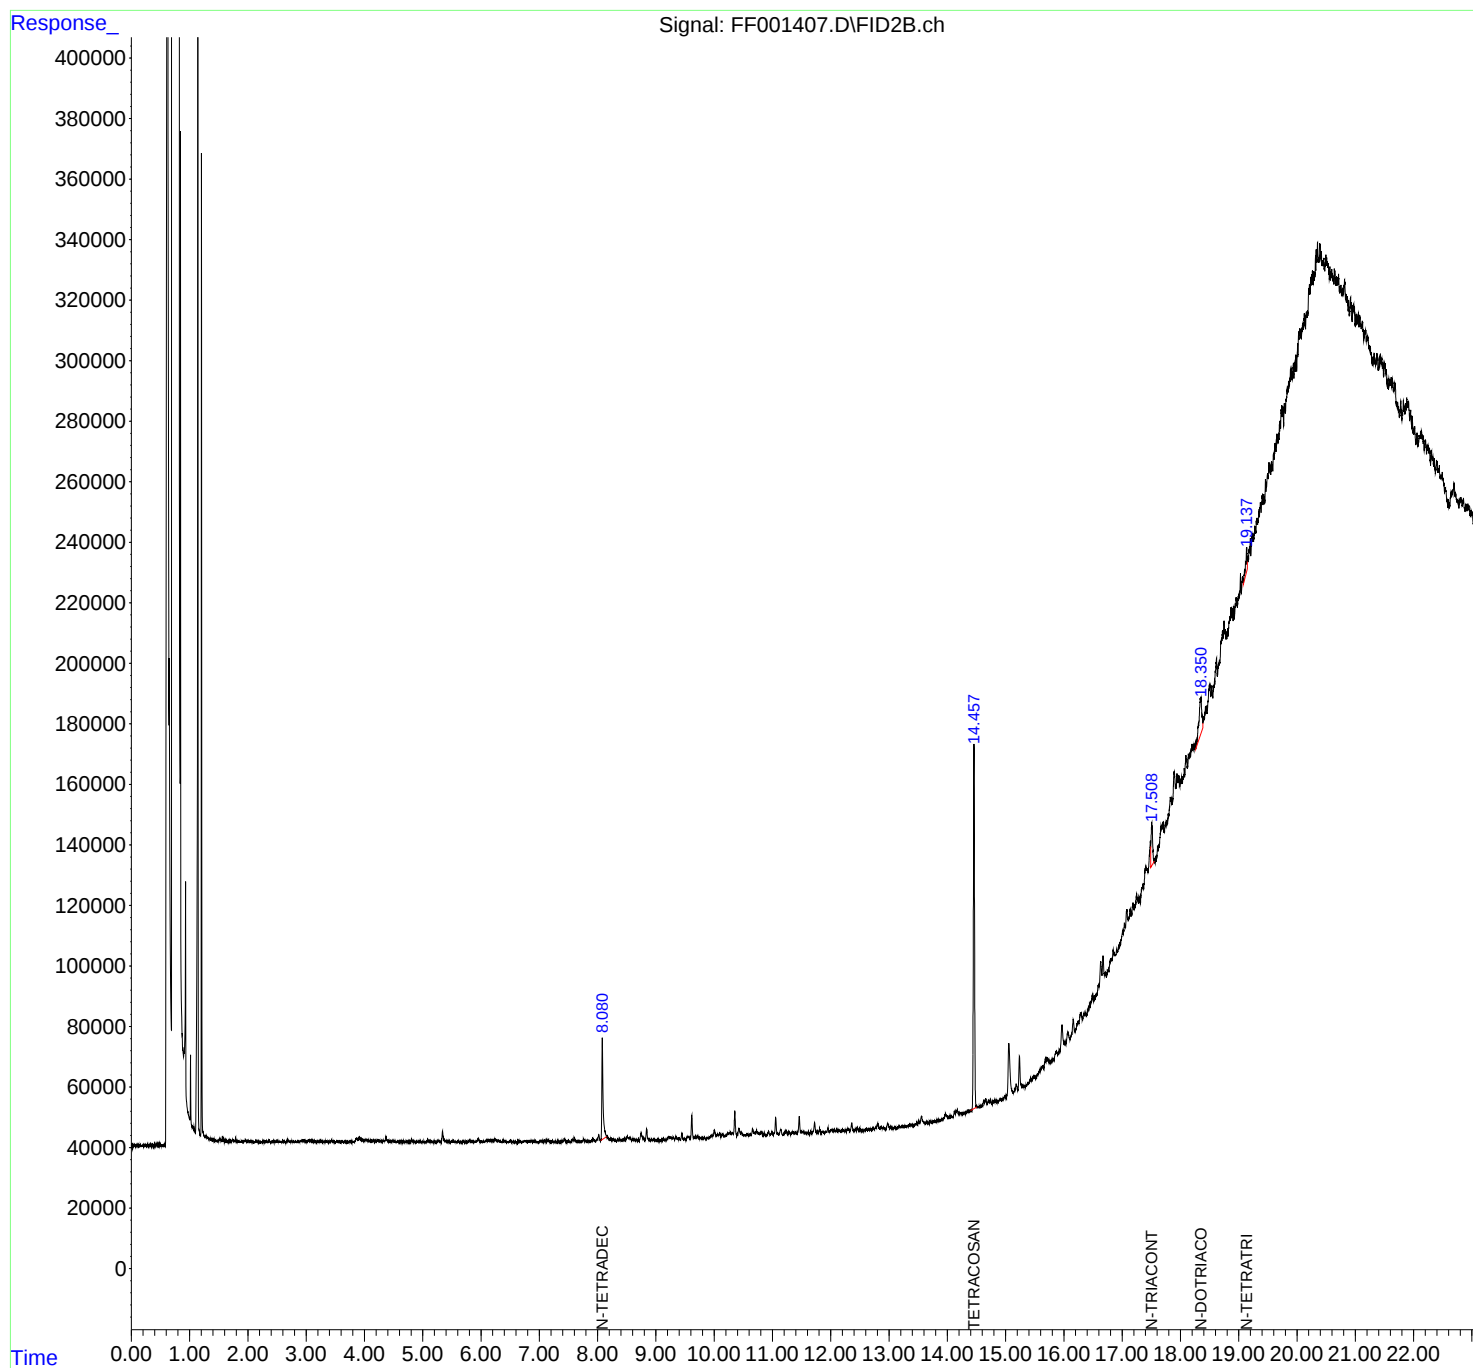

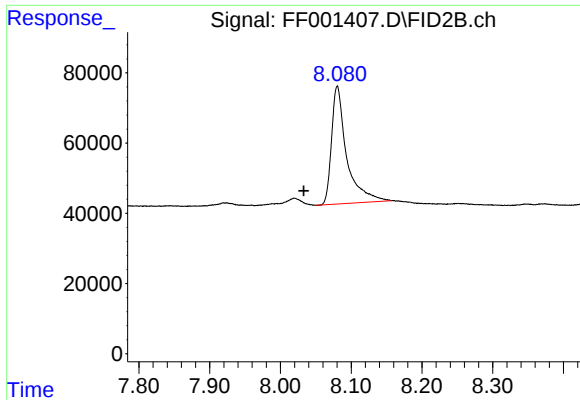


#4 N-TETRADECANE

R.T.: 8.080 min
Delta R.T.: 0.048 min
Response: 497350
Conc: 3.95 ug/ml

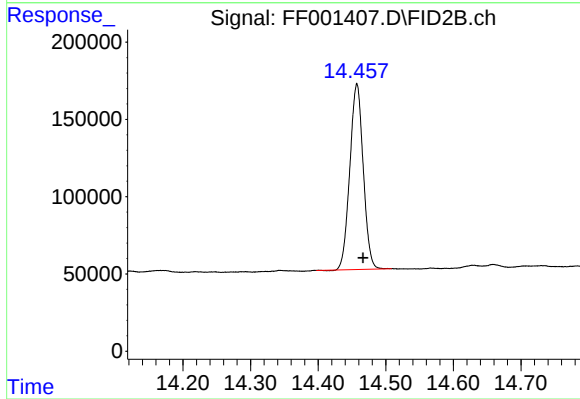


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.457 min
Delta R.T.: -0.009 min
Response: 1653463
Conc: 15.35 ug/ml

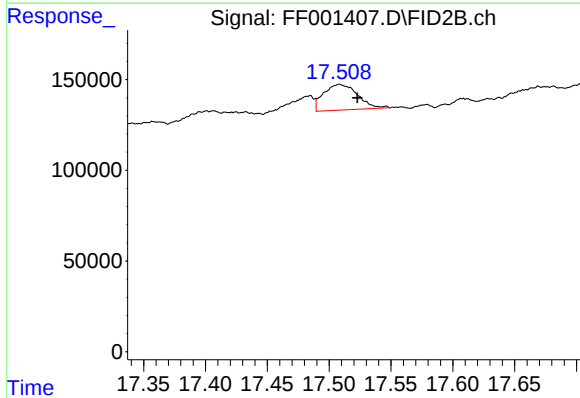


#13 N-TRIACONTANE

R.T.: 17.508 min
Delta R.T.: -0.014 min
Response: 269478
Conc: 2.24 ug/ml

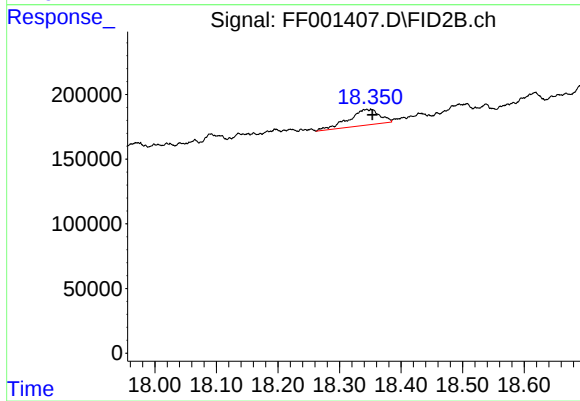

#14 N-DOTRIACONTANE

R.T.: 18.344 min
Delta R.T.: -0.009 min
Response: 425942
Conc: 3.61 ug/ml

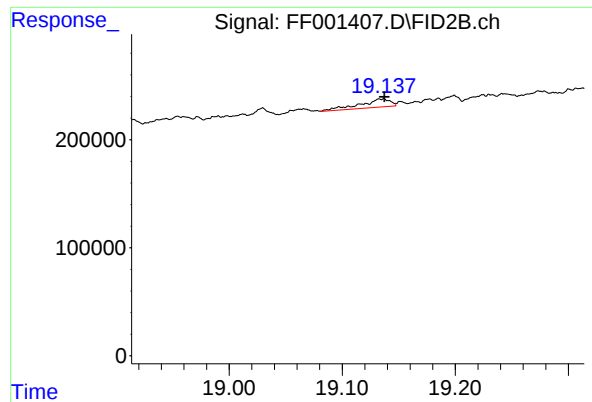

#15 N-TETRATRIACONTANE

R.T.: 19.136 min

Delta R.T.: 0.000 min

Response: 143568

Conc: 1.22 ug/ml