

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071822\
Data File : FF011056.D
Signal(s) : FID2B.ch
Acq On : 18 Jul 2022 13:05
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 19 01:38:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.537	1970988	17.698 ug/ml
12)	N-OCTACOSANE	16.986	1703727	16.324 ug/ml
14)	N-DOTRIACONTANE	18.702	100726	0.939 ug/ml
15)	N-TETRATRIACONTANE	19.485	103212	1.059 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071822\
Data File : FF011056.D
Signal(s) : FID2B.ch
Acq On : 18 Jul 2022 13:05
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 19 01:38:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

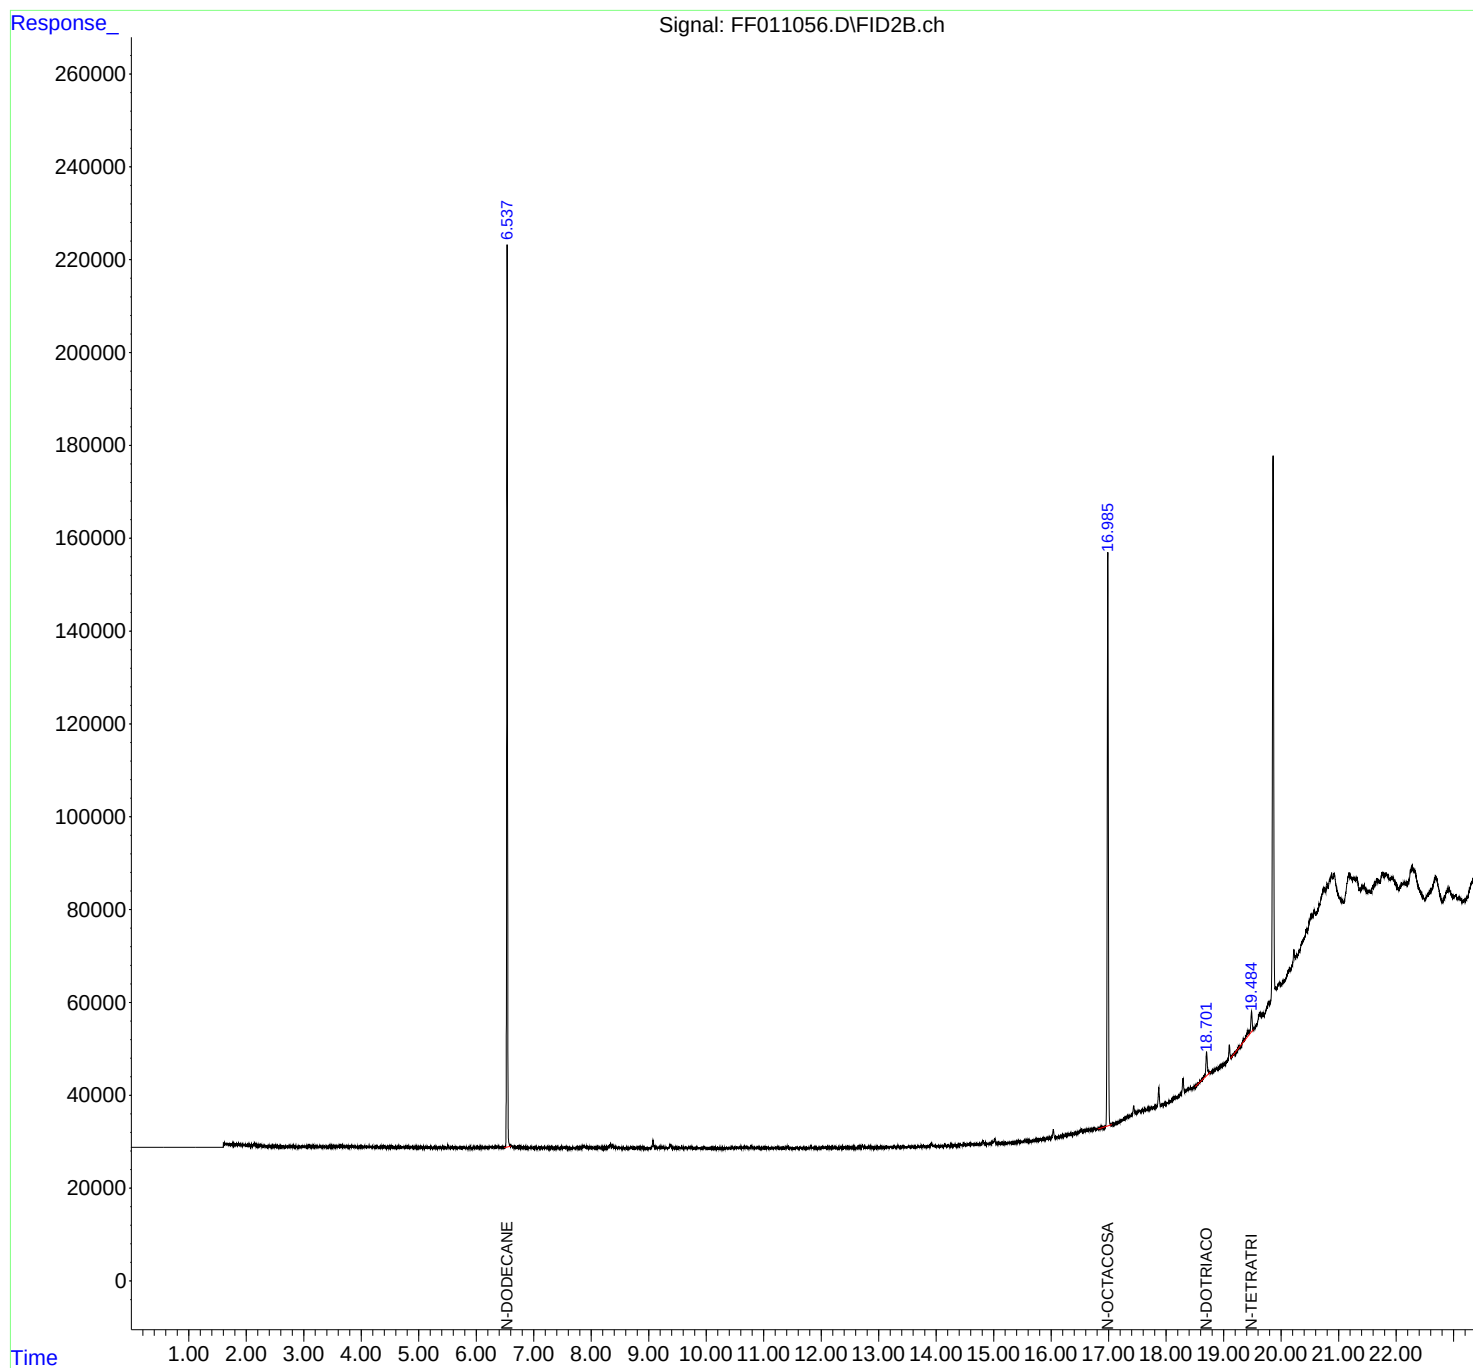

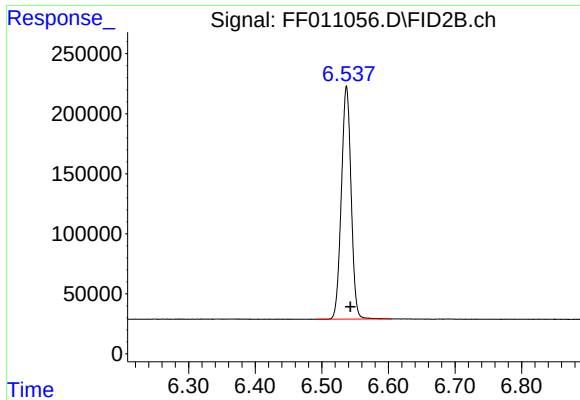


#3 N-DODECANE

R.T.: 6.537 min
Delta R.T.: -0.006 min
Response: 1970988
Conc: 17.70 ug/ml

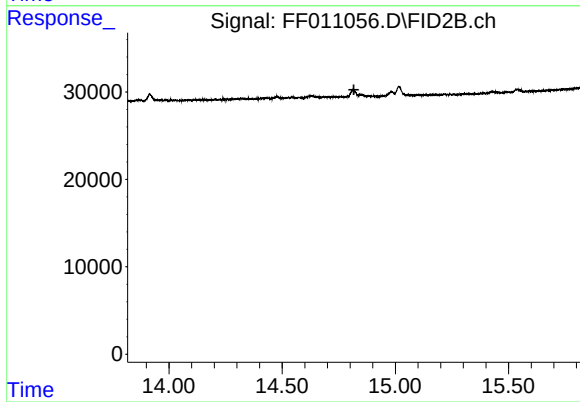


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

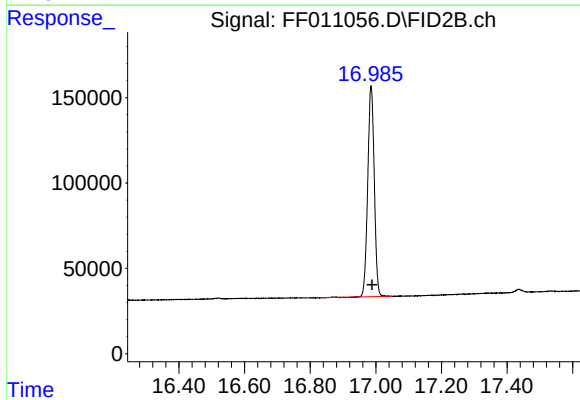


#12 N-OCTACOSANE

R.T.: 16.986 min
Delta R.T.: -0.003 min
Response: 1703727
Conc: 16.32 ug/ml

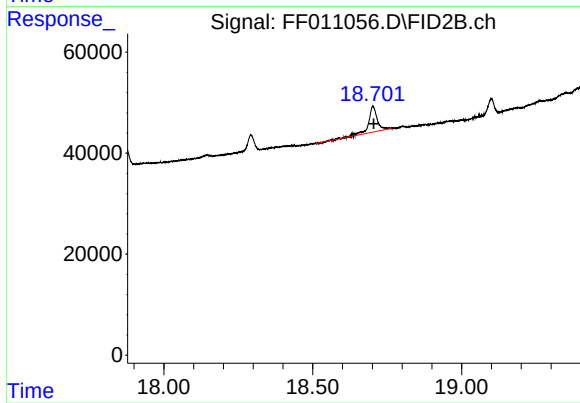

#14 N-DOTRIACONTANE

R.T.: 18.702 min
Delta R.T.: -0.003 min
Response: 100726
Conc: 0.94 ug/ml

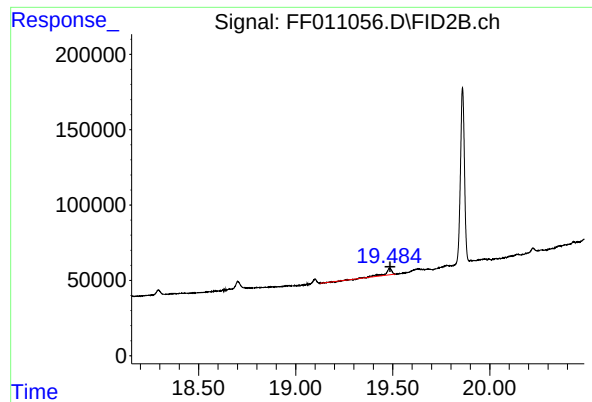

#15 N-TETRATRIACONTANE

R.T.: 19.485 min

Delta R.T.: -0.002 min

Response: 103212

Conc: 1.06 ug/ml