

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071822\
 Data File : FF011058.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jul 2022 14:05
 Operator : AJ\MA
 Sample : N3730-06 2X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 19 01:38:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
 Quant Title :
 QLast Update : Fri Jul 01 01:40:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.814	739389	7.882 ug/ml
Target Compounds			
7) N-EICOSANE	12.759	612451	5.697 ug/ml
8) N-DOCOSANE	13.922	100423	0.948 ug/ml
10) N-TETRACOSANE	14.976	397376	3.790 ug/ml
11) N-HEXACOSANE	16.038	81183	0.779 ug/ml
12) N-OCTACOSANE	16.979	271657	2.603 ug/ml
13) N-TRIACONTANE	17.871	396852	3.780 ug/ml
14) N-DOTRIACONTANE	18.704	342277	3.189 ug/ml
15) N-TETRATRIACONTANE	19.490	104063	1.067 ug/ml
16) N-HEXATRIACONTANE	20.228	101784	1.184 ug/ml
17) N-OCTATRIACONTANE	20.940	120662	1.609 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071822\
Data File : FF011058.D
Signal(s) : FID2B.ch
Acq On : 18 Jul 2022 14:05
Operator : AJ\MA
Sample : N3730-06 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 19 01:38:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

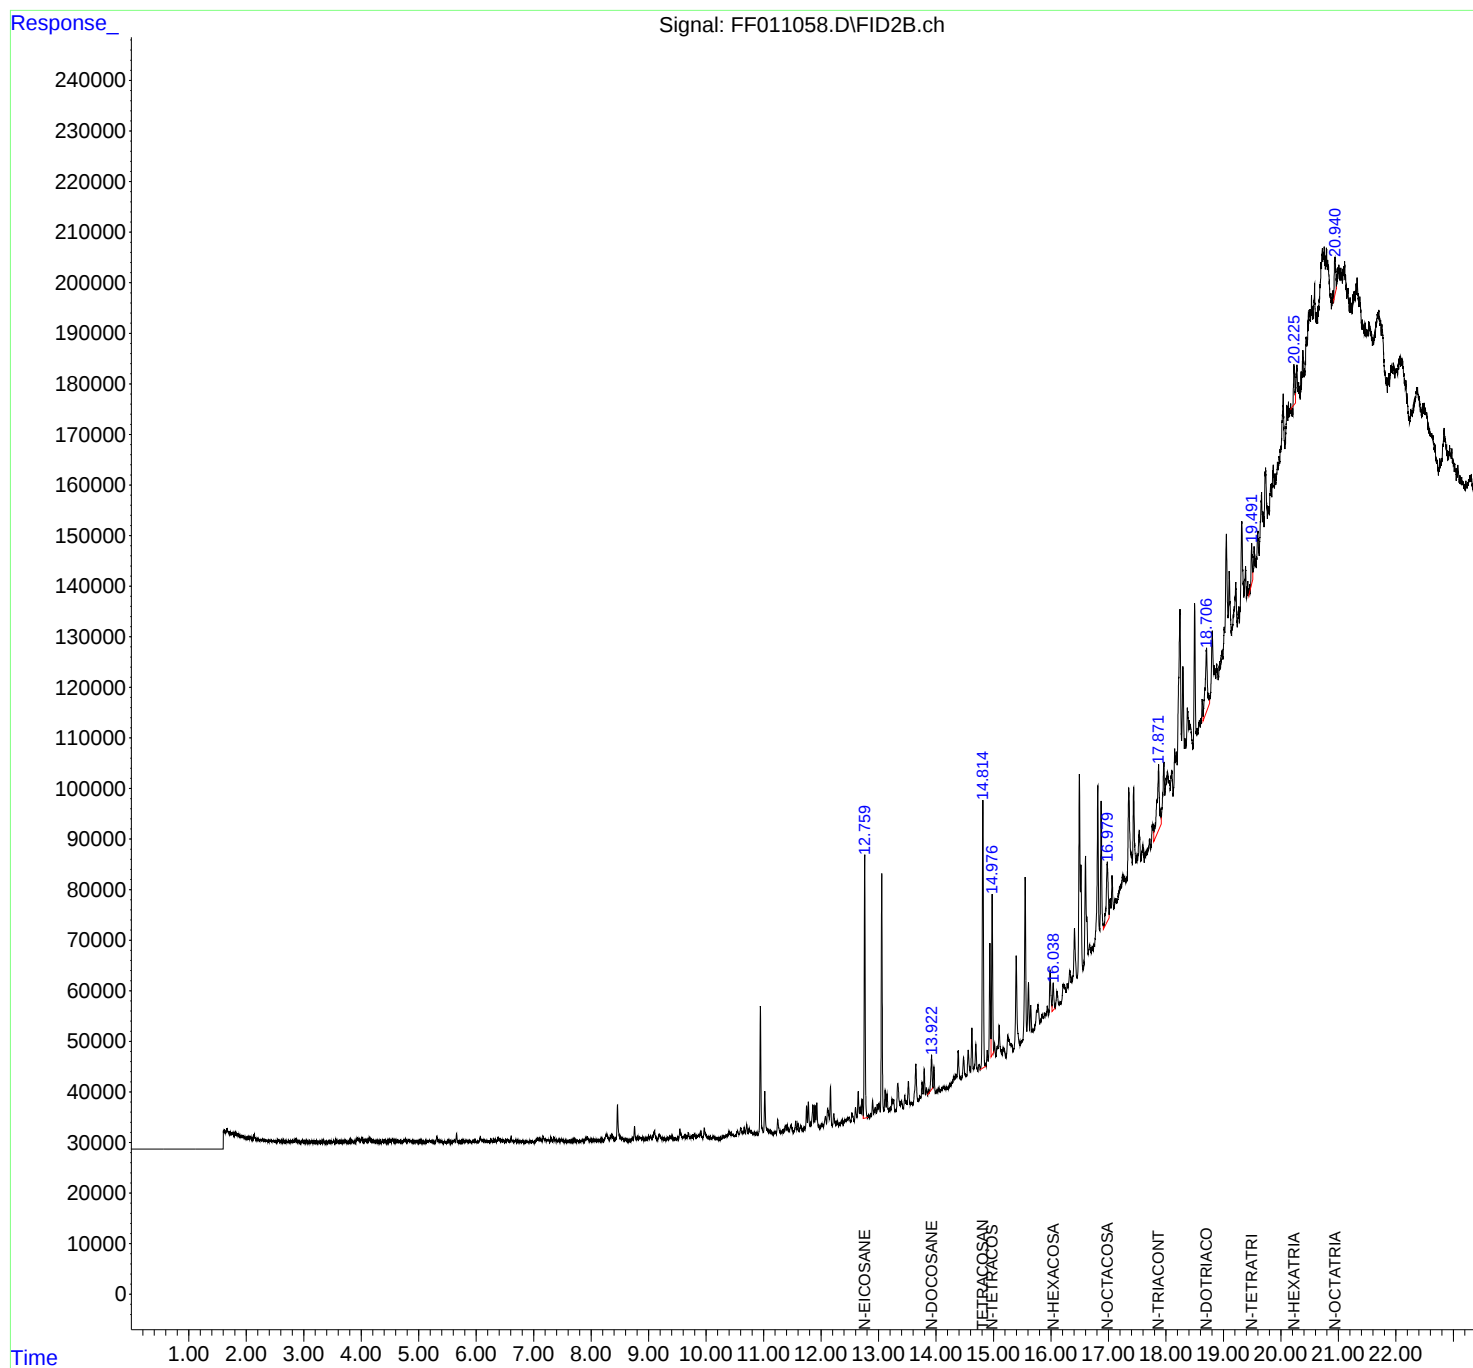

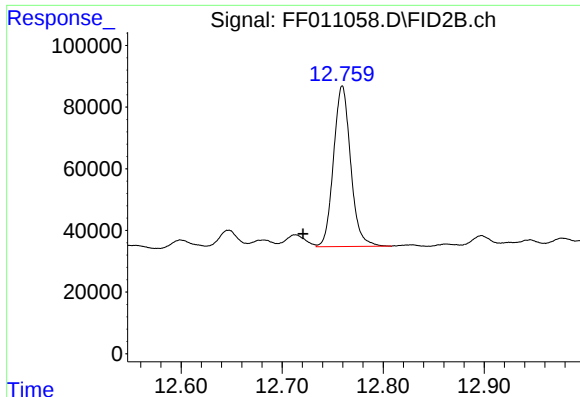


#7 N-EICOSANE

R.T.: 12.759 min
Delta R.T.: 0.039 min
Response: 612451
Conc: 5.70 ug/ml

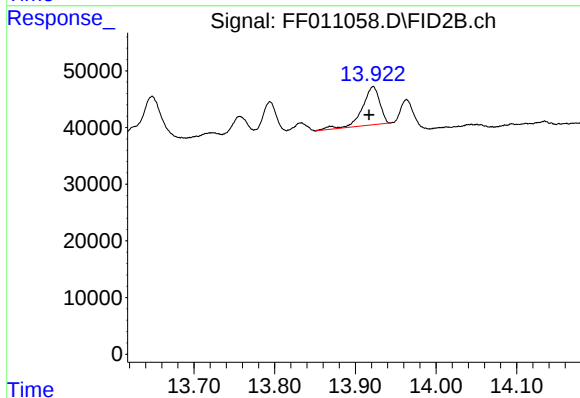


#8 N-DOCOSANE

R.T.: 13.922 min
Delta R.T.: 0.005 min
Response: 100423
Conc: 0.95 ug/ml

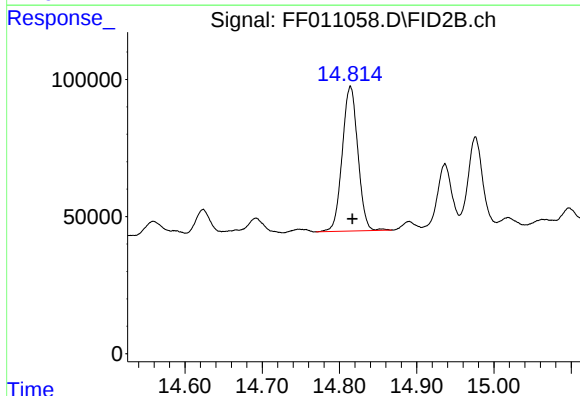


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.814 min
Delta R.T.: -0.003 min
Response: 739389
Conc: 7.88 ug/ml

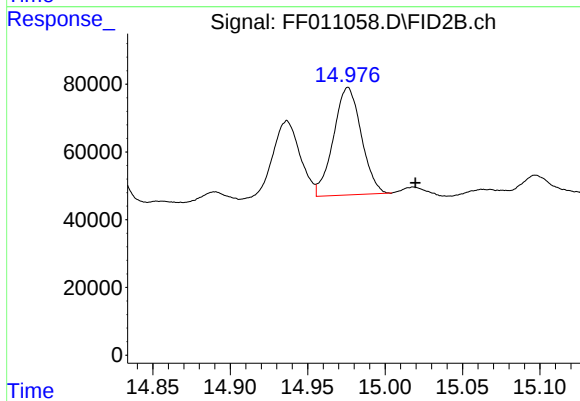


#10 N-TETRACOSANE

R.T.: 14.976 min
Delta R.T.: -0.044 min
Response: 397376
Conc: 3.79 ug/ml

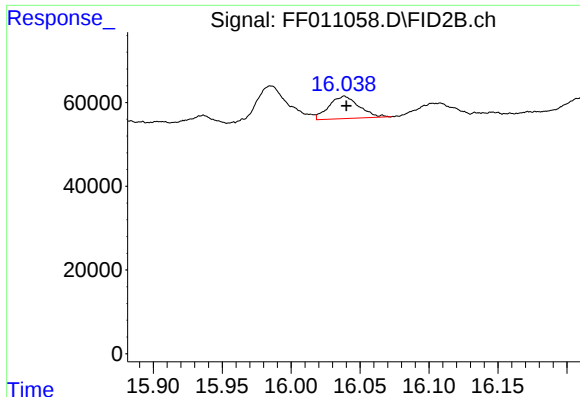


#11 N-HEXACOSANE

R.T.: 16.038 min
Delta R.T.: -0.002 min
Response: 81183
Conc: 0.78 ug/ml

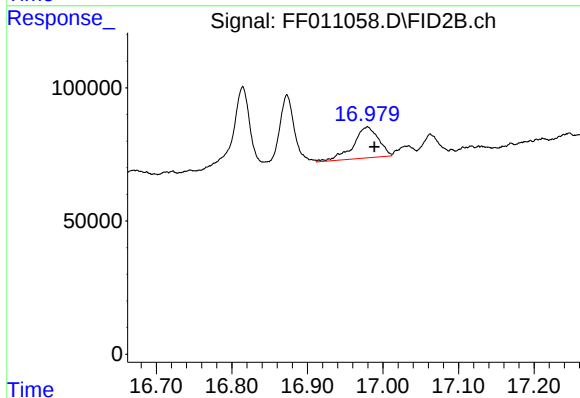


#12 N-OCTACOSANE

R.T.: 16.979 min
Delta R.T.: -0.010 min
Response: 271657
Conc: 2.60 ug/ml

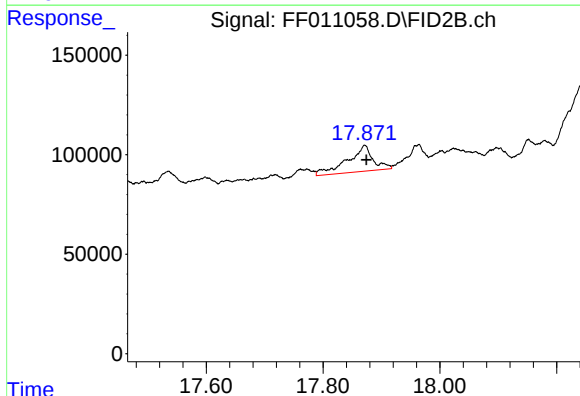


#13 N-TRIACONTANE

R.T.: 17.871 min
Delta R.T.: -0.003 min
Response: 396852
Conc: 3.78 ug/ml

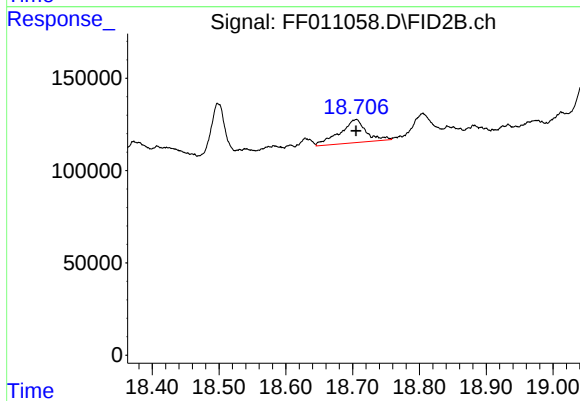


#14 N-DOTRIACONTANE

R.T.: 18.704 min
Delta R.T.: 0.000 min
Response: 342277
Conc: 3.19 ug/ml

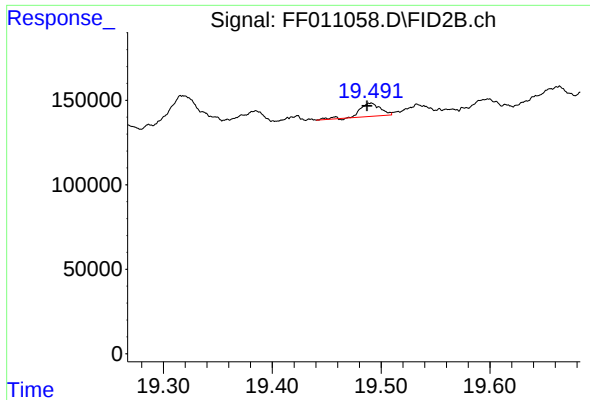


#15 N-TETRATRIACONTANE

R.T.: 19.490 min
Delta R.T.: 0.003 min
Response: 104063
Conc: 1.07 ug/ml

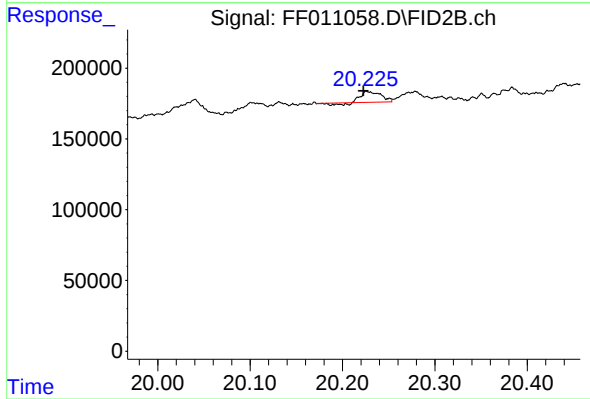

#16 N-HEXATRIACONTANE

R.T.: 20.228 min
Delta R.T.: 0.006 min
Response: 101784
Conc: 1.18 ug/ml

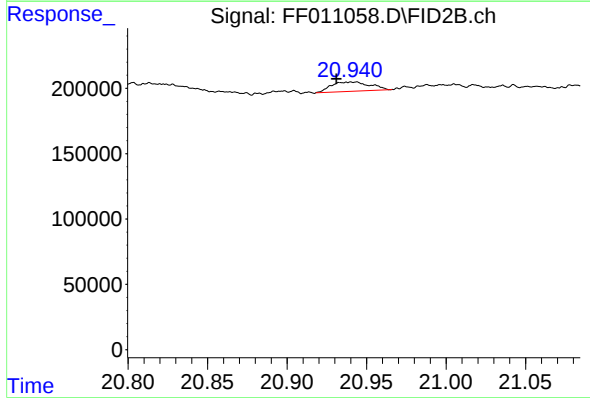

#17 N-OCTATRIACONTANE

R.T.: 20.940 min
Delta R.T.: 0.009 min
Response: 120662
Conc: 1.61 ug/ml