

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071921\
Data File : FF008837.D
Signal(s) : FID2B.ch
Acq On : 19 Jul 2021 10:27
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 20 01:38:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.633	200079	1.708 ug/ml
16)	N-HEXATRIACONTANE	20.180	167037	1.778 ug/ml
18)	N-TETRACONTANE	21.841	83599	0.903 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071921\
Data File : FF008837.D
Signal(s) : FID2B.ch
Acq On : 19 Jul 2021 10:27
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 20 01:38:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

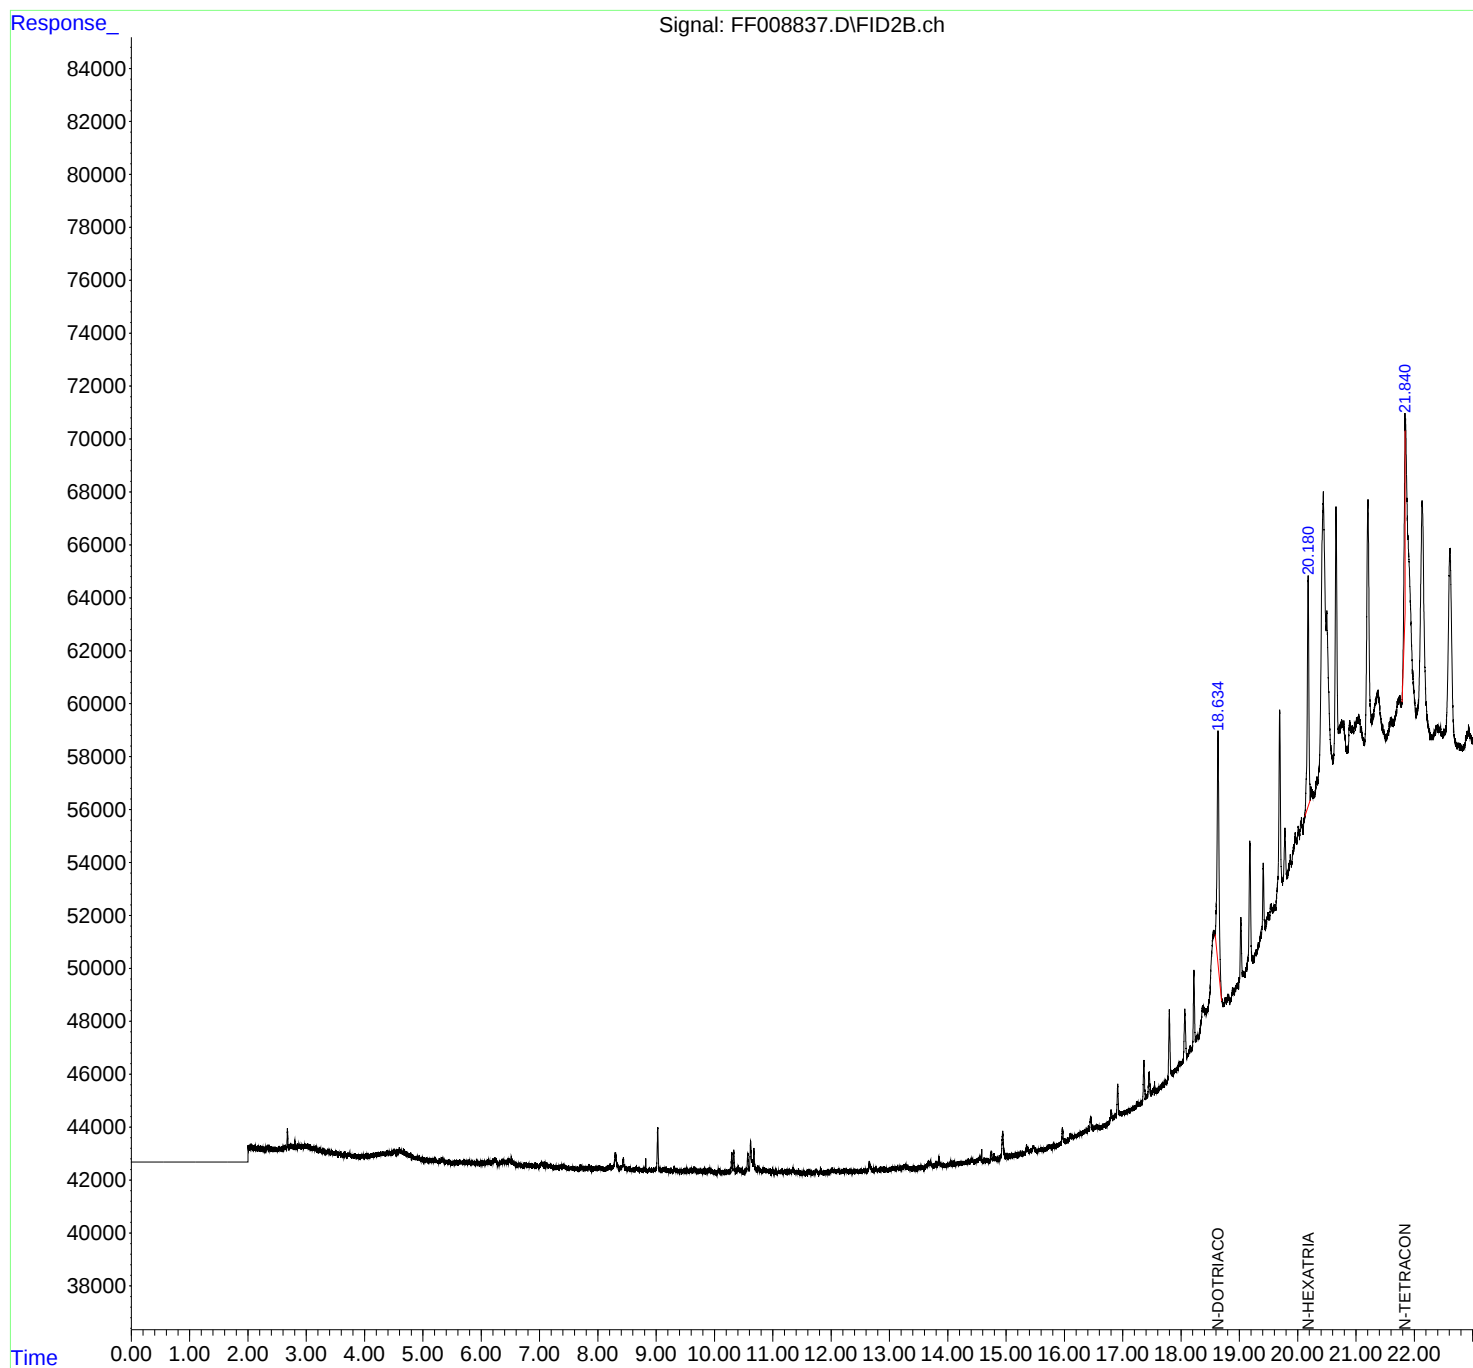

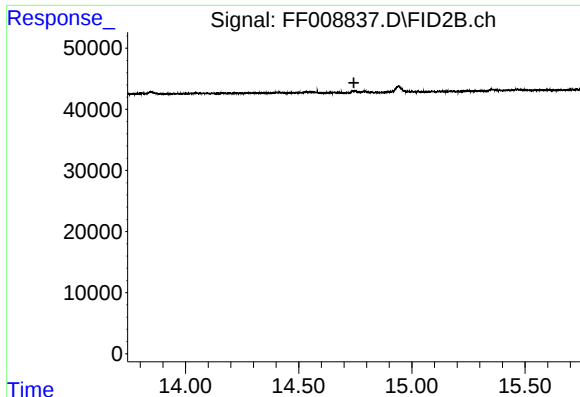


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.744 min
Response: 0
Conc: N.D.

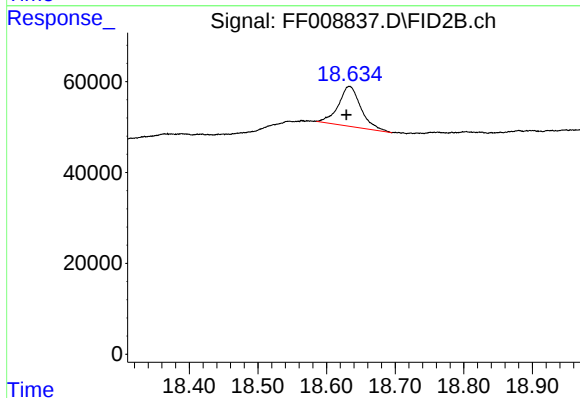


#14 N-DOTRIACONTANE

R.T.: 18.633 min
Delta R.T.: 0.004 min
Response: 200079
Conc: 1.71 ug/ml

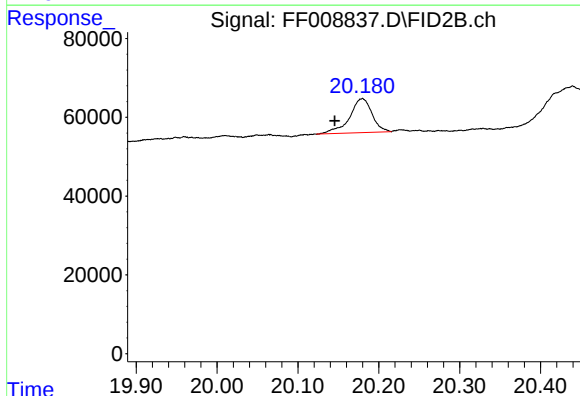

#16 N-HEXATRIACONTANE

R.T.: 20.180 min
Delta R.T.: 0.034 min
Response: 167037
Conc: 1.78 ug/ml

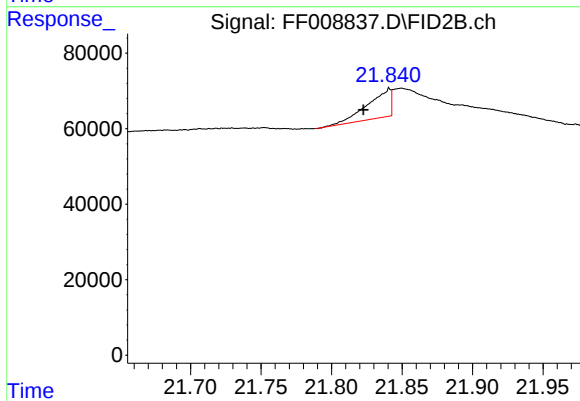

#18 N-TETRACONTANE

R.T.: 21.841 min
Delta R.T.: 0.018 min
Response: 83599
Conc: 0.90 ug/ml