

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071921\
Data File : FF008845.D
Signal(s) : FID2B.ch
Acq On : 19 Jul 2021 15:40
Operator : DD\AJ
Sample : PB137713BL
Misc : LOD 2.5 PPM
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 20 01:39:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.744	2238307	19.640 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.630	111264	0.950 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071921\
Data File : FF008845.D
Signal(s) : FID2B.ch
Acq On : 19 Jul 2021 15:40
Operator : DD\AJ
Sample : PB137713BL
Misc : LOD 2.5 PPM
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 20 01:39:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

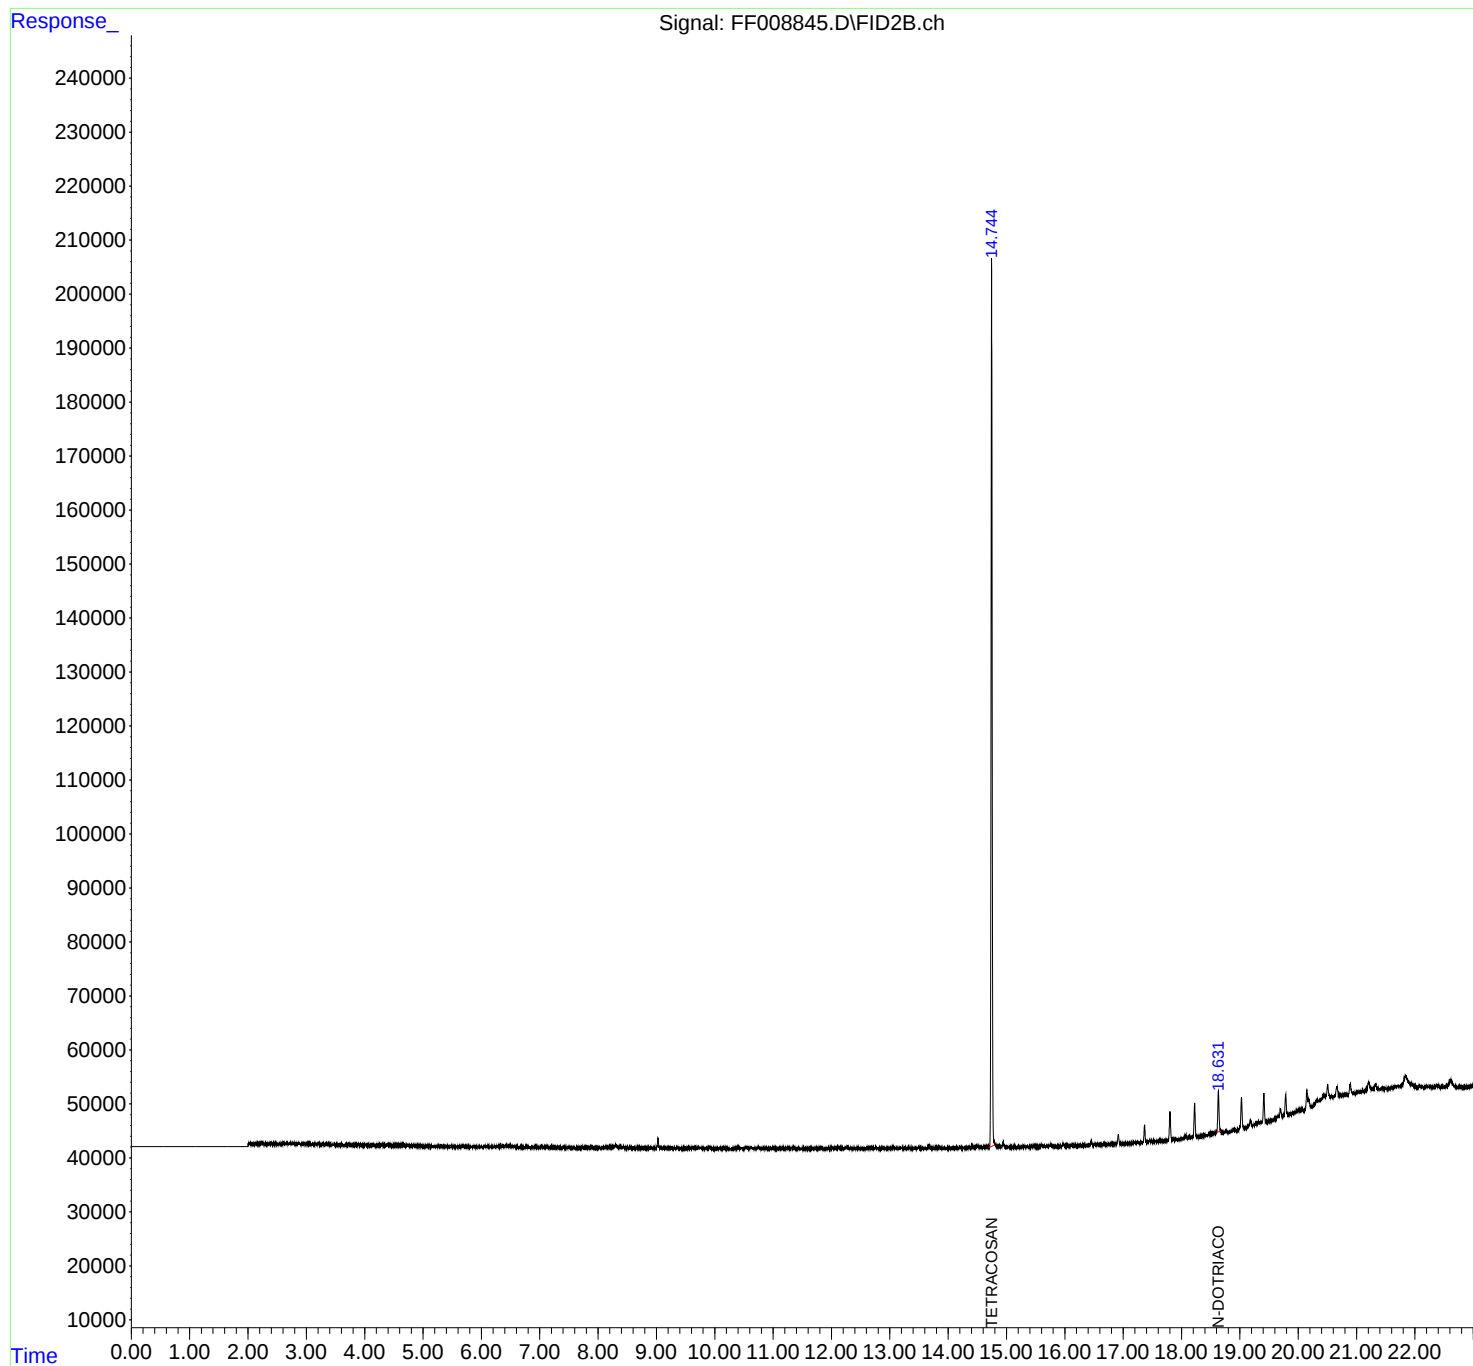

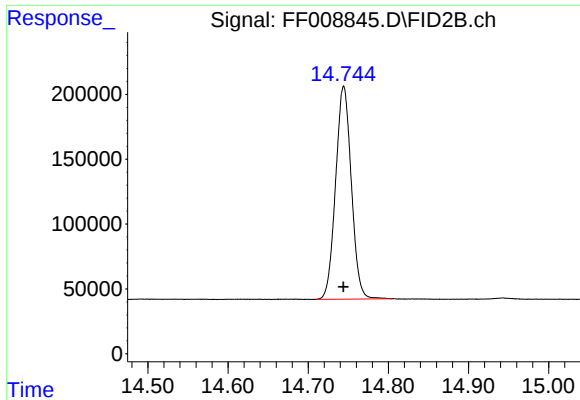

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.744 min
Delta R.T.: 0.000 min
Response: 2238307
Conc: 19.64 ug/ml

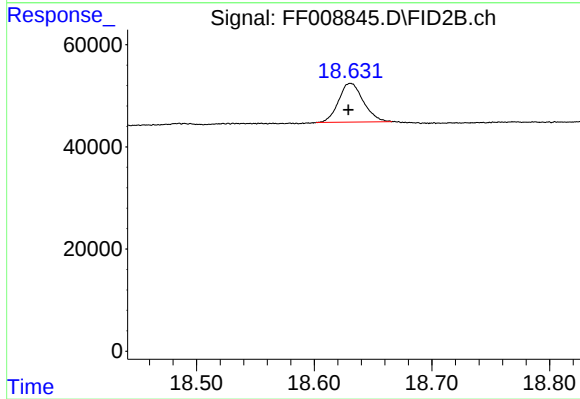

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: 0.002 min
Response: 111264
Conc: 0.95 ug/ml