

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072021\
 Data File : FF008855.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jul 2021 11:26
 Operator : DD\AJ
 Sample : PB137734BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 21 01:08:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.743	2439457	21.405 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.799	162550	1.356 ug/ml
14) N-DOTRIACONTANE	18.629	248577	2.122 ug/ml
15) N-TETRATRIACONTANE	19.409	180317	1.725 ug/ml
16) N-HEXATRIACONTANE	20.148	87916	0.936 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072021\
Data File : FF008855.D
Signal(s) : FID2B.ch
Acq On : 20 Jul 2021 11:26
Operator : DD\AJ
Sample : PB137734BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 21 01:08:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

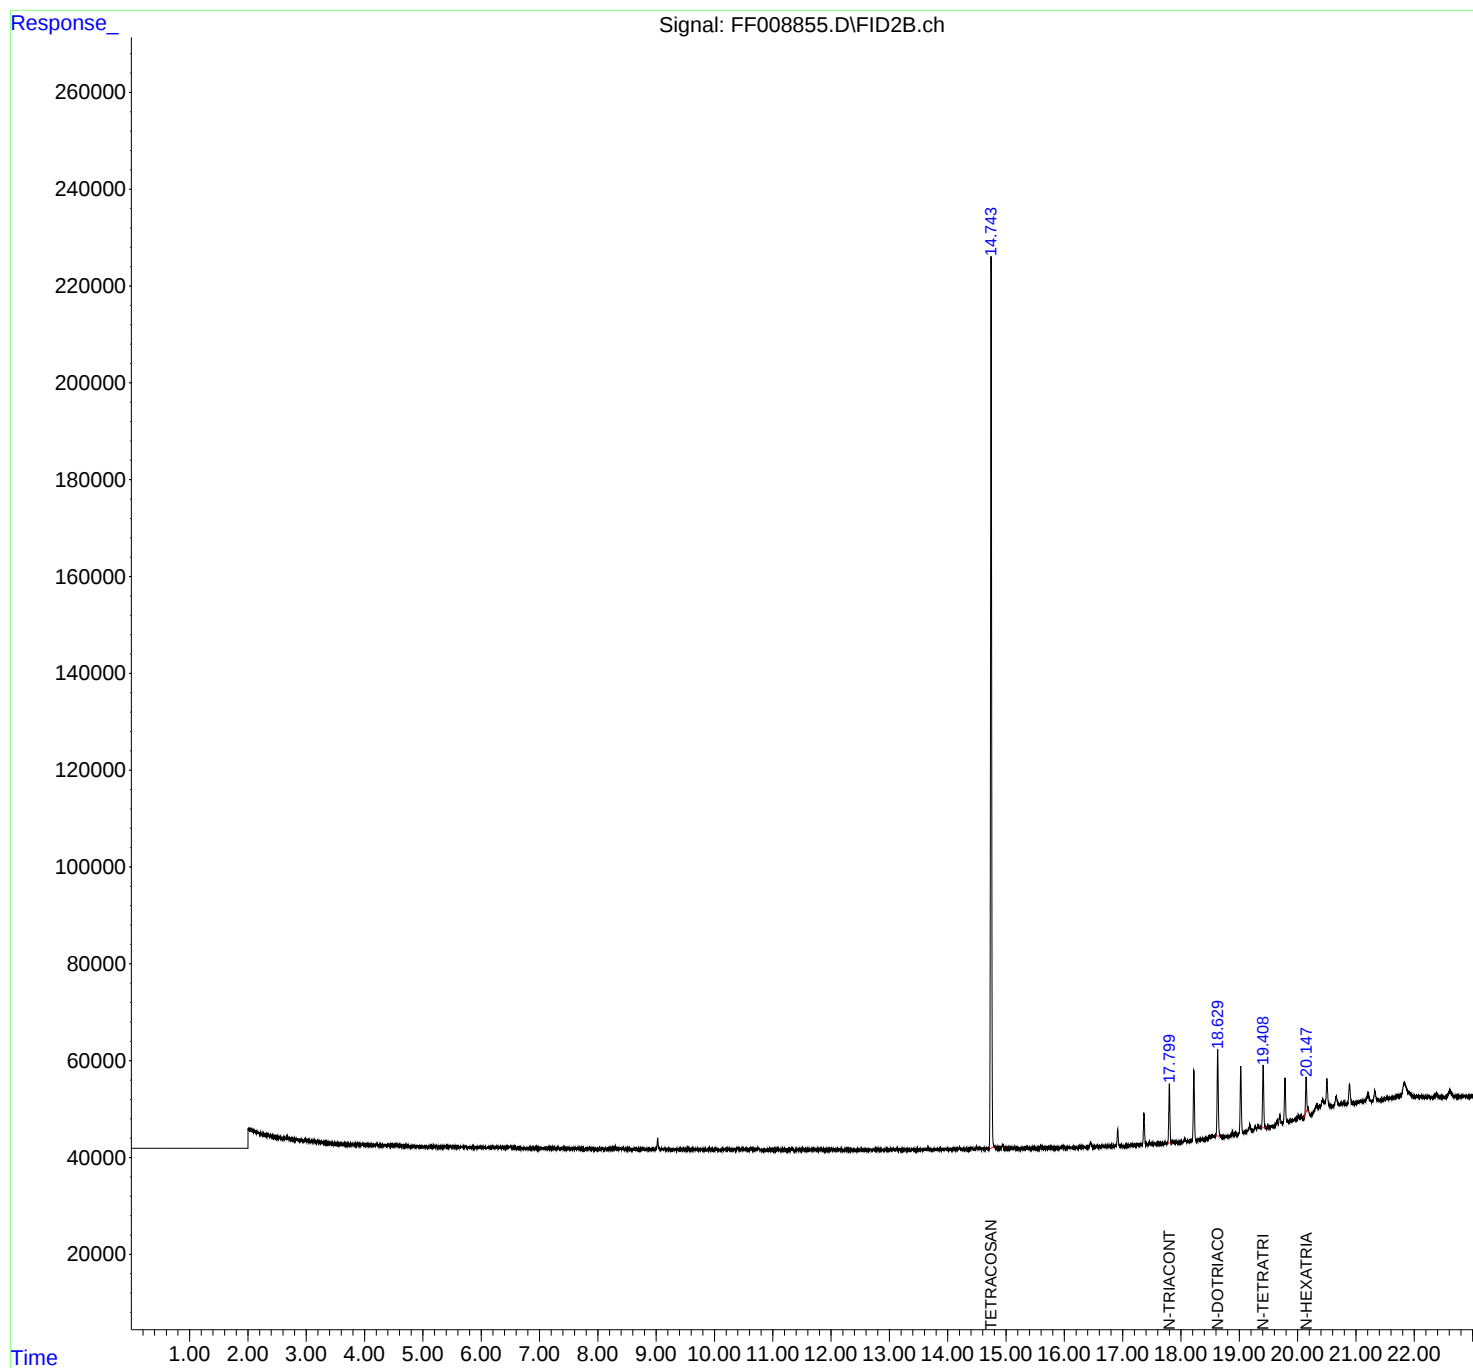

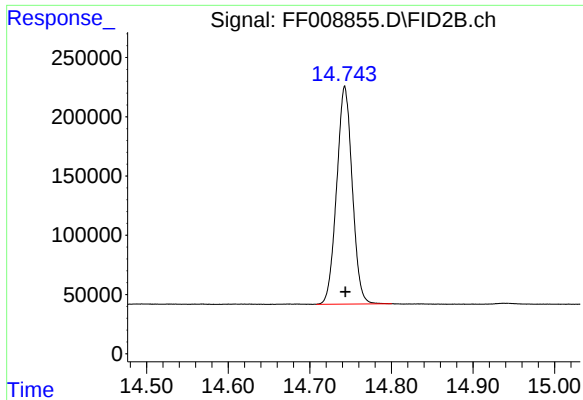


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.743 min
Delta R.T.: -0.001 min
Response: 2439457
Conc: 21.40 ug/ml

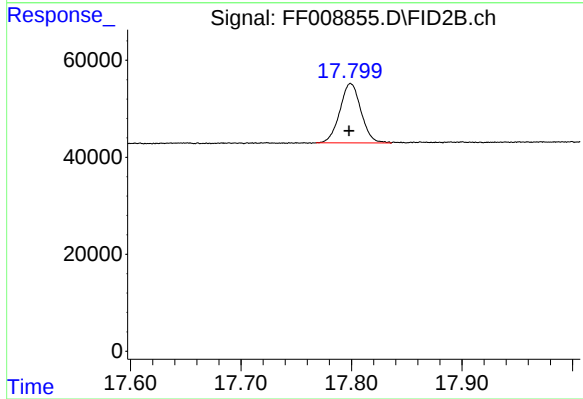


#13 N-TRIACONTANE

R.T.: 17.799 min
Delta R.T.: 0.001 min
Response: 162550
Conc: 1.36 ug/ml

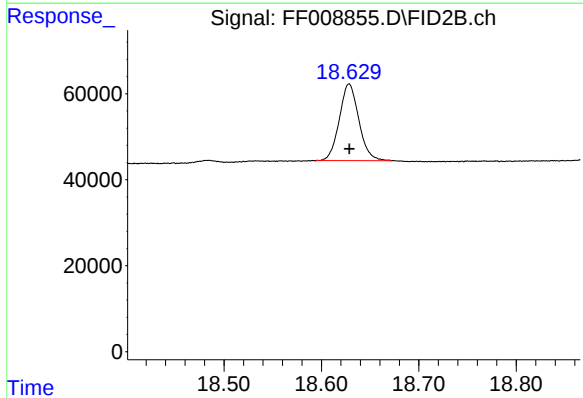


#14 N-DOTRIACONTANE

R.T.: 18.629 min
Delta R.T.: 0.000 min
Response: 248577
Conc: 2.12 ug/ml

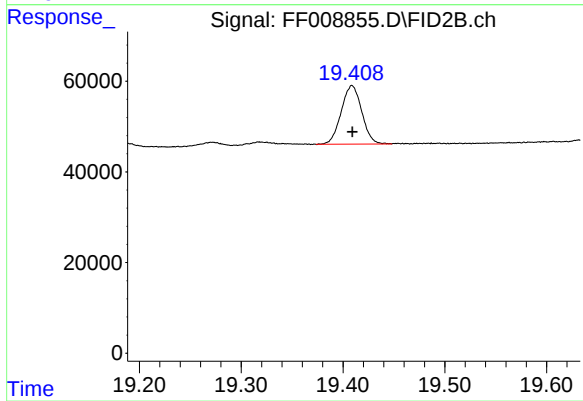

#15 N-TETRATRIACONTANE

R.T.: 19.409 min
Delta R.T.: 0.000 min
Response: 180317
Conc: 1.72 ug/ml

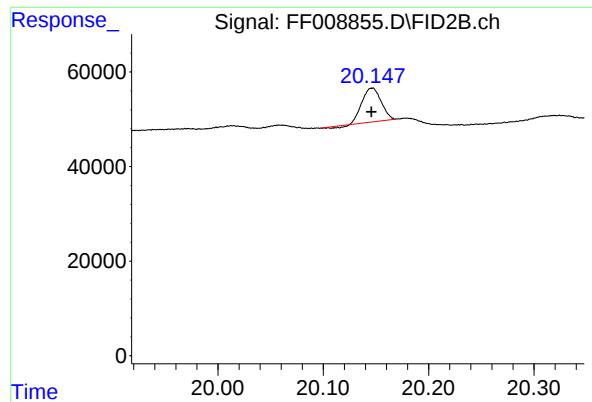

#16 N-HEXATRIACONTANE

R.T.: 20.148 min
Delta R.T.: 0.002 min
Response: 87916
Conc: 0.94 ug/ml