

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
 Data File : FF007184.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jul 2020 14:45
 Operator : DD\AJ
 Sample : L3354-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 BACK-YARD

Integration File: autoint1.e
 Quant Time: Jul 22 01:12:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.744	2991489	21.220 ug/ml
Target Compounds			
4) N-TETRADECANE	8.342f	928434	5.996 ug/ml
10) N-TETRACOSANE	14.915	232822	1.422 ug/ml
12) N-OCTACOSANE	16.999f	597216	3.645 ug/ml
14) N-DOTRIACONTANE	18.631	580854	3.699 ug/ml
15) N-TETRATRIACONTANE	19.500f	294314	2.261 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
Data File : FF07184.D
Signal(s) : FID2B.ch
Acq On : 21 Jul 2020 14:45
Operator : DD\AJ
Sample : L3354-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
BACK-YARD

Integration File: autoint1.e
Quant Time: Jul 22 01:12:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

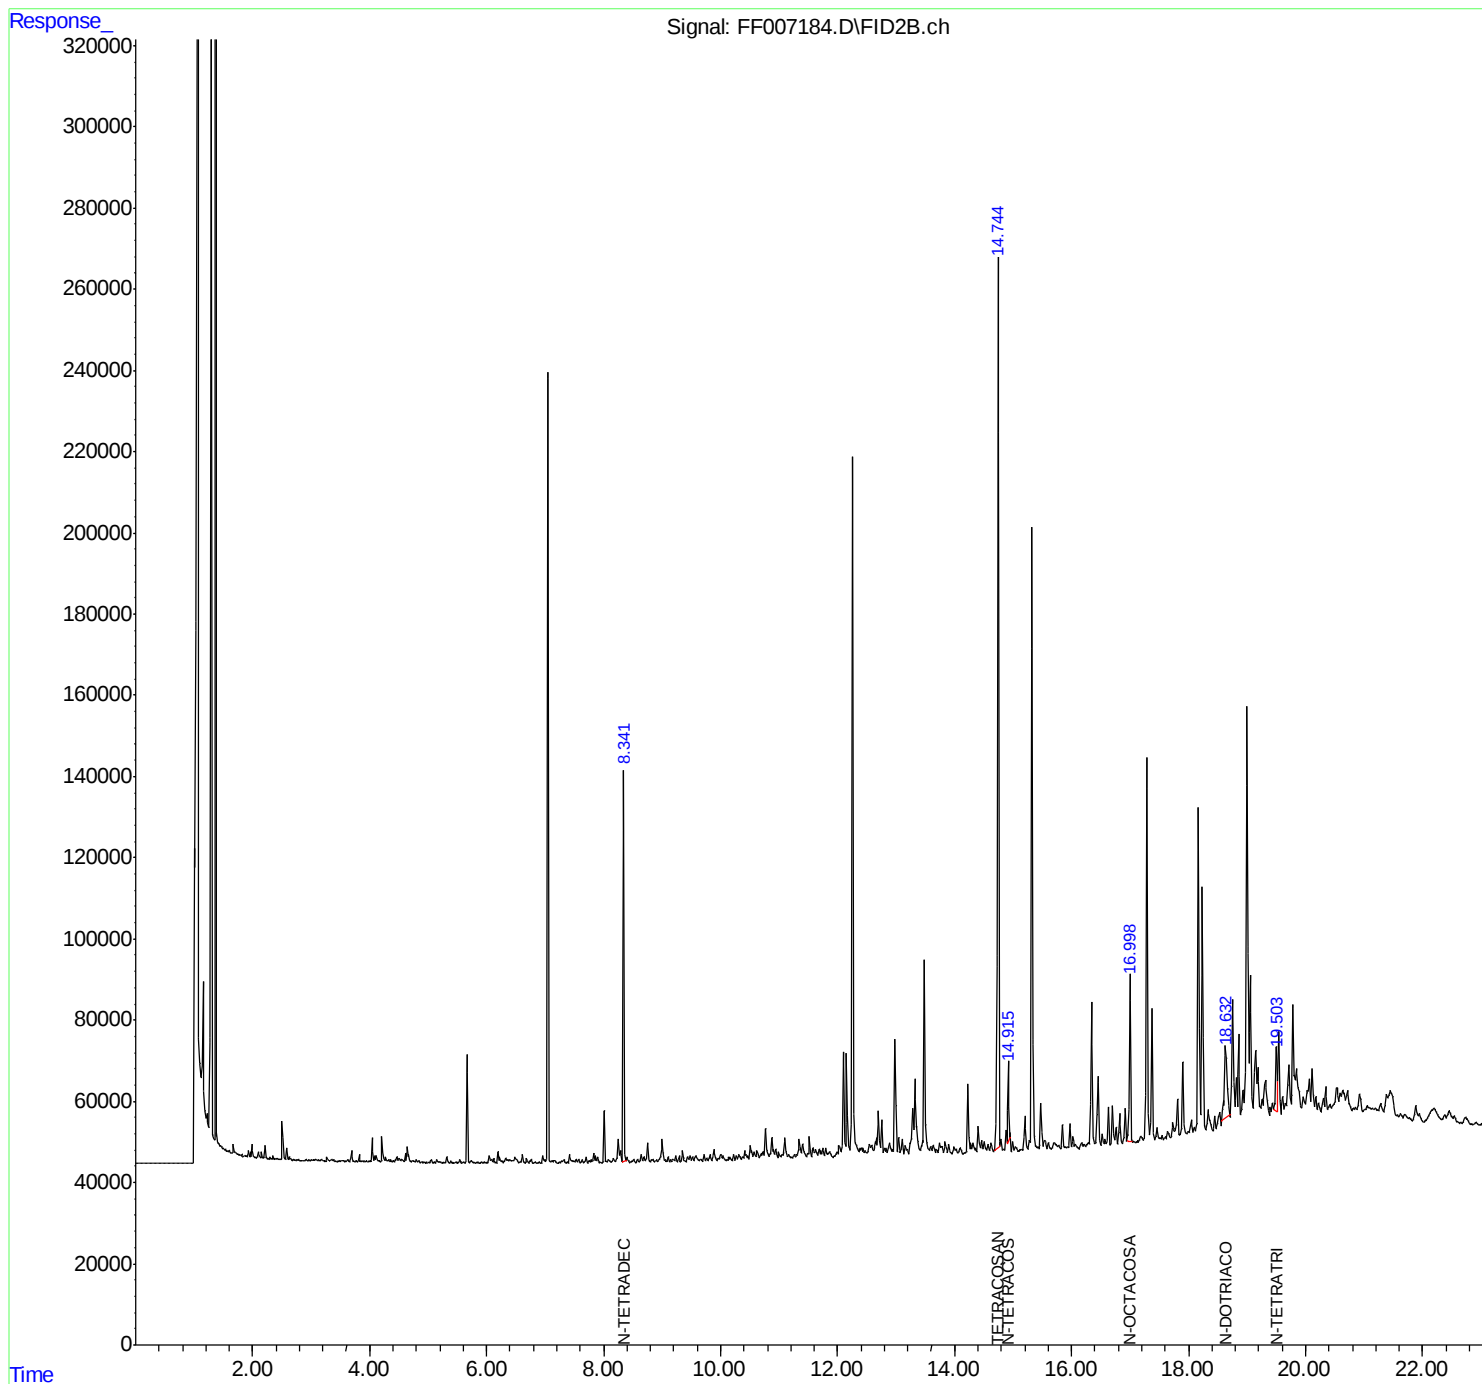


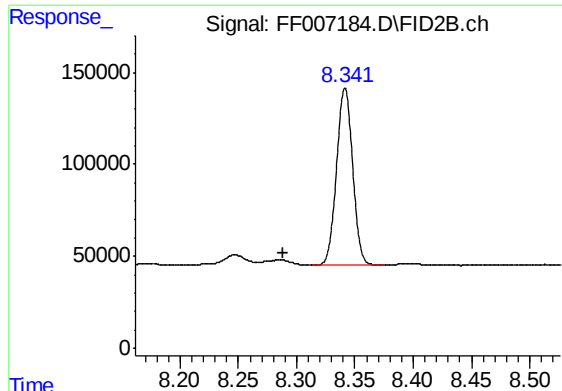

#4 N-TETRADECANE


R.T.: 8.342 min
Delta R.T.: 0.053 min
Response: 928434
Conc: 6.00 ug/ml

Instrument :
FID_F
ClientSampleId :
BACK-YARD

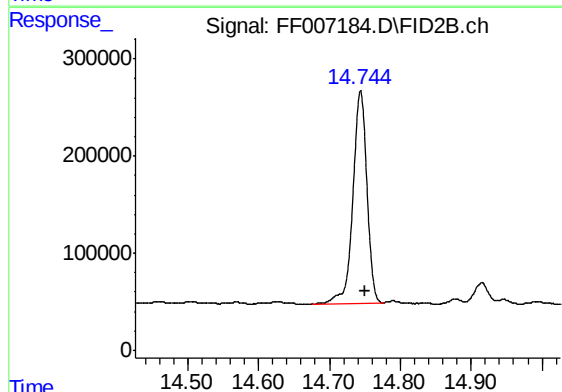


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.744 min
Delta R.T.: -0.007 min
Response: 2991489
Conc: 21.22 ug/ml

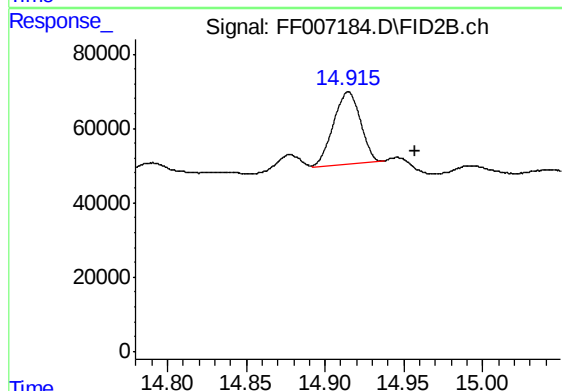


#10 N-TETRACOSANE

R.T.: 14.915 min
Delta R.T.: -0.042 min
Response: 232822
Conc: 1.42 ug/ml

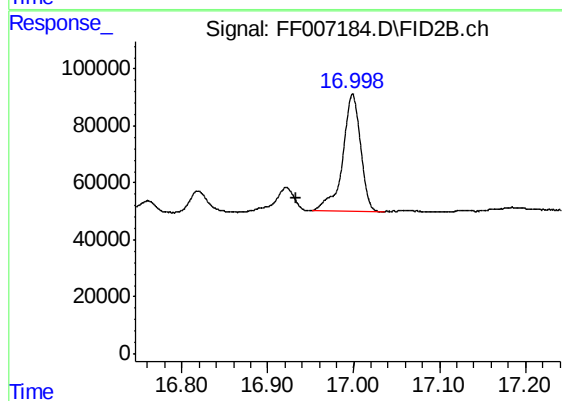

#12 N-OCTACOSANE


R.T.: 16.999 min
Delta R.T.: 0.066 min
Response: 597216
Conc: 3.64 ug/ml

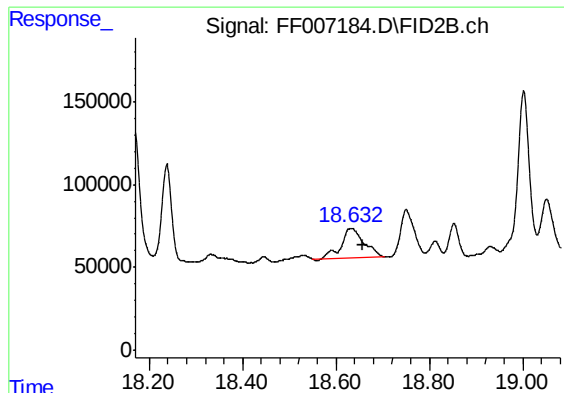

#14 N-DOTRIACONTANE

R.T.: 18.631 min
Delta R.T.: -0.025 min
Response: 580854
Conc: 3.70 ug/ml

Instrument :
FID_F
ClientSampleId :
BACK-YARD

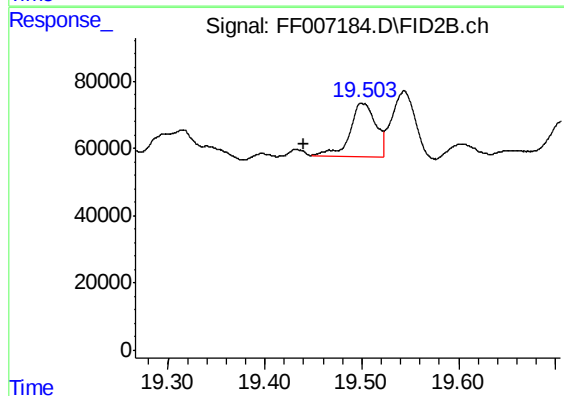

#15 N-TETRATRIACONTANE

R.T.: 19.500 min
Delta R.T.: 0.060 min
Response: 294314
Conc: 2.26 ug/ml