

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
 Data File : FF007185.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jul 2020 15:16
 Operator : DD\AJ
 Sample : L3360-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SP-1A

Integration File: autoint1.e
 Quant Time: Jul 22 01:12:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	2506680	17.781 ug/ml
Target Compounds			
4) N-TETRADECANE	8.342f	842283	5.440 ug/ml
7) N-EICOSANE	12.643	362529	2.245 ug/ml
8) N-DOCOSANE	13.870	992173	6.118 ug/ml
10) N-TETRACOSANE	14.933	4041328	24.677 ug/ml
11) N-HEXACOSANE	15.978	507670	3.122 ug/ml
12) N-OCTACOSANE	16.932	1437836	8.775 ug/ml
13) N-TRIACONTANE	17.820	1063016	6.431 ug/ml
14) N-DOTRIACONTANE	18.654	478972	3.050 ug/ml
15) N-TETRATRIACONTANE	19.444	250507	1.924 ug/ml
16) N-HEXATRIACONTANE	20.188	220105	2.253 ug/ml
17) N-OCTATRIACONTANE	20.945	367155	4.656 ug/ml
18) N-TETRACONTANE	21.884	177505	2.478 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
Data File : FF07185.D
Signal(s) : FID2B.ch
Acq On : 21 Jul 2020 15:16
Operator : DD\AJ
Sample : L3360-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP-1A

Integration File: autoint1.e
Quant Time: Jul 22 01:12:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

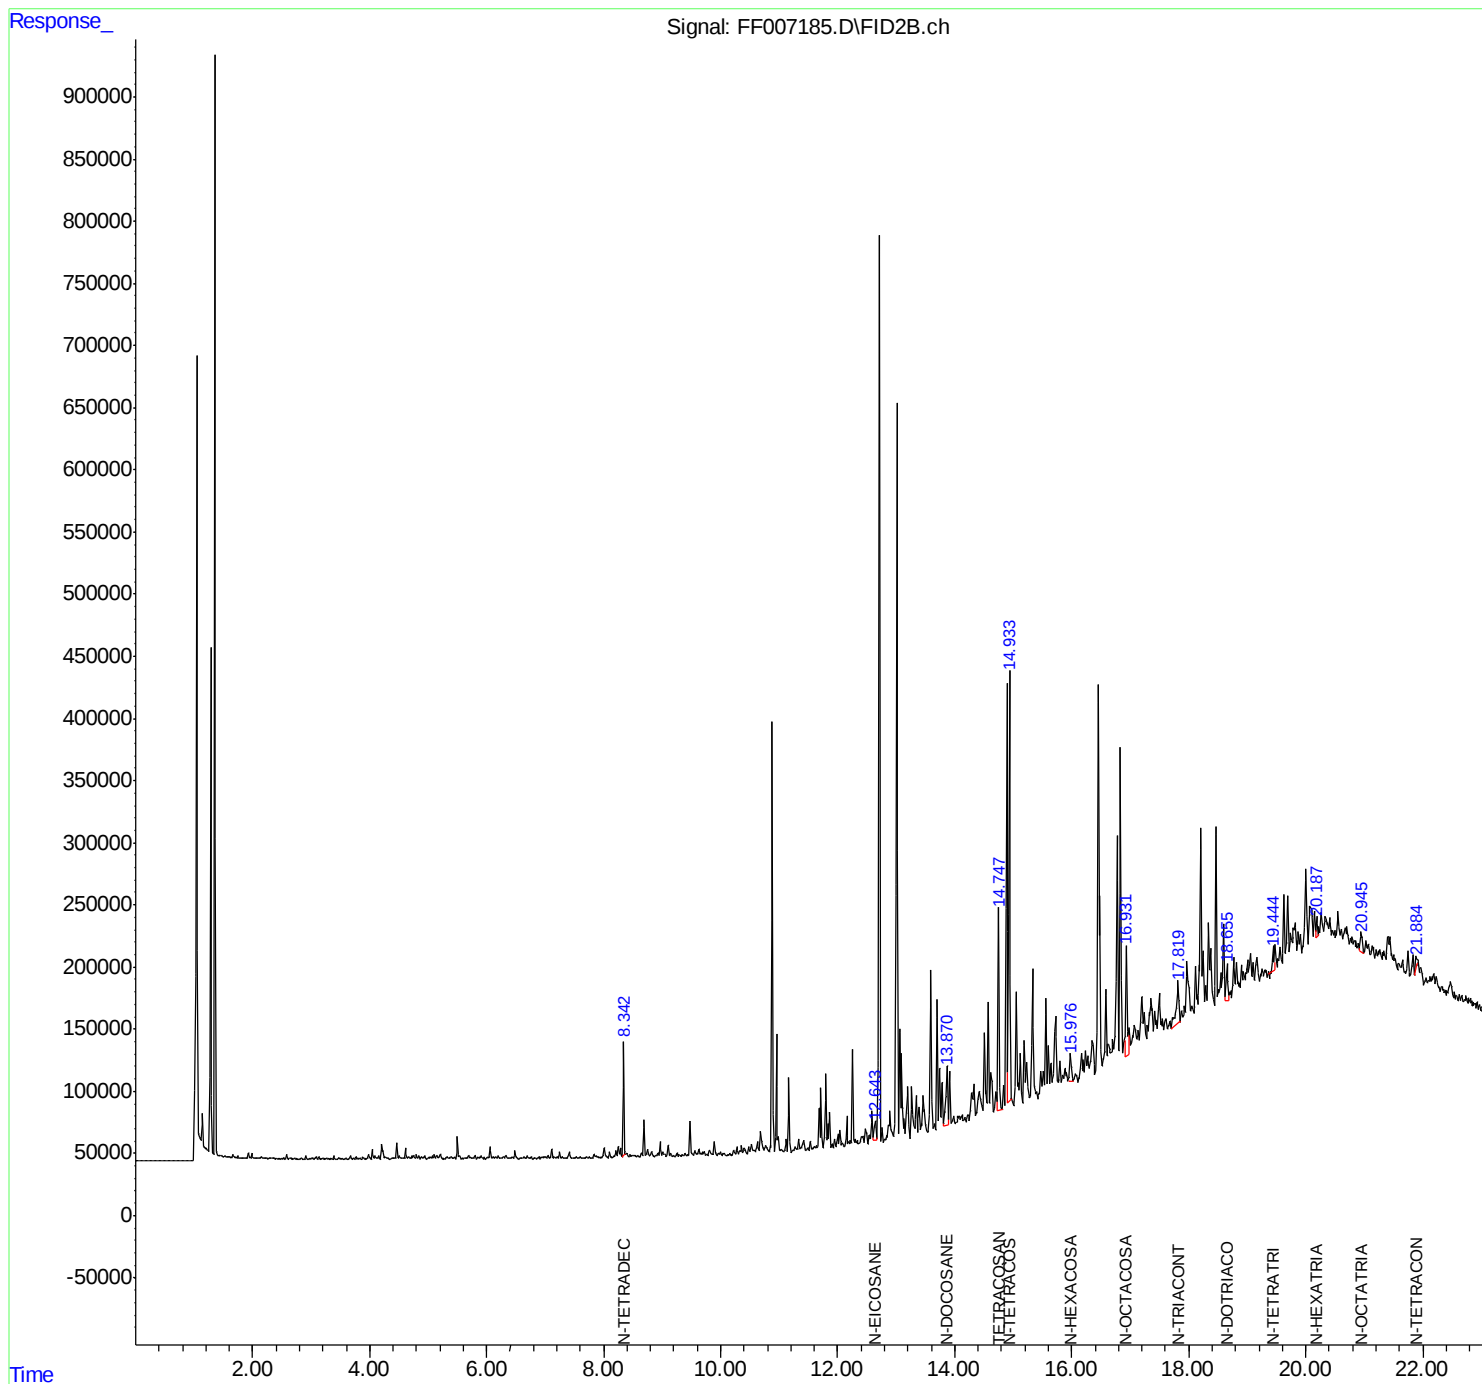


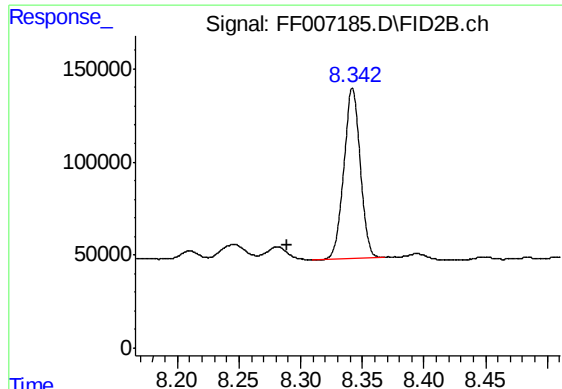

#4 N-TETRADECANE


R.T.: 8.342 min
Delta R.T.: 0.053 min
Response: 842283
Conc: 5.44 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1A

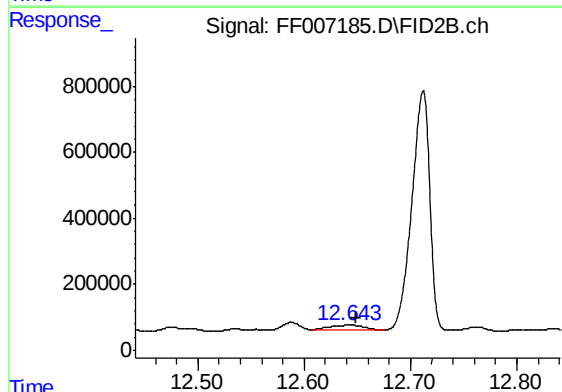


#7 N-EICOSANE

R.T.: 12.643 min
Delta R.T.: -0.007 min
Response: 362529
Conc: 2.24 ug/ml

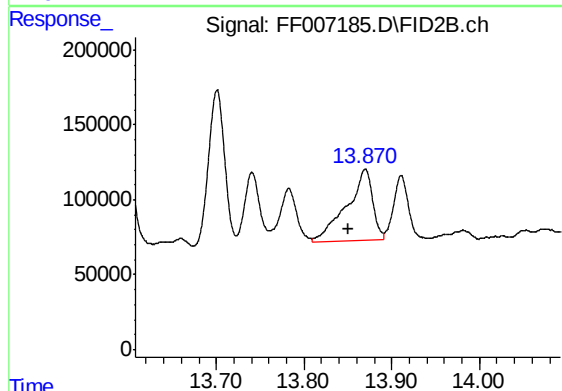


#8 N-DOCOSANE

R.T.: 13.870 min
Delta R.T.: 0.020 min
Response: 992173
Conc: 6.12 ug/ml

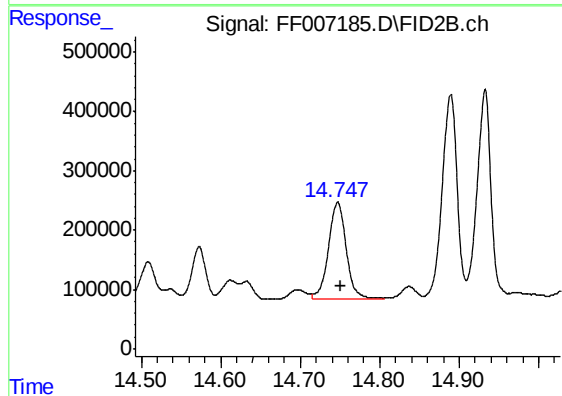

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.747 min
Delta R.T.: -0.003 min
Response: 2506680
Conc: 17.78 ug/ml

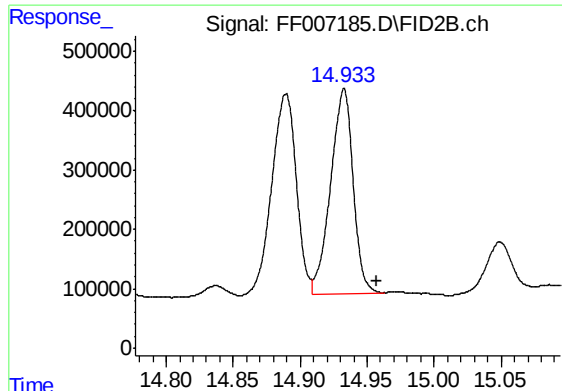

#10 N-TETRACOSANE


R.T.: 14.933 min
Delta R.T.: -0.024 min
Response: 4041328
Conc: 24.68 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1A

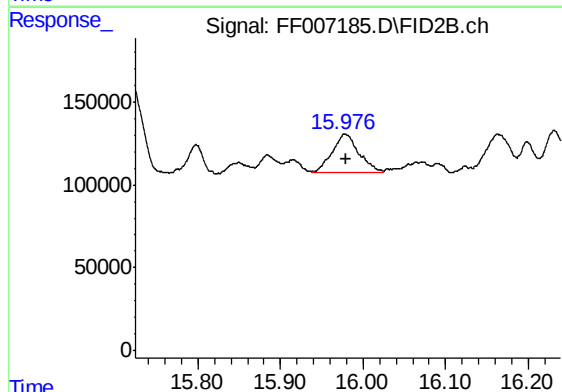


#11 N-HEXACOSANE

R.T.: 15.978 min
Delta R.T.: -0.001 min
Response: 507670
Conc: 3.12 ug/ml

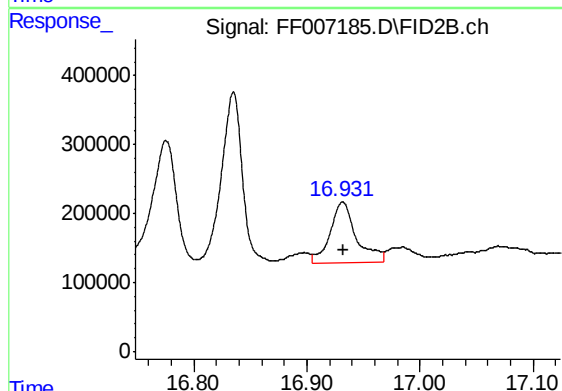


#12 N-OCTACOSANE

R.T.: 16.932 min
Delta R.T.: 0.000 min
Response: 1437836
Conc: 8.77 ug/ml

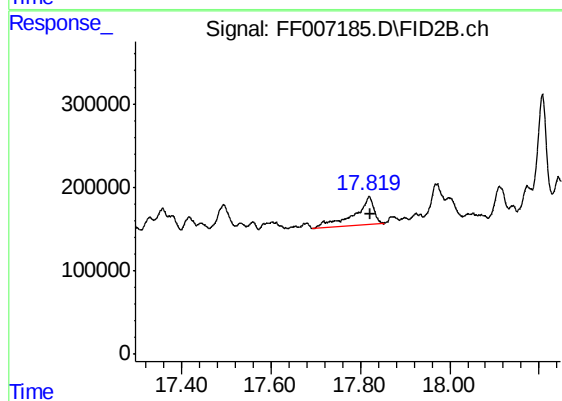

#13 N-TRIACONTANE


R.T.: 17.820 min
Delta R.T.: -0.002 min
Response: 1063016
Conc: 6.43 ug/ml

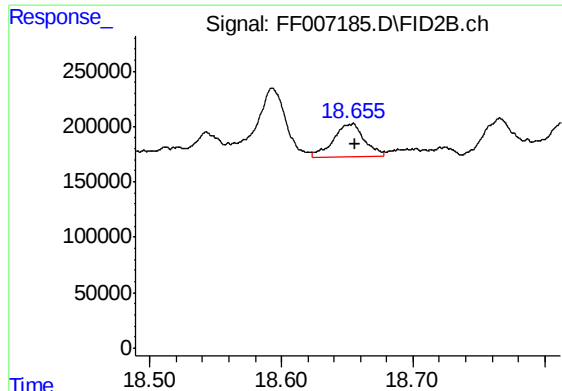

#14 N-DOTRIACONTANE


R.T.: 18.654 min
Delta R.T.: -0.002 min
Response: 478972
Conc: 3.05 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1A

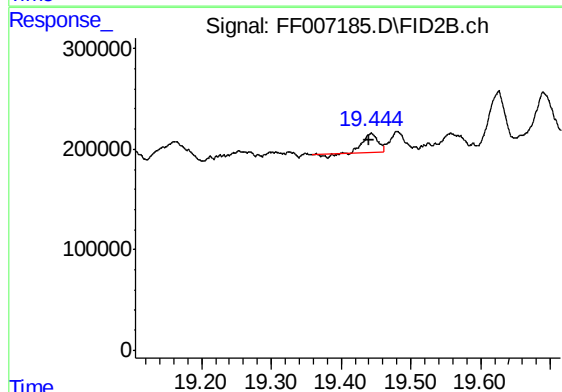


#15 N-TETRATRIACONTANE

R.T.: 19.444 min
Delta R.T.: 0.003 min
Response: 250507
Conc: 1.92 ug/ml

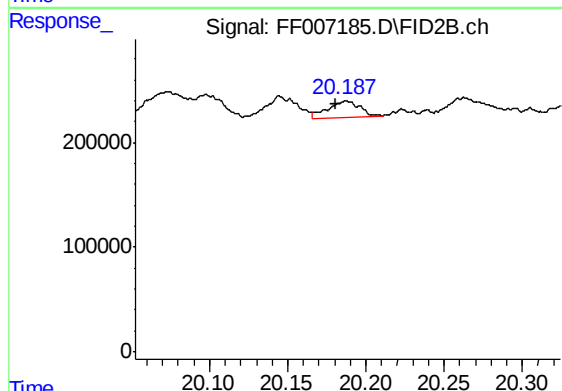


#16 N-HEXATRIACONTANE

R.T.: 20.188 min
Delta R.T.: 0.007 min
Response: 220105
Conc: 2.25 ug/ml

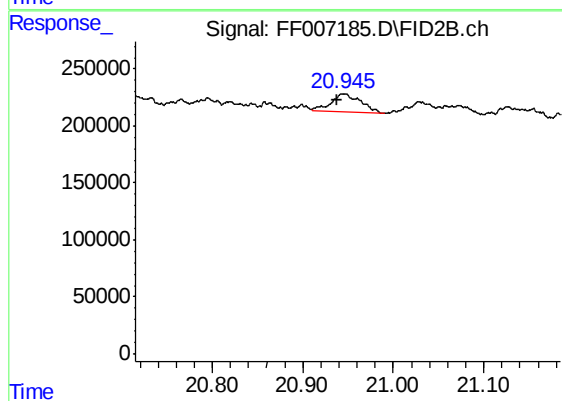

#17 N-OCTATRIACONTANE

R.T.: 20.945 min
Delta R.T.: 0.007 min
Response: 367155
Conc: 4.66 ug/ml

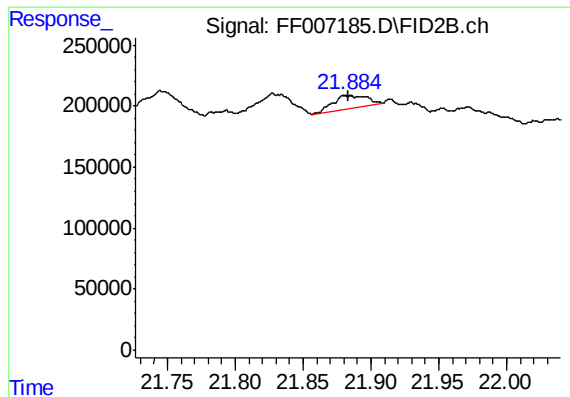

#18 N-TETRACONTANE

R.T.: 21.884 min
Delta R.T.: 0.000 min
Response: 177505
Conc: 2.48 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1A