

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
 Data File : FF007186.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jul 2020 15:48
 Operator : DD\AJ
 Sample : L3360-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SP-1B

Integration File: autoint1.e
 Quant Time: Jul 22 01:12:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	2170383	15.395 ug/ml
Target Compounds			
4) N-TETRADECANE	8.345f	692695	4.474 ug/ml
7) N-EICOSANE	12.591f	144417	0.894 ug/ml
8) N-DOCOSANE	13.850	218421	1.347 ug/ml
10) N-TETRACOSANE	14.933	2001476	12.221 ug/ml
11) N-HEXACOSANE	15.980	433575	2.666 ug/ml
12) N-OCTACOSANE	16.935	955774	5.833 ug/ml
13) N-TRIACONTANE	17.827	1025062	6.201 ug/ml
14) N-DOTRIACONTANE	18.658	531978	3.387 ug/ml
15) N-TETRATRIACONTANE	19.448	516996	3.971 ug/ml
16) N-HEXATRIACONTANE	20.185	298860	3.059 ug/ml
17) N-OCTATRIACONTANE	20.957	206477	2.618 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
Data File : FF07186.D
Signal(s) : FID2B.ch
Acq On : 21 Jul 2020 15:48
Operator : DD\AJ
Sample : L3360-02
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP-1B

Integration File: autoint1.e
Quant Time: Jul 22 01:12:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

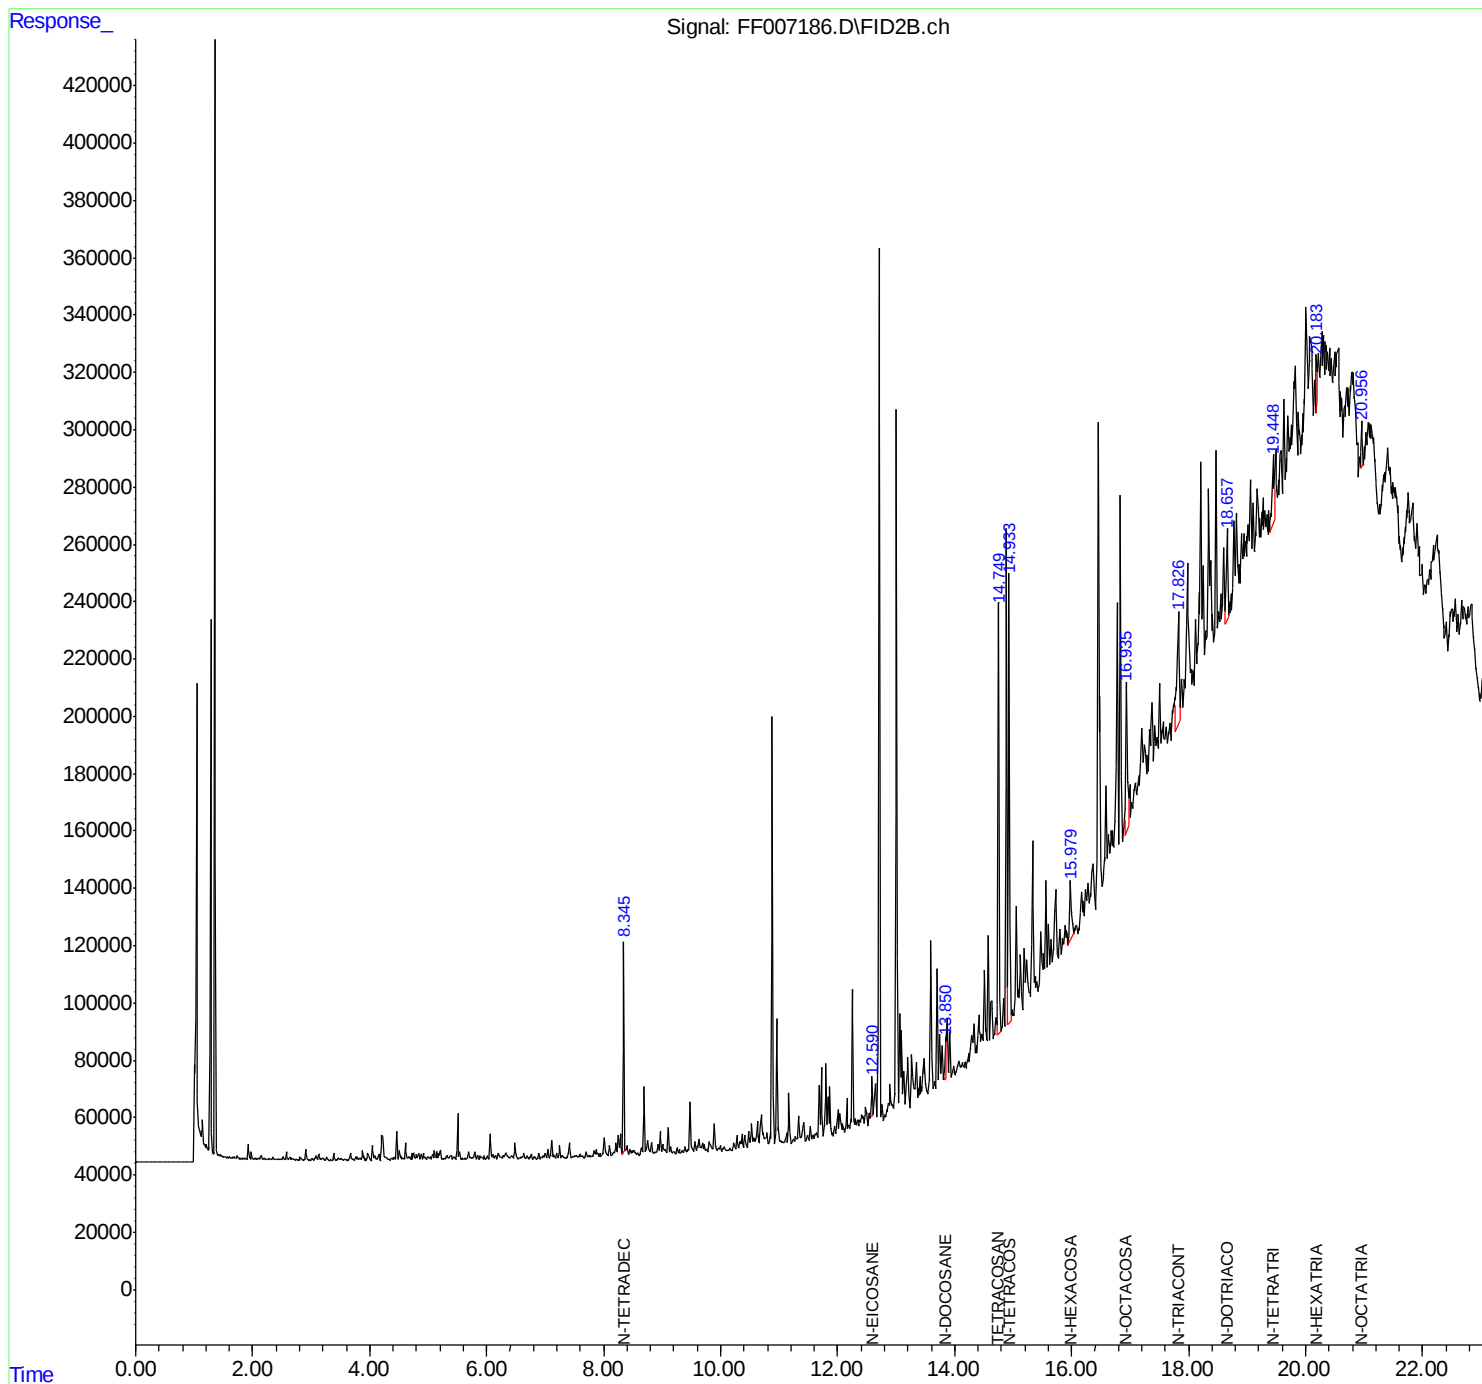


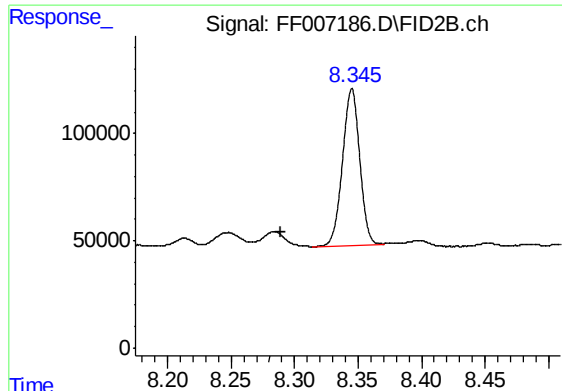

#4 N-TETRADECANE


R.T.: 8.345 min
Delta R.T.: 0.056 min
Response: 692695
Conc: 4.47 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1B

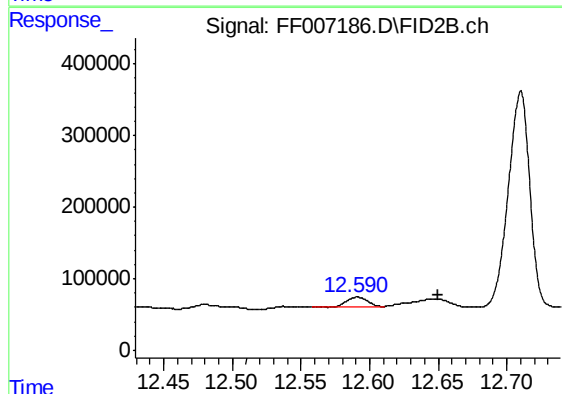


#7 N-EICOSANE

R.T.: 12.591 min
Delta R.T.: -0.058 min
Response: 144417
Conc: 0.89 ug/ml

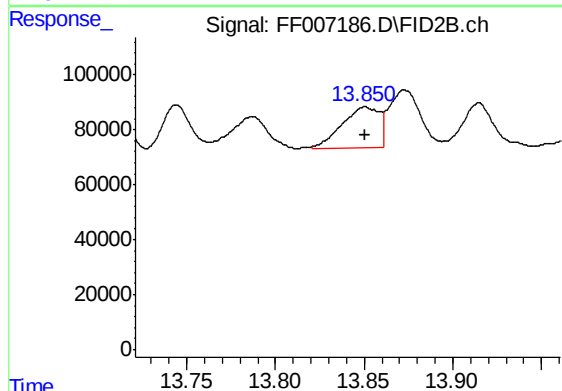


#8 N-DOCOSANE

R.T.: 13.850 min
Delta R.T.: 0.000 min
Response: 218421
Conc: 1.35 ug/ml

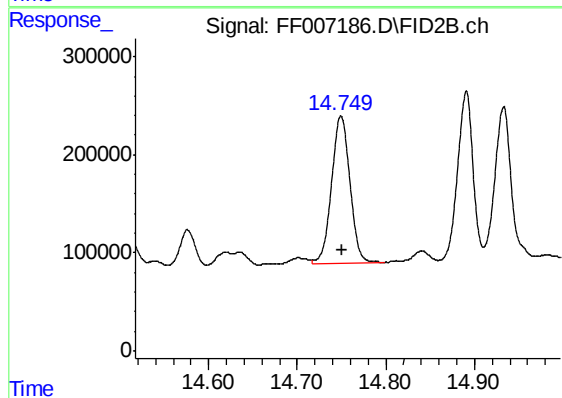

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.749 min
Delta R.T.: -0.001 min
Response: 2170383
Conc: 15.40 ug/ml

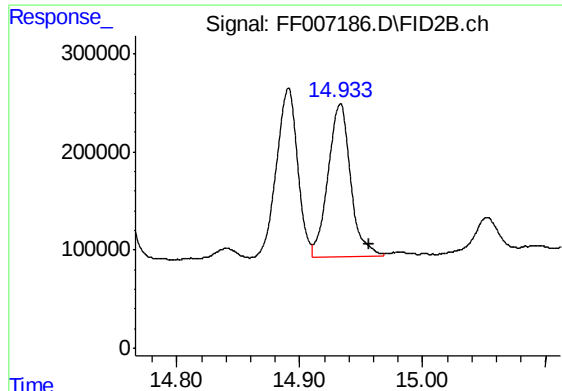

#10 N-TETRACOSANE


R.T.: 14.933 min
Delta R.T.: -0.024 min
Response: 2001476
Conc: 12.22 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1B

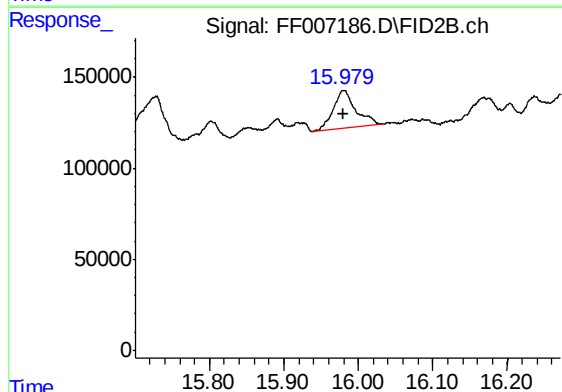


#11 N-HEXACOSANE

R.T.: 15.980 min
Delta R.T.: 0.000 min
Response: 433575
Conc: 2.67 ug/ml

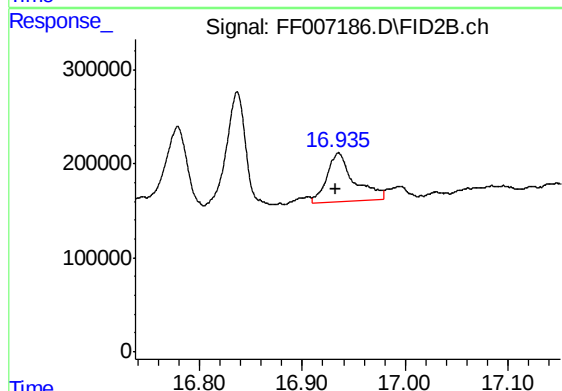


#12 N-OCTACOSANE

R.T.: 16.935 min
Delta R.T.: 0.003 min
Response: 955774
Conc: 5.83 ug/ml

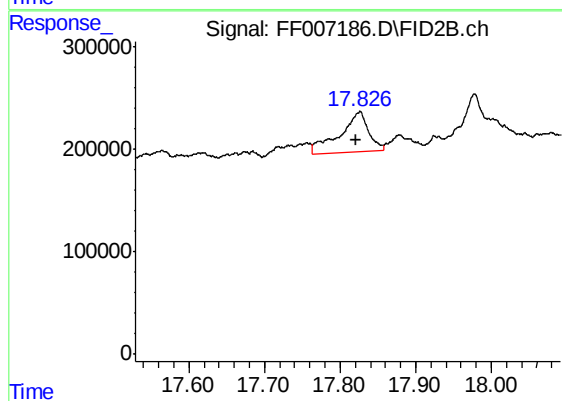

#13 N-TRIACONTANE


R.T.: 17.827 min
Delta R.T.: 0.004 min
Response: 1025062
Conc: 6.20 ug/ml

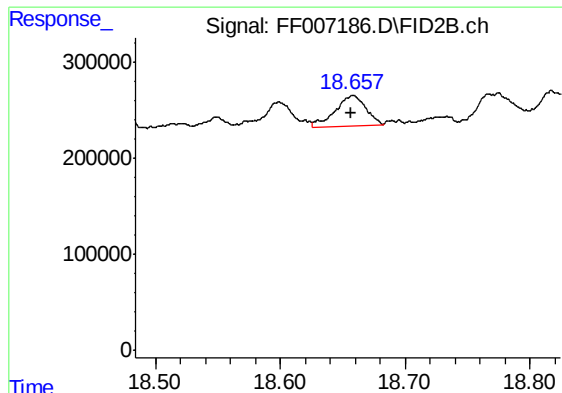

#14 N-DOTRIACONTANE


R.T.: 18.658 min
Delta R.T.: 0.002 min
Response: 531978
Conc: 3.39 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1B

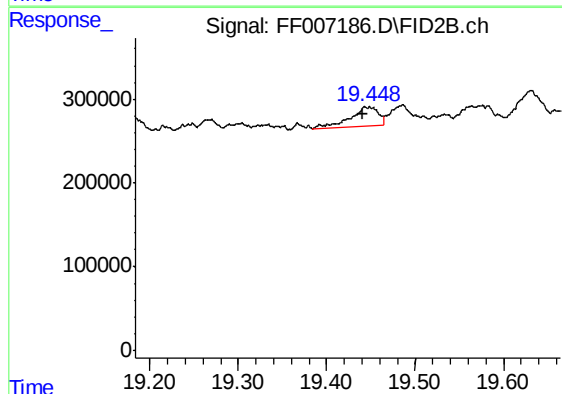


#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: 0.008 min
Response: 516996
Conc: 3.97 ug/ml

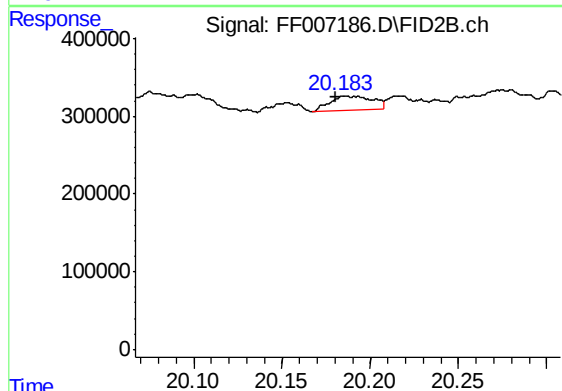

#16 N-HEXATRIACONTANE

R.T.: 20.185 min
Delta R.T.: 0.005 min
Response: 298860
Conc: 3.06 ug/ml

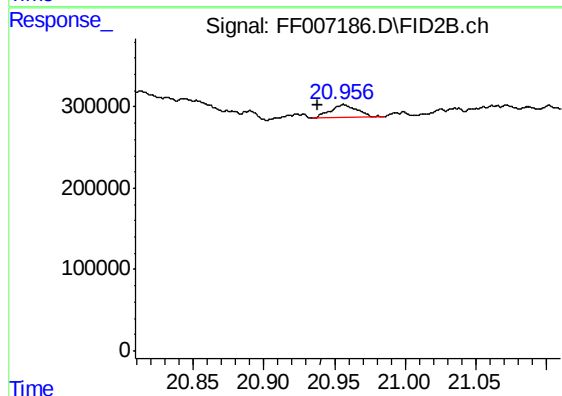

#17 N-OCTATRIACONTANE

R.T.: 20.957 min
Delta R.T.: 0.019 min
Response: 206477
Conc: 2.62 ug/ml