

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
 Data File : FF007191.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jul 2020 18:25
 Operator : DD\AJ
 Sample : L3360-01 5X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SP-1A

Integration File: autoint1.e
 Quant Time: Jul 22 01:13:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	471539	3.345 ug/ml
Target Compounds			
4) N-TETRADECANE	8.347f	148609	0.960 ug/ml
7) N-EICOSANE	12.712f	1521586	9.422 ug/ml
10) N-TETRACOSANE	14.934	755357	4.612 ug/ml
12) N-OCTACOSANE	16.937	225076	1.374 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
Data File : FF07191.D
Signal(s) : FID2B.ch
Acq On : 21 Jul 2020 18:25
Operator : DD\AJ
Sample : L3360-01 5X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP-1A

Integration File: autoint1.e
Quant Time: Jul 22 01:13:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

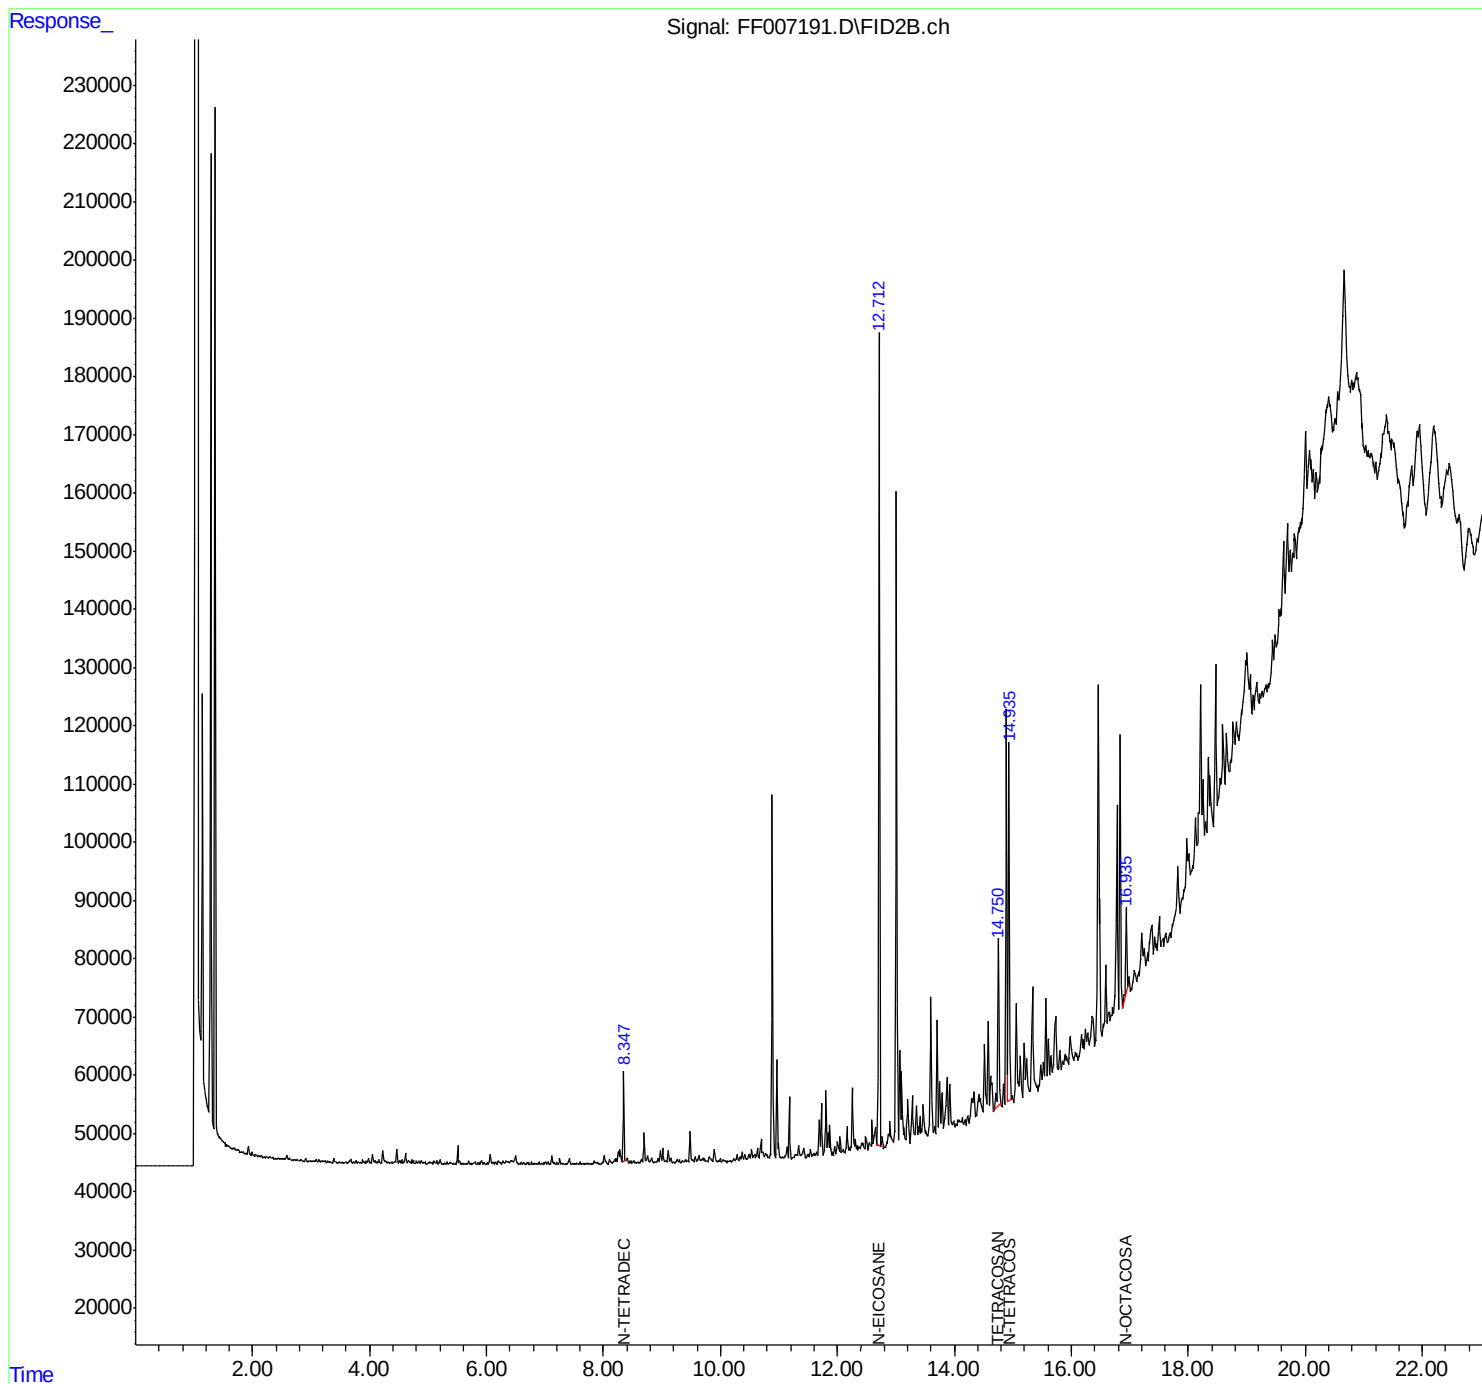


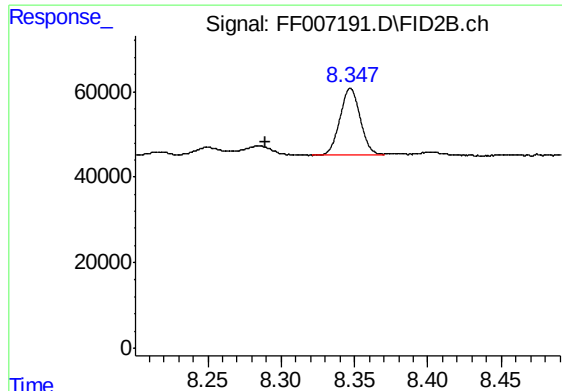

#4 N-TETRADECANE


R.T.: 8.347 min
Delta R.T.: 0.058 min
Response: 148609
Conc: 0.96 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1A

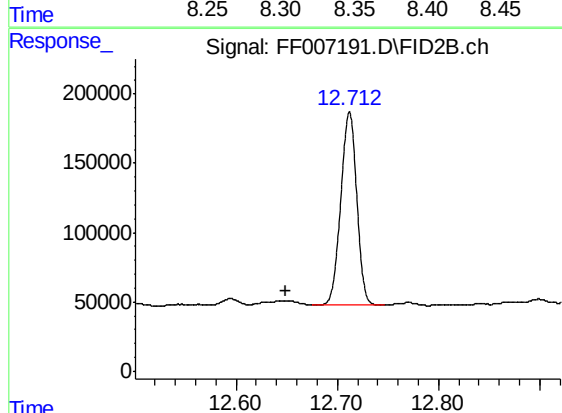


#7 N-EICOSANE

R.T.: 12.712 min
Delta R.T.: 0.063 min
Response: 1521586
Conc: 9.42 ug/ml

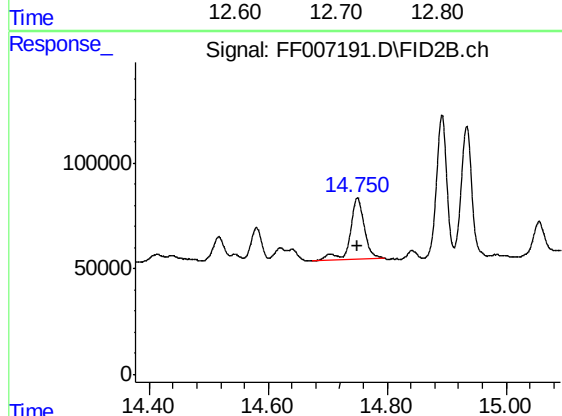


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: 0.000 min
Response: 471539
Conc: 3.34 ug/ml

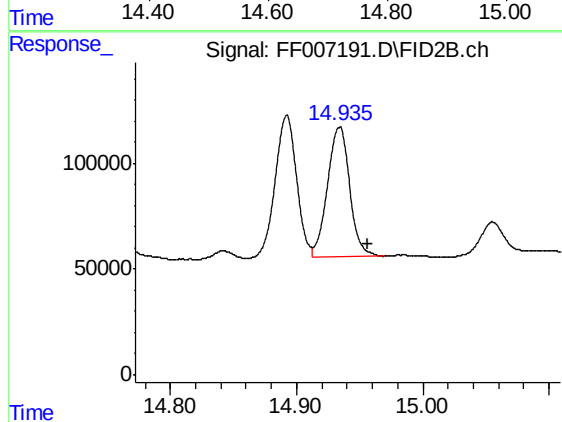

#10 N-TETRACOSANE

R.T.: 14.934 min
Delta R.T.: -0.023 min
Response: 755357
Conc: 4.61 ug/ml

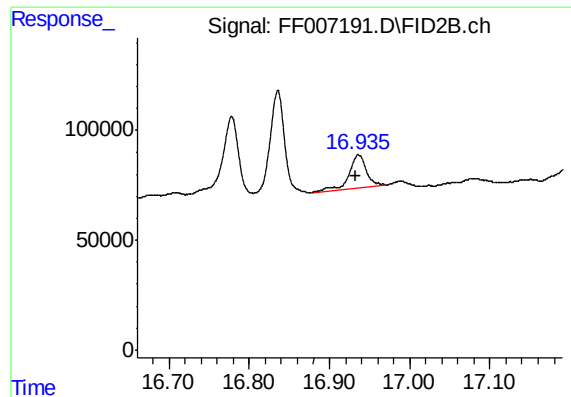

#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: 0.004 min
Response: 225076
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1A