

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
 Data File : FF007192.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jul 2020 18:56
 Operator : DD\AJ
 Sample : L3360-02 5X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SP-1B

Integration File: autoint1.e
 Quant Time: Jul 22 01:13:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	429418	3.046 ug/ml
Target Compounds			
4) N-TETRADECANE	8.347f	142315	0.919 ug/ml
7) N-EICOSANE	12.711f	672525	4.164 ug/ml
10) N-TETRACOSANE	14.933	400189	2.444 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072120\
Data File : FF07192.D
Signal(s) : FID2B.ch
Acq On : 21 Jul 2020 18:56
Operator : DD\AJ
Sample : L3360-02 5X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP-1B

Integration File: autoint1.e
Quant Time: Jul 22 01:13:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

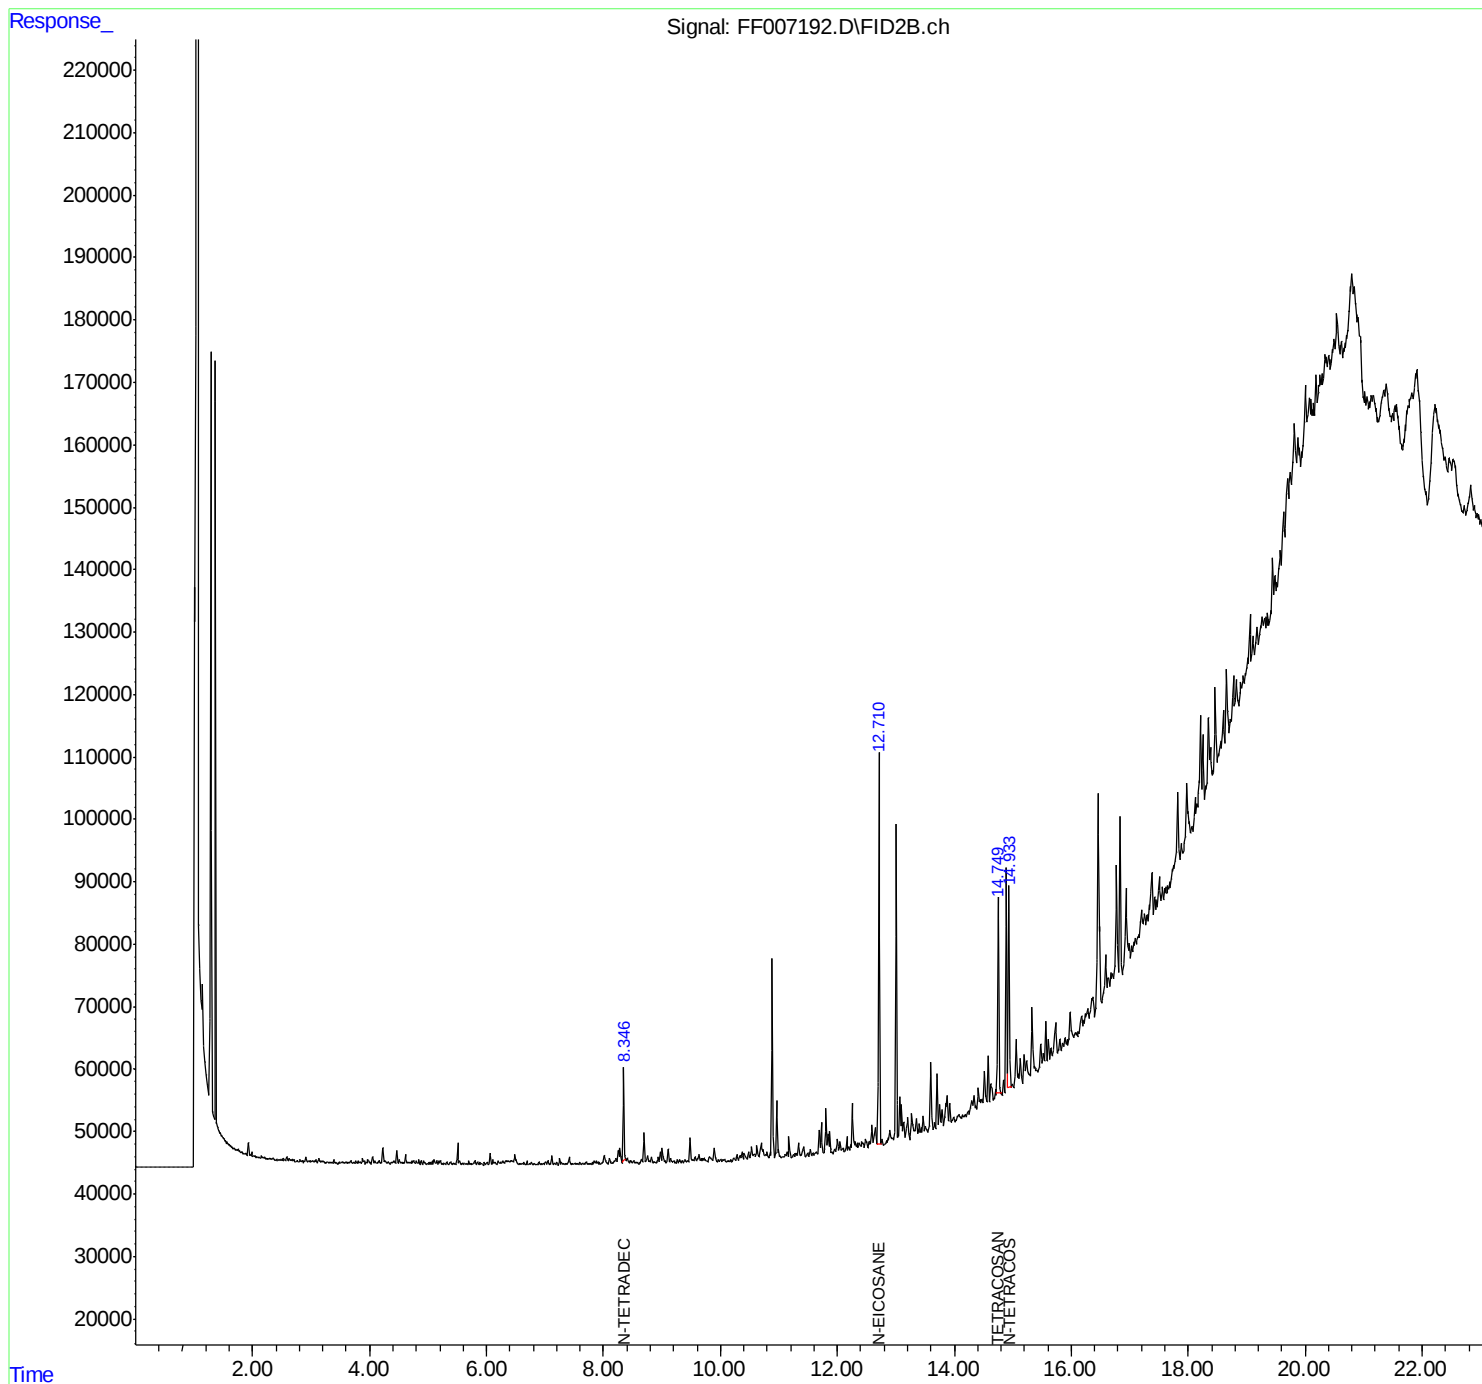


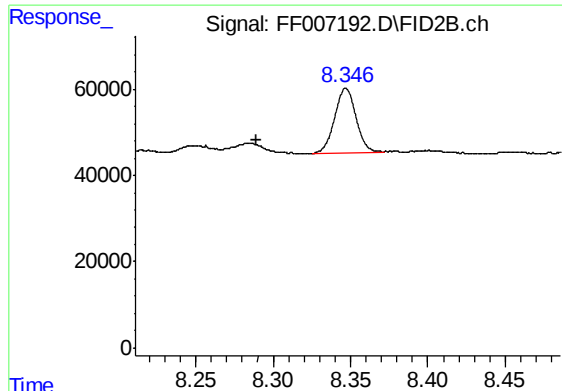

#4 N-TETRADECANE


R.T.: 8.347 min
Delta R.T.: 0.058 min
Response: 142315
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :
SP-1B

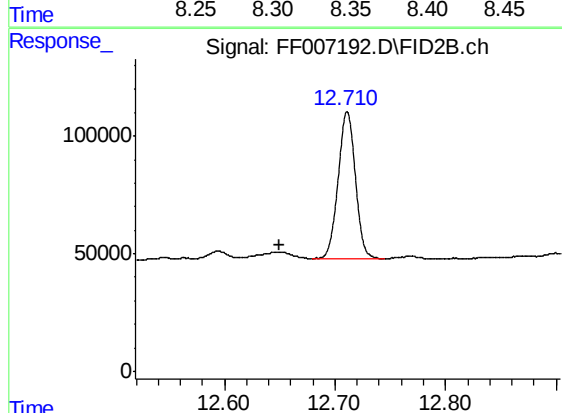


#7 N-EICOSANE

R.T.: 12.711 min
Delta R.T.: 0.061 min
Response: 672525
Conc: 4.16 ug/ml

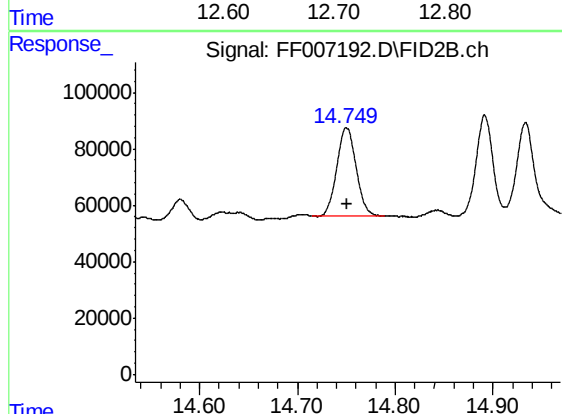

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: 0.000 min
Response: 429418
Conc: 3.05 ug/ml

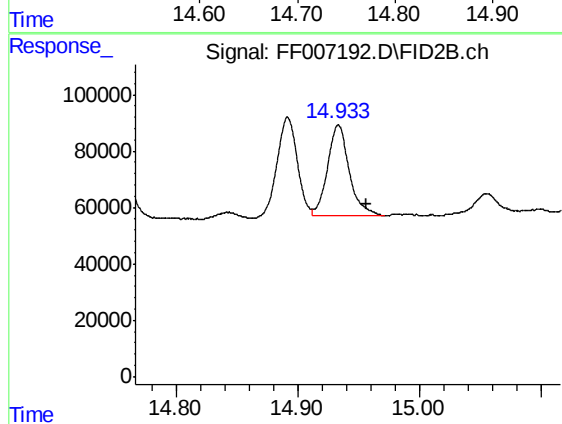

#10 N-TETRACOSANE

R.T.: 14.933 min
Delta R.T.: -0.023 min
Response: 400189
Conc: 2.44 ug/ml