

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072121\
 Data File : FF008864.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jul 2021 18:50
 Operator : DD\AJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 22 01:34:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:33:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	5865688	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.395	6292450	50.000 ug/ml
2) N-DECANE	4.504	6419595	50.000 ug/ml
3) N-DODECANE	6.520	6552120	50.000 ug/ml
4) N-TETRADECANE	8.310	6688012	50.000 ug/ml
5) N-HEXADECANE	9.908	6722877	50.000 ug/ml
6) N-OCTADECANE	11.347	6892647	50.000 ug/ml
7) N-EICOSANE	12.653	6863225	50.000 ug/ml
8) N-DOCOSANE	13.847	6785928	50.000 ug/ml
10) N-TETRACOSANE	14.951	6782122	50.000 ug/ml
11) N-HEXACOSANE	15.970	6665902	50.000 ug/ml
12) N-OCTACOSANE	16.918	6530351	50.000 ug/ml
13) N-TRIACONTANE	17.804	6366178	50.000 ug/ml
14) N-DOTRIACONTANE	18.634	6039350	50.000 ug/ml
15) N-TETRATRIACONTANE	19.414	5717918	50.000 ug/ml
16) N-HEXATRIACONTANE	20.150	5242220	50.000 ug/ml
17) N-OCTATRIACONTANE	20.893	4804024	50.000 ug/ml
18) N-TETRACONTANE	21.823	4812252	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072121\
 Data File : FF008864.D
 Signal(s) : FID2B.ch
 Acq On : 21 Jul 2021 18:50
 Operator : DD\AJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1


Integration File: autoint1.e
 Quant Time: Jul 22 01:34:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:33:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

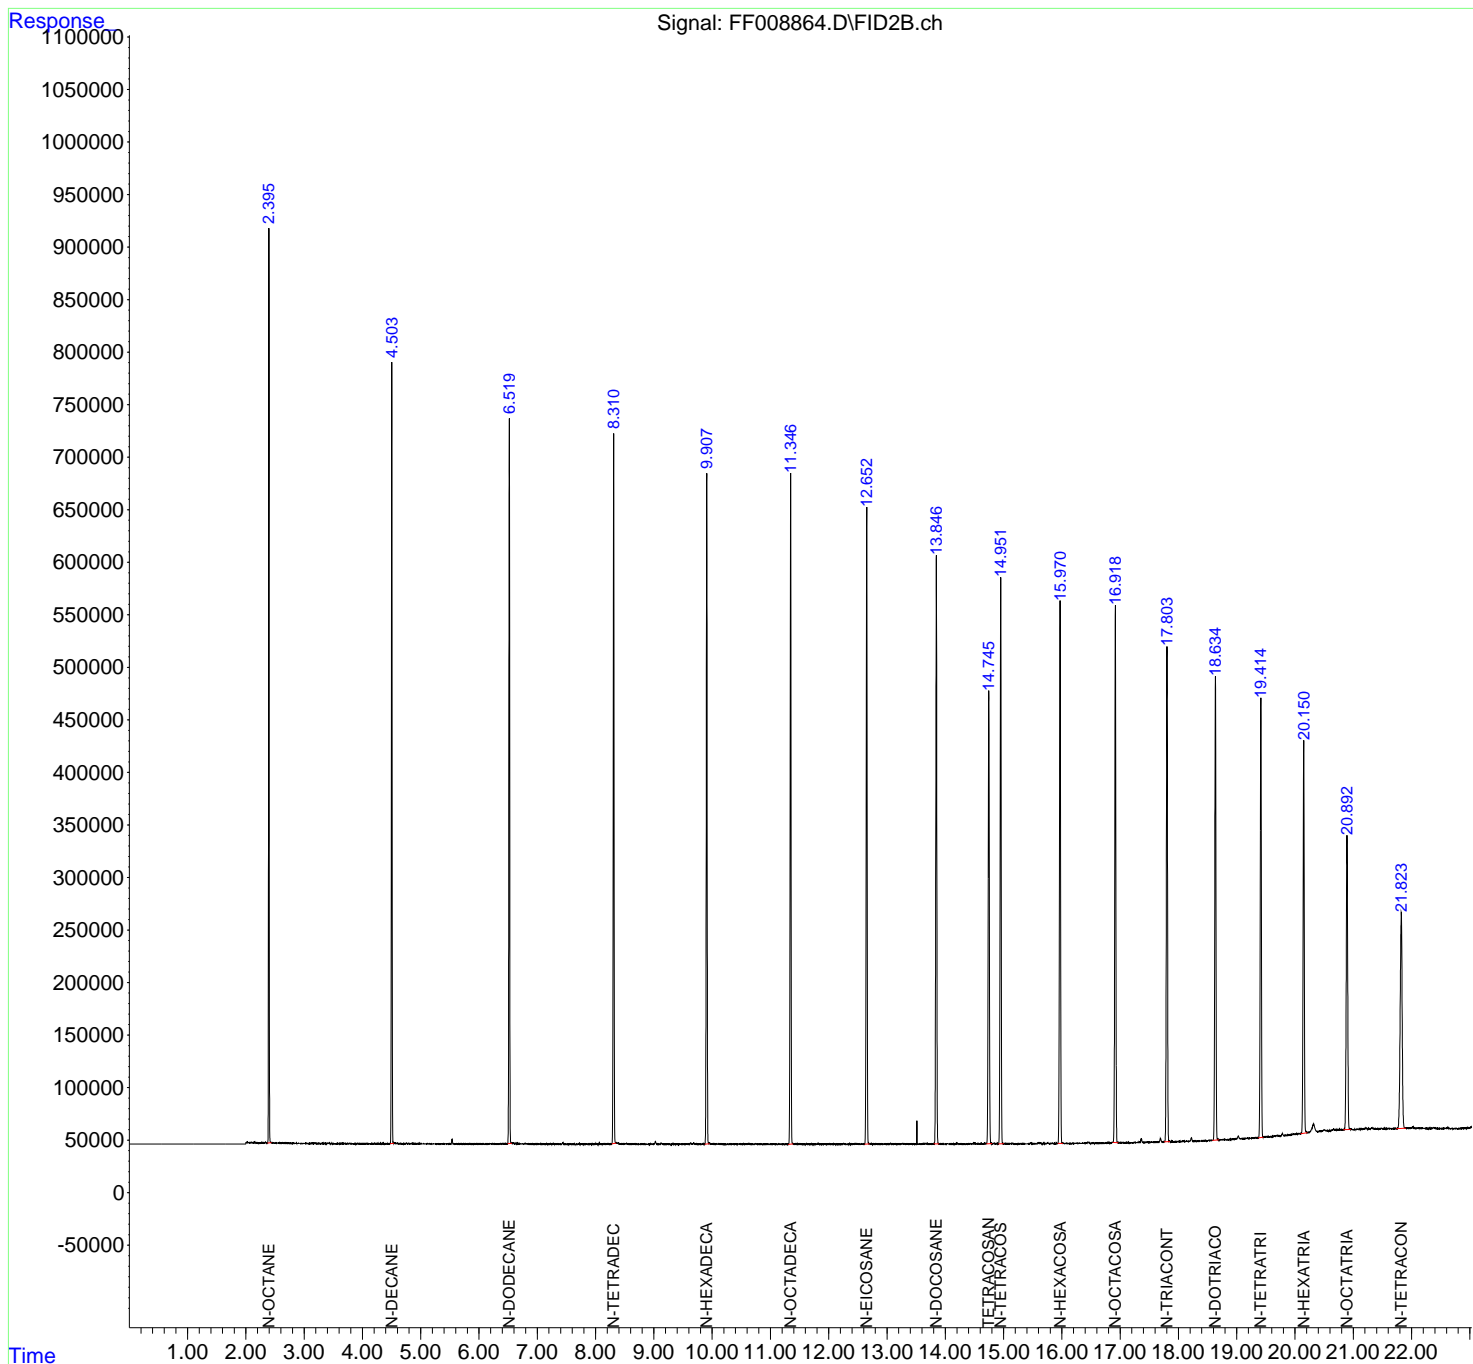


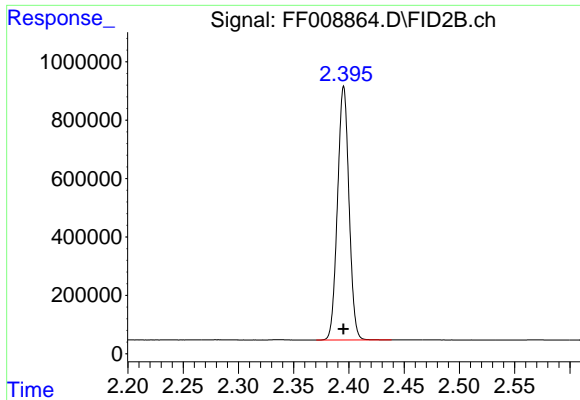


#1 N-OCTANE
R.T.: 2.395 min
Delta R.T.: 0.000 min
Response: 6292450
Conc: 50.00 ug/ml

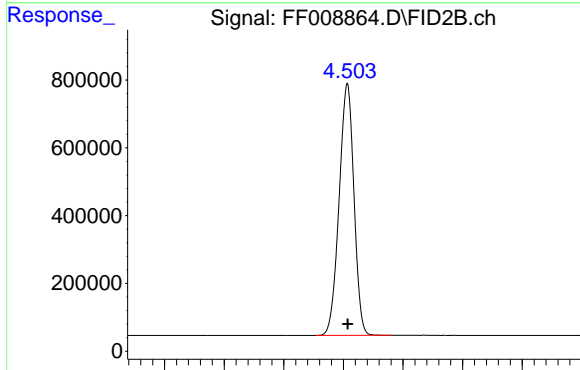


#2 N-DECANE
R.T.: 4.504 min
Delta R.T.: 0.000 min
Response: 6419595
Conc: 50.00 ug/ml

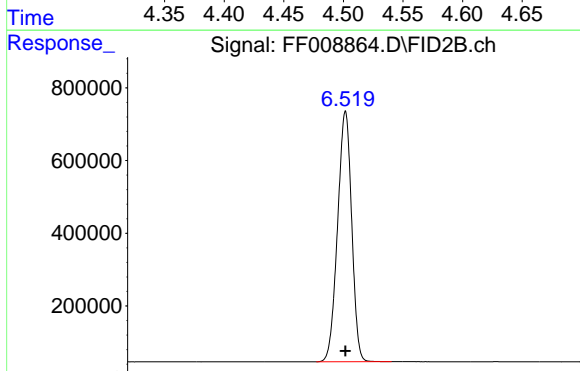


#3 N-DODECANE
R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 6552120
Conc: 50.00 ug/ml

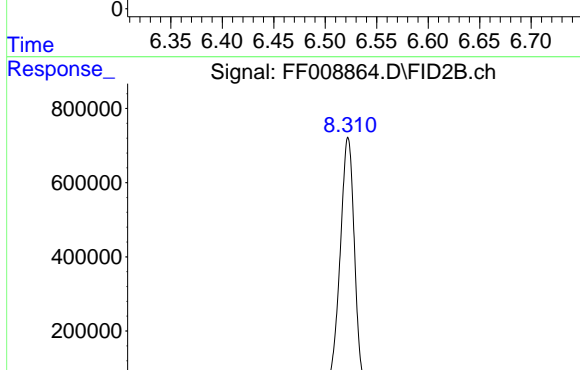


#4 N-TETRADECANE
R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 6688012
Conc: 50.00 ug/ml

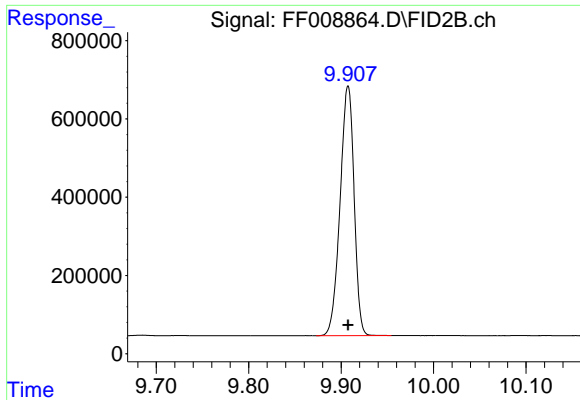


#5 N-HEXADECANE
R.T.: 9.908 min
Delta R.T.: 0.000 min
Response: 6722877
Conc: 50.00 ug/ml

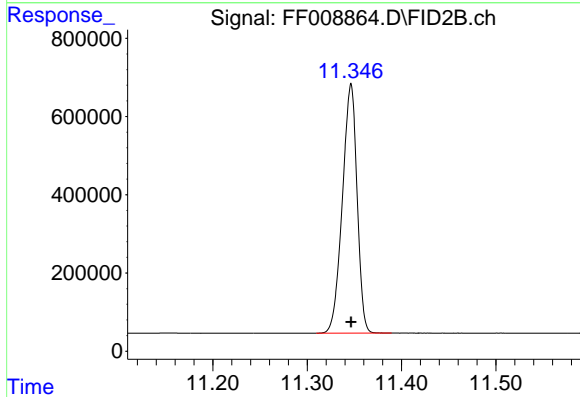


#6 N-OCTADECANE
R.T.: 11.347 min
Delta R.T.: 0.000 min
Response: 6892647
Conc: 50.00 ug/ml

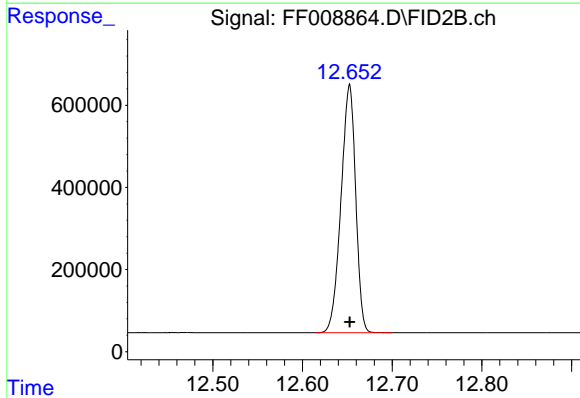

#7 N-EICOSANE
R.T.: 12.653 min
Delta R.T.: 0.000 min
Response: 6863225
Conc: 50.00 ug/ml

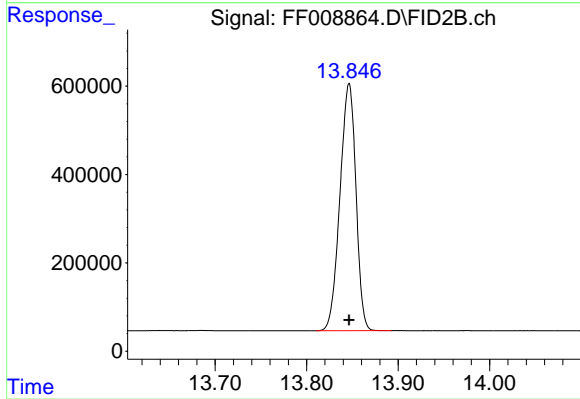


#8 N-DOCOSANE
R.T.: 13.847 min
Delta R.T.: 0.000 min
Response: 6785928
Conc: 50.00 ug/ml

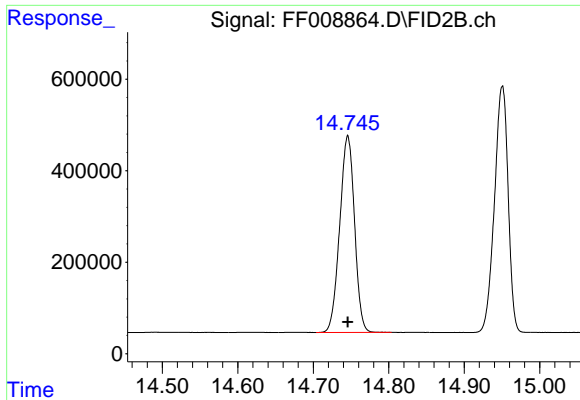


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.746 min
Delta R.T.: 0.000 min
Response: 5865688
Conc: 50.00 ug/ml

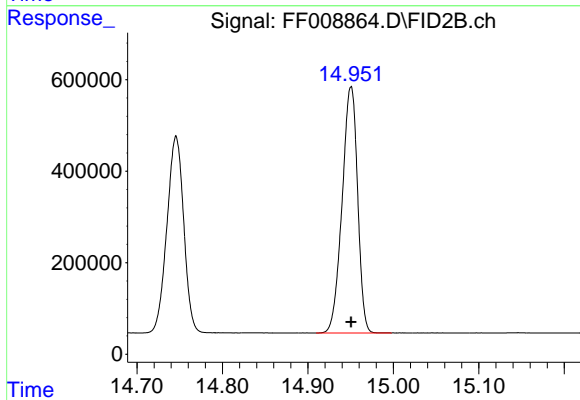


#10 N-TETRACOSANE

R.T.: 14.951 min
Delta R.T.: 0.000 min
Response: 6782122
Conc: 50.00 ug/ml

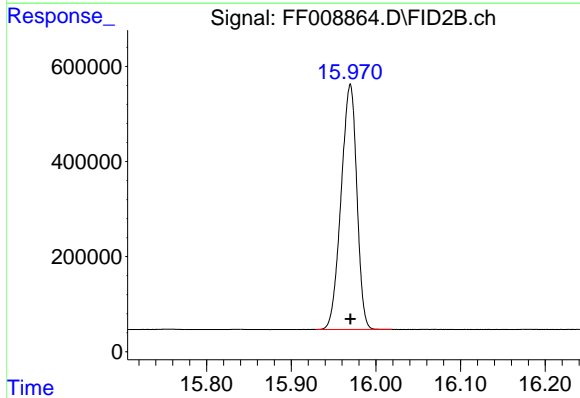


#11 N-HEXACOSANE

R.T.: 15.970 min
Delta R.T.: 0.000 min
Response: 6665902
Conc: 50.00 ug/ml

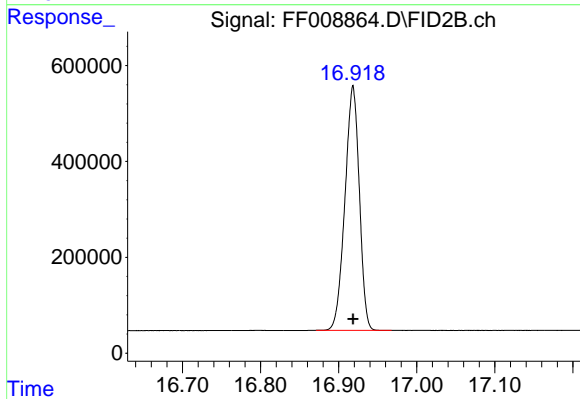


#12 N-OCTACOSANE


R.T.: 16.918 min
Delta R.T.: 0.000 min
Response: 6530351
Conc: 50.00 ug/ml

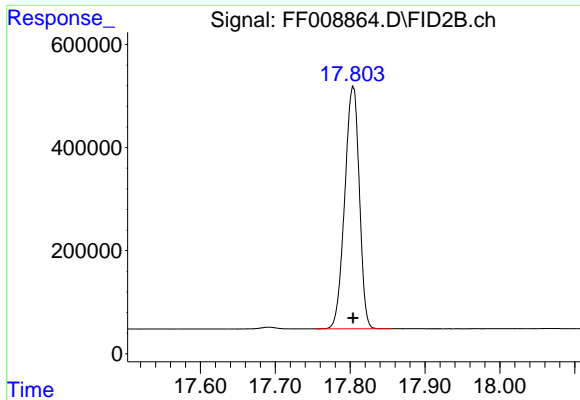


#13 N-TRIACONTANE
R.T.: 17.804 min
Delta R.T.: 0.000 min
Response: 6366178
Conc: 50.00 ug/ml

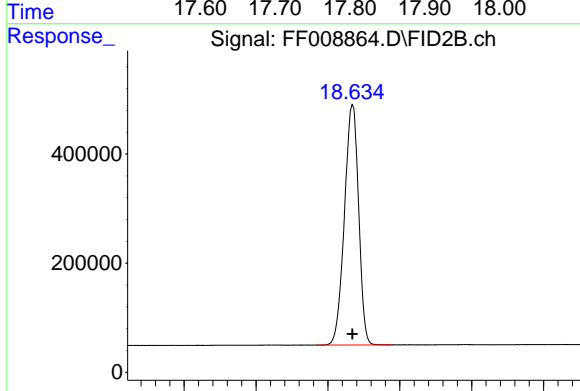


#14 N-DOTRIACONTANE
R.T.: 18.634 min
Delta R.T.: 0.000 min
Response: 6039350
Conc: 50.00 ug/ml

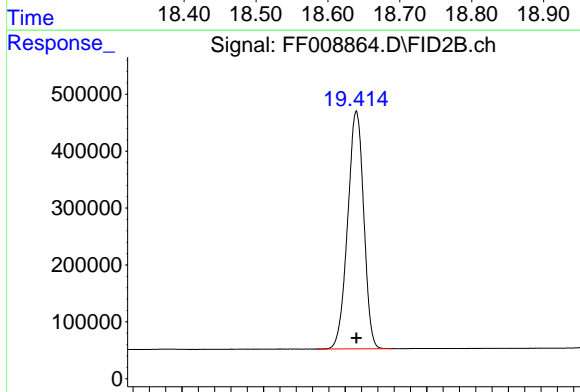


#15 N-TETRATRIACONTANE
R.T.: 19.414 min
Delta R.T.: 0.000 min
Response: 5717918
Conc: 50.00 ug/ml

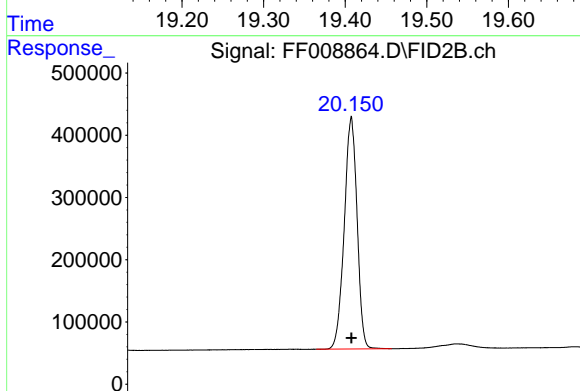

#16 N-HEXATRIACONTANE
R.T.: 20.150 min
Delta R.T.: 0.000 min
Response: 5242220
Conc: 50.00 ug/ml

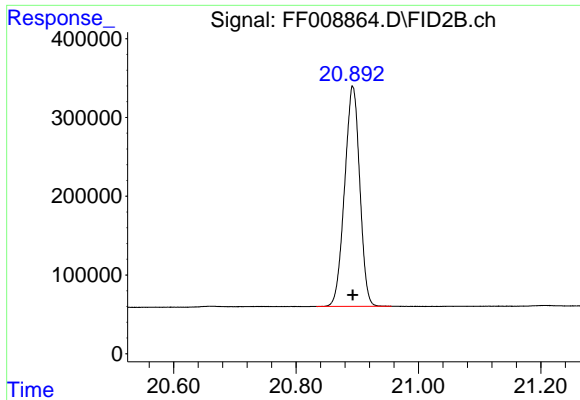

#17 N-OCTATRIACONTANE
R.T.: 20.893 min
Delta R.T.: 0.000 min
Response: 4804024
Conc: 50.00 ug/ml

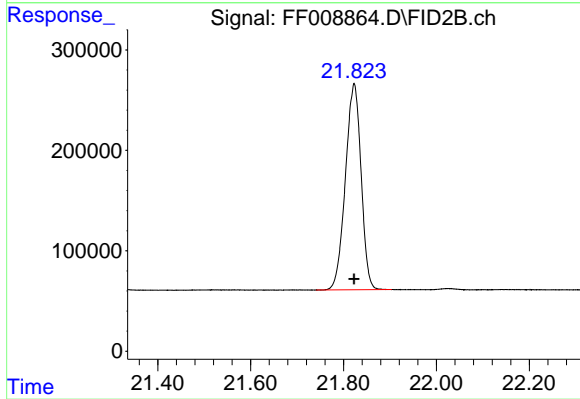

#18 N-TETRACONTANE
R.T.: 21.823 min
Delta R.T.: 0.000 min
Response: 4812252
Conc: 50.00 ug/ml