

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072219\
 Data File : FF005110.D
 Signal(s) : FID2B.ch
 Acq On : 22 Jul 2019 13:05
 Operator : DD\AJ
 Sample : PB121590BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 23 01:10:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.672	2223102	22.858 ug/ml
Target Compounds			
2) N-DECANE	4.386	2620350	20.750 ug/ml
3) N-DODECANE	6.409	2655056	20.925 ug/ml
4) N-TETRADECANE	8.204	2641188	21.108 ug/ml
5) N-HEXADECANE	9.807	2623689	21.248 ug/ml
6) N-OCTADECANE	11.252	2608564	22.019 ug/ml
7) N-EICOSANE	12.565	2592800	22.347 ug/ml
8) N-DOCOSANE	13.769	2584117	22.967 ug/ml
10) N-TETRACOSANE	14.877	2621086	23.547 ug/ml
11) N-HEXACOSANE	15.903	2617547	23.666 ug/ml
12) N-OCTACOSANE	16.859	2665763	23.900 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072219\
Data File : FF005110.D
Signal(s) : FID2B.ch
Acq On : 22 Jul 2019 13:05
Operator : DD\AJ
Sample : PB121590BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 23 01:10:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

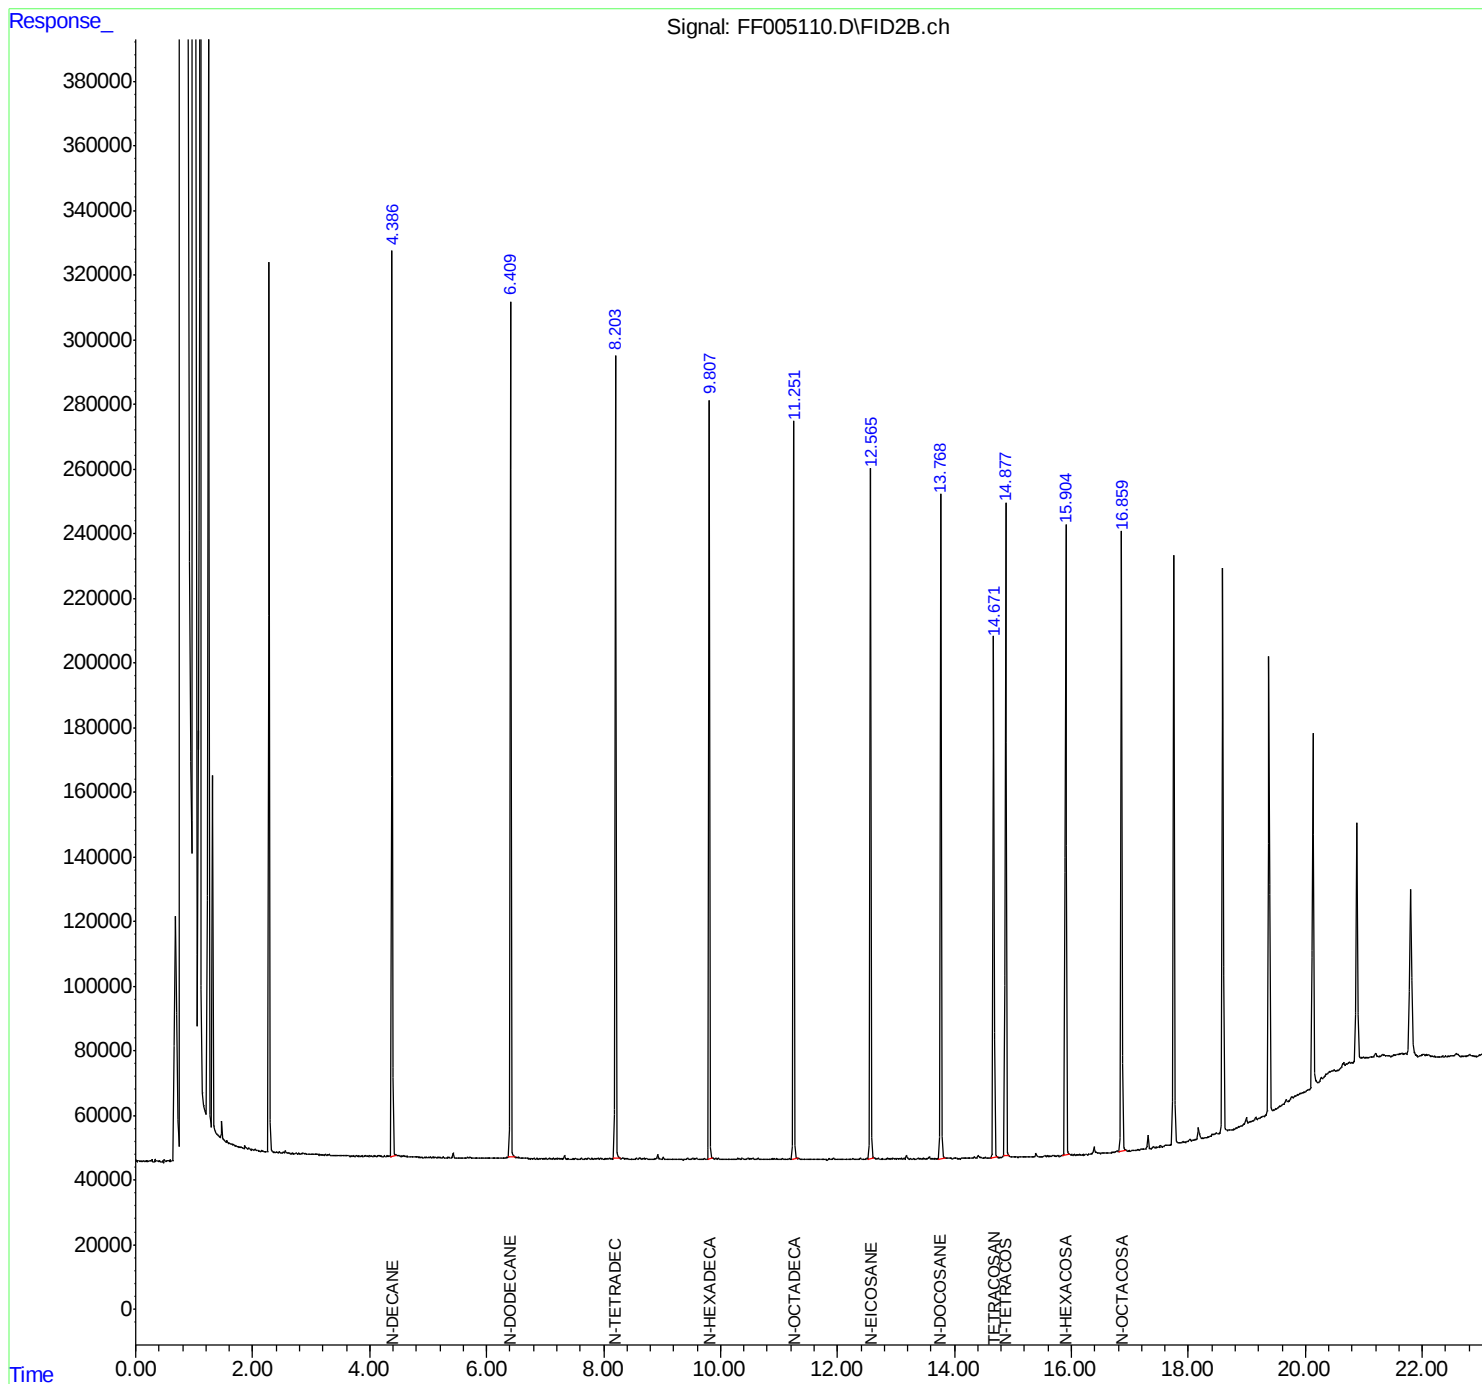

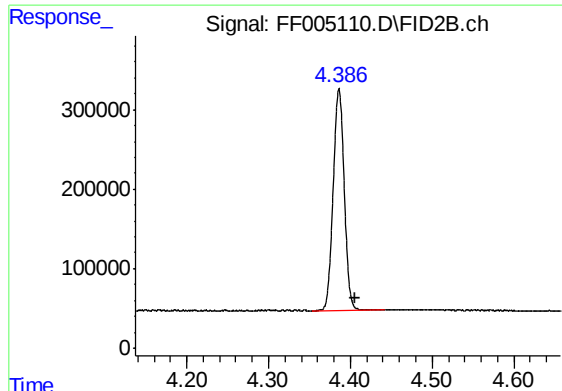


#2 N-DECANE

R.T.: 4.386 min
Delta R.T.: -0.020 min
Response: 2620350
Conc: 20.75 ug/ml

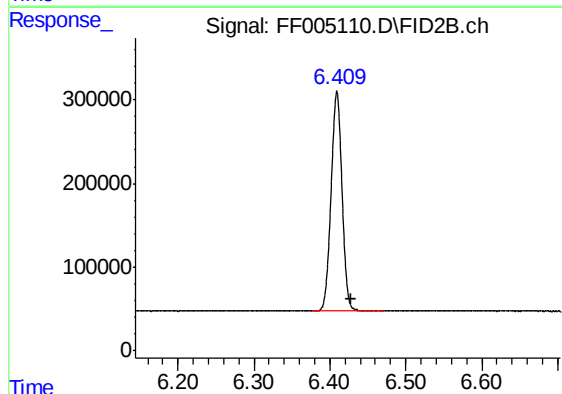


#3 N-DODECANE

R.T.: 6.409 min
Delta R.T.: -0.019 min
Response: 2655056
Conc: 20.93 ug/ml

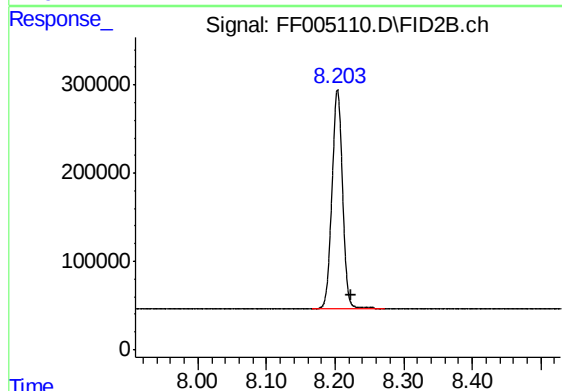


#4 N-TETRADECANE

R.T.: 8.204 min
Delta R.T.: -0.020 min
Response: 2641188
Conc: 21.11 ug/ml

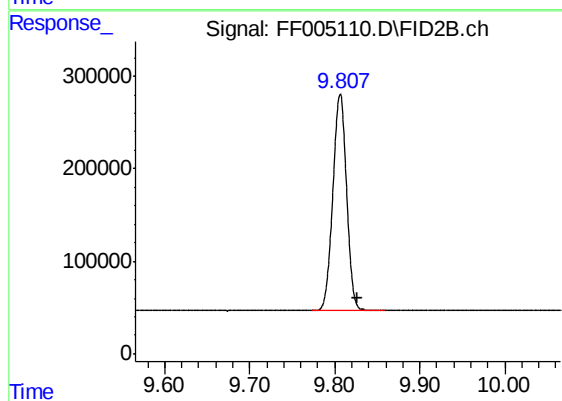


#5 N-HEXADECANE

R.T.: 9.807 min
Delta R.T.: -0.020 min
Response: 2623689
Conc: 21.25 ug/ml

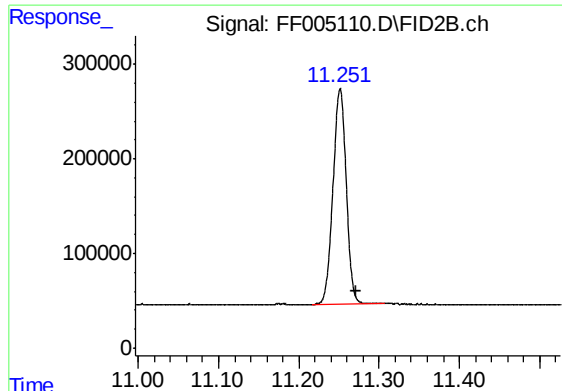


#6 N-OCTADECANE

R.T.: 11.252 min
Delta R.T.: -0.020 min
Response: 2608564
Conc: 22.02 ug/ml

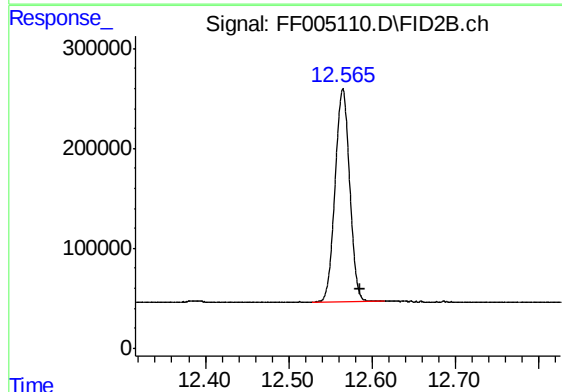


#7 N-EICOSANE

R.T.: 12.565 min
Delta R.T.: -0.020 min
Response: 2592800
Conc: 22.35 ug/ml

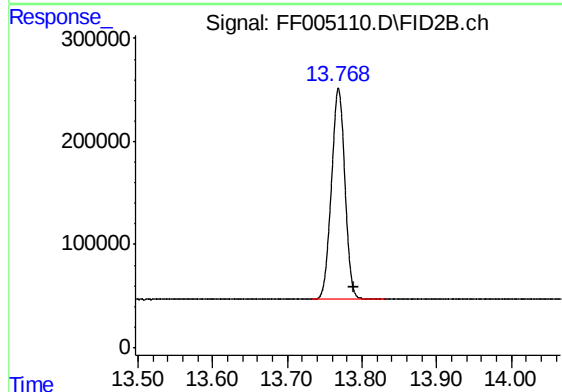


#8 N-DOCOSANE

R.T.: 13.769 min
Delta R.T.: -0.020 min
Response: 2584117
Conc: 22.97 ug/ml

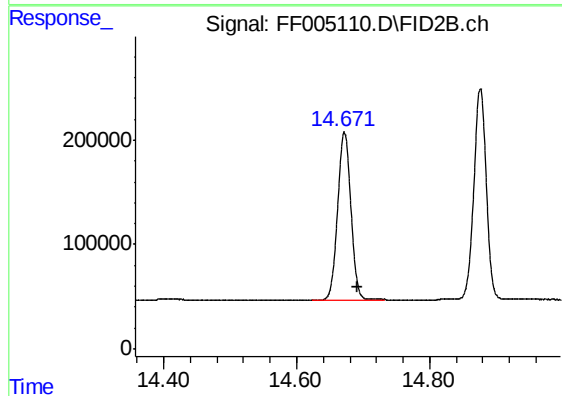


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.672 min
Delta R.T.: -0.020 min
Response: 2223102
Conc: 22.86 ug/ml

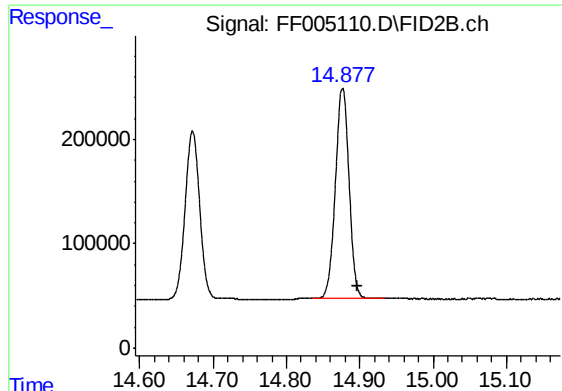


#10 N-TETRACOSANE

R.T.: 14.877 min
Delta R.T.: -0.020 min
Response: 2621086
Conc: 23.55 ug/ml

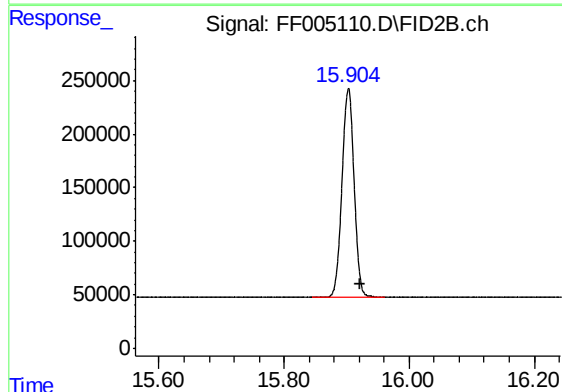

#11 N-HEXACOSANE

R.T.: 15.903 min
Delta R.T.: -0.019 min
Response: 2617547
Conc: 23.67 ug/ml

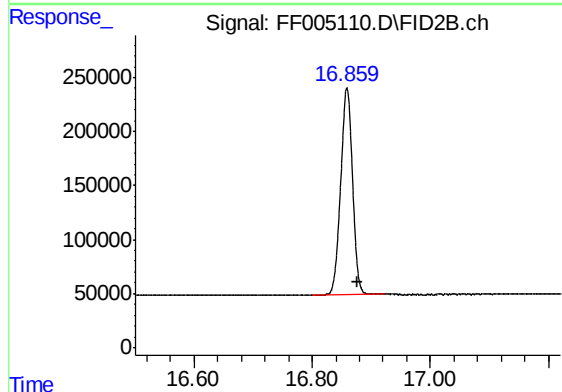

#12 N-OCTACOSANE

R.T.: 16.859 min
Delta R.T.: -0.019 min
Response: 2665763
Conc: 23.90 ug/ml