

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF072220\  
Data File : FF007204.D  
Signal(s) : FID2B.ch  
Acq On : 22 Jul 2020 12:23  
Operator : DD\AJ  
Sample : L3360-04 10X  
Misc :  
ALS Vial : 58 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
SP-3

Manual Integrations  
APPROVED

Ankita  
7/23/2020 1:08:09 PM

Integration File: autoint1.e  
Quant Time: Jul 23 01:19:13 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF071520.M  
Quant Title :  
QLast Update : Thu Jul 16 09:27:07 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.747 | 293949   | 2.085 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF072220\  
Data File : FF007204.D  
Signal(s) : FID2B.ch  
Acq On : 22 Jul 2020 12:23  
Operator : DD\AJ  
Sample : L3360-04 10X  
Misc :  
ALS Vial : 58 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
SP-3


Manual Integrations  
APPROVED

Ankita  
7/23/2020 1:08:09 PM

Integration File: autoint1.e  
Quant Time: Jul 23 01:19:13 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF071520.M  
Quant Title :  
QLast Update : Thu Jul 16 09:27:07 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

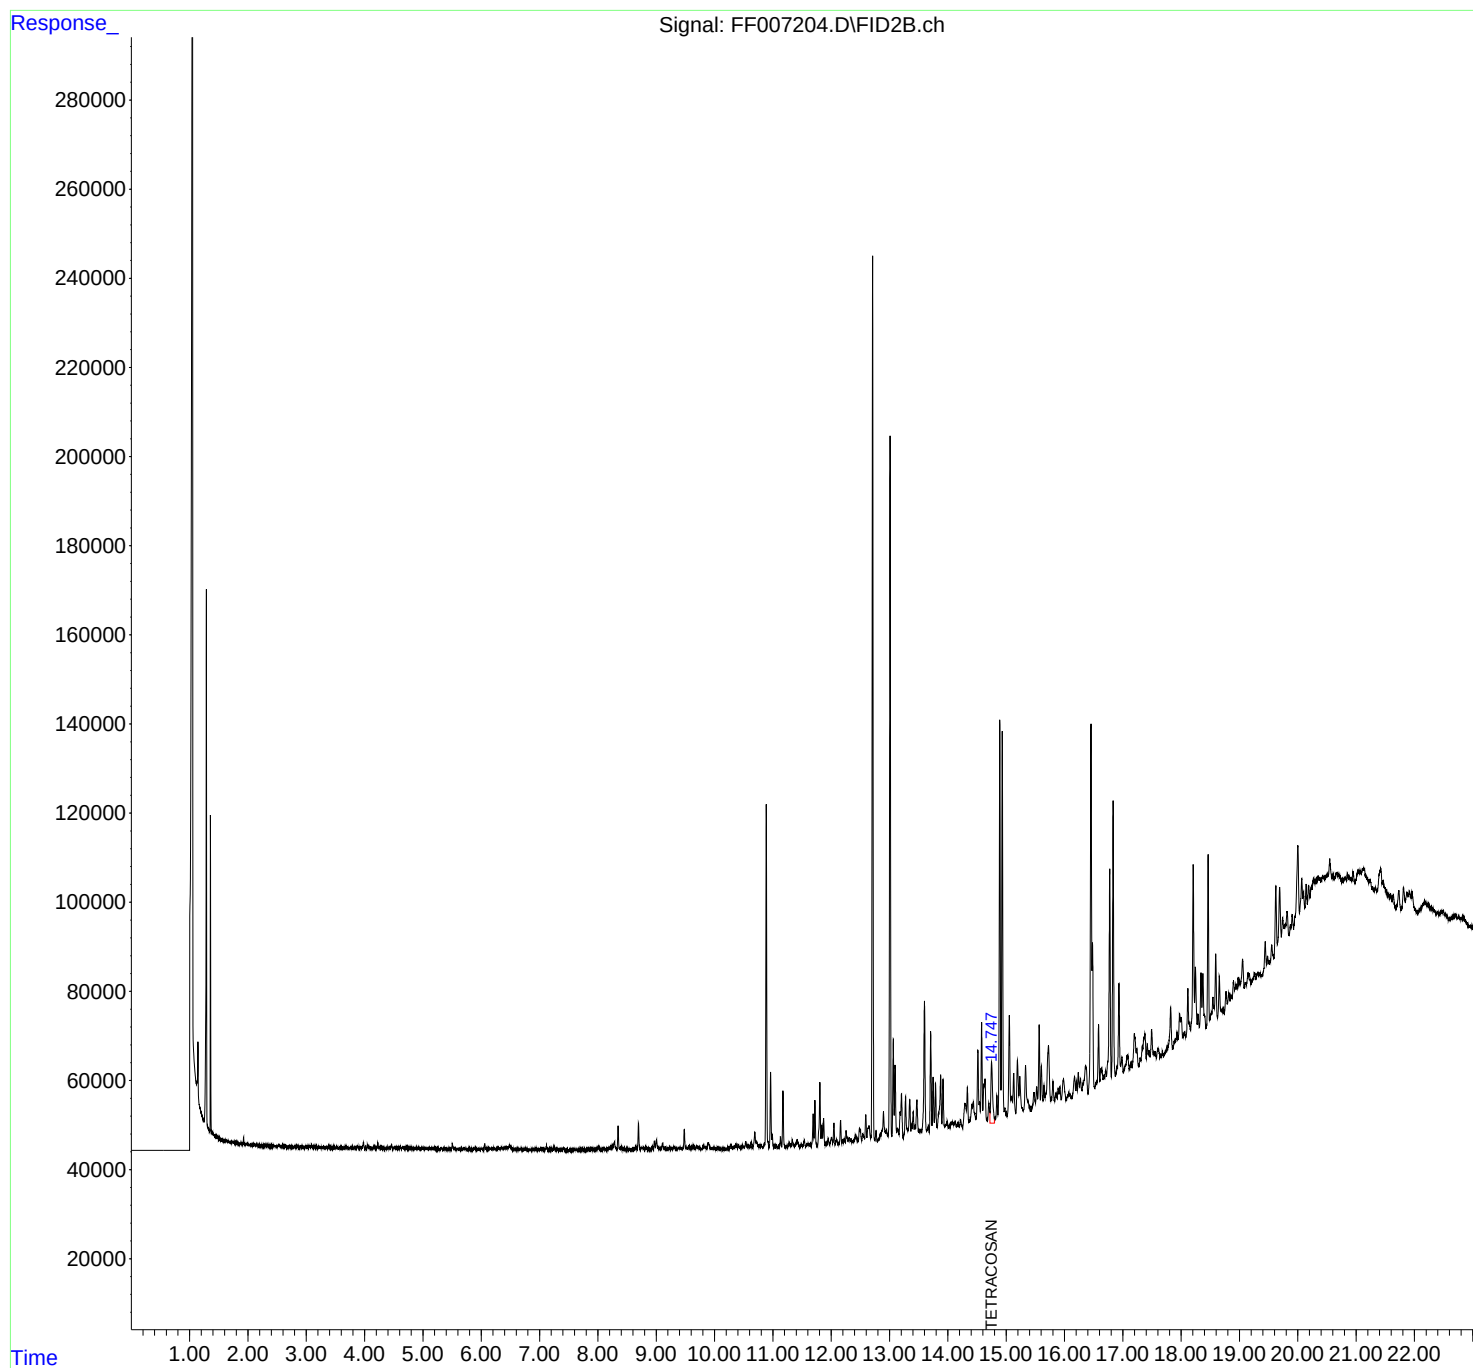

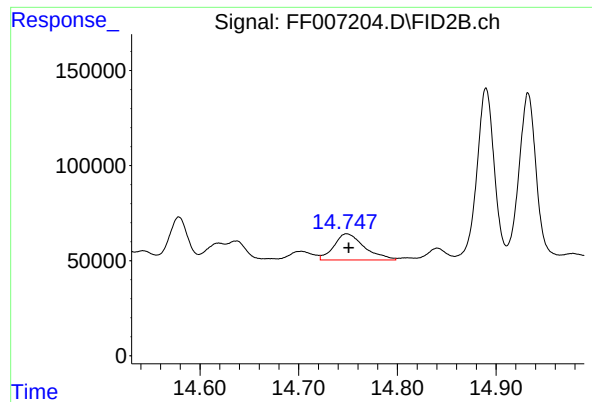

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.747 min  
Delta R.T.: -0.004 min  
Response: 293949  
Conc: 2.09 ug/ml m

Instrument :  
FID\_F  
ClientSampleId :  
SP-3

Manual Integrations  
APPROVED

Ankita  
7/23/2020 1:08:09 PM