

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072318\
 Data File : FF001458.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jul 2018 14:32
 Operator : AJ\SJ
 Sample : J3827-03 10X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 24 04:46:29 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.446	488493	4.535 ug/ml
Target Compounds			
7) N-EICOSANE	12.405	4490119	36.097 ug/ml
8) N-DOCOSANE	13.567	491259	3.984 ug/ml
10) N-TETRACOSANE	14.621	2118505	17.378 ug/ml
11) N-HEXACOSANE	15.664	227857	1.880 ug/ml
12) N-OCTACOSANE	16.624	600234	4.982 ug/ml
13) N-TRIACONTANE	17.485	217083	1.806 ug/ml
14) N-DOTRIACONTANE	18.292f	647789	5.494 ug/ml
16) N-HEXATRIACONTANE	19.846	364833	3.212 ug/ml
18) N-TETRACONTANE	21.427	138553	1.353 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072318\
Data File : FF001458.D
Signal(s) : FID2B.ch
Acq On : 23 Jul 2018 14:32
Operator : AJ\SJ
Sample : J3827-03 10X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 24 04:46:29 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

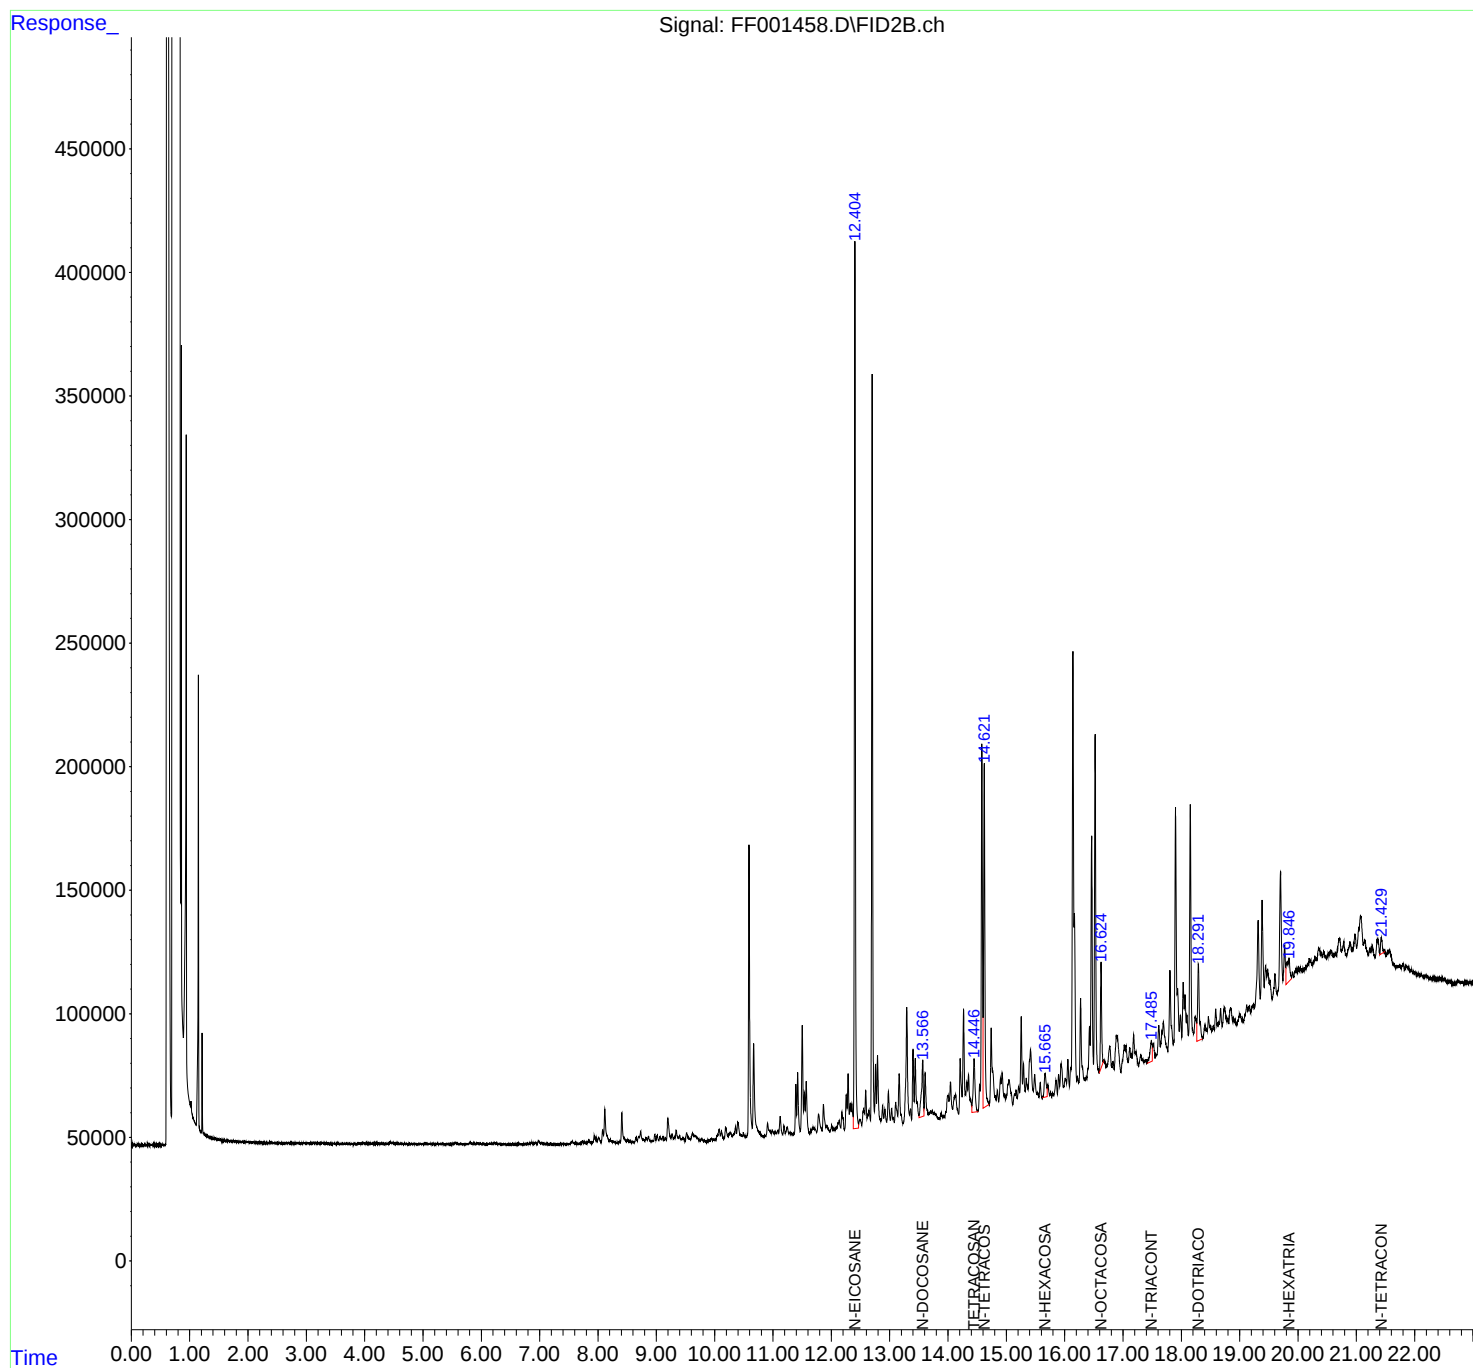

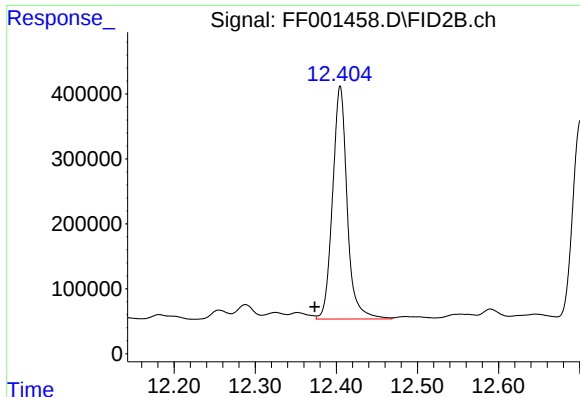


#7 N-EICOSANE

R.T.: 12.405 min
Delta R.T.: 0.031 min
Response: 4490119
Conc: 36.10 ug/ml

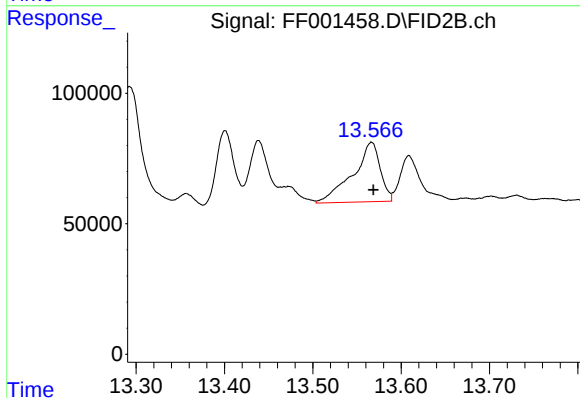


#8 N-DOCOSANE

R.T.: 13.567 min
Delta R.T.: -0.002 min
Response: 491259
Conc: 3.98 ug/ml

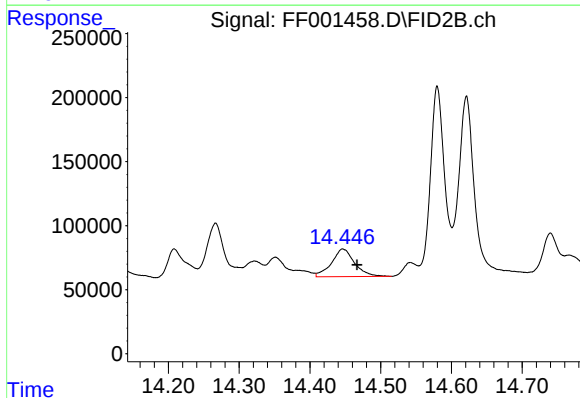


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.446 min
Delta R.T.: -0.020 min
Response: 488493
Conc: 4.53 ug/ml

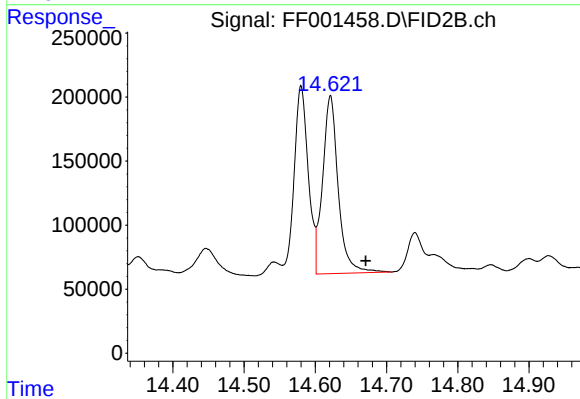


#10 N-TETRACOSANE

R.T.: 14.621 min
Delta R.T.: -0.049 min
Response: 2118505
Conc: 17.38 ug/ml

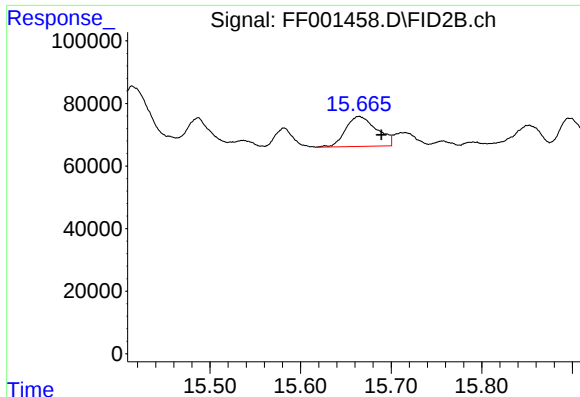


#11 N-HEXACOSANE

R.T.: 15.664 min
Delta R.T.: -0.025 min
Response: 227857
Conc: 1.88 ug/ml

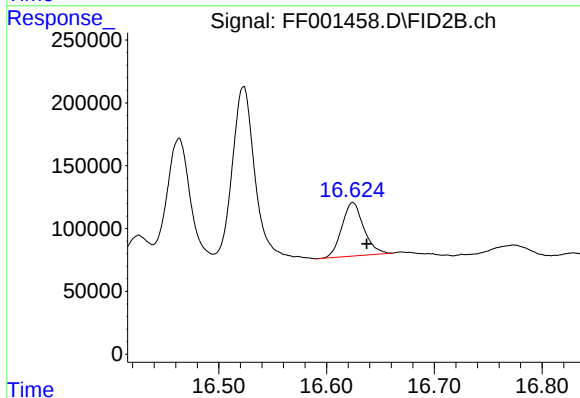


#12 N-OCTACOSANE

R.T.: 16.624 min
Delta R.T.: -0.013 min
Response: 600234
Conc: 4.98 ug/ml

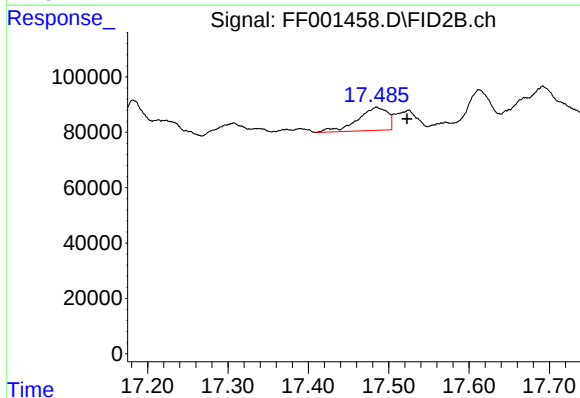


#13 N-TRIACONTANE

R.T.: 17.485 min
Delta R.T.: -0.038 min
Response: 217083
Conc: 1.81 ug/ml

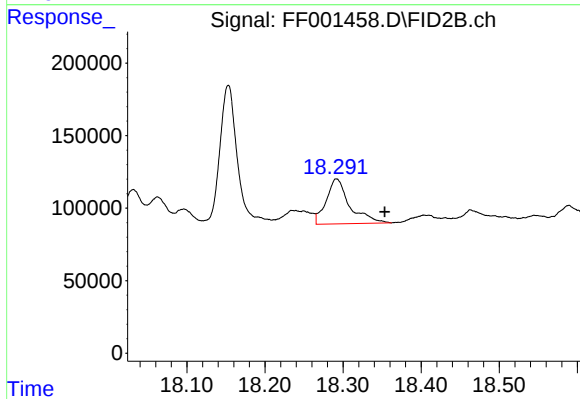


#14 N-DOTRIACONTANE

R.T.: 18.292 min
Delta R.T.: -0.062 min
Response: 647789
Conc: 5.49 ug/ml

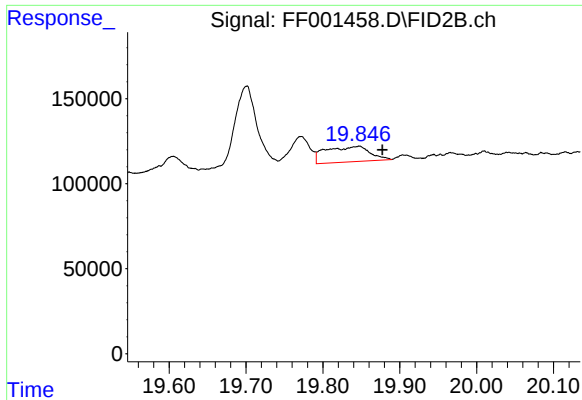

#16 N-HEXATRIACONTANE

R.T.: 19.846 min
Delta R.T.: -0.031 min
Response: 364833
Conc: 3.21 ug/ml

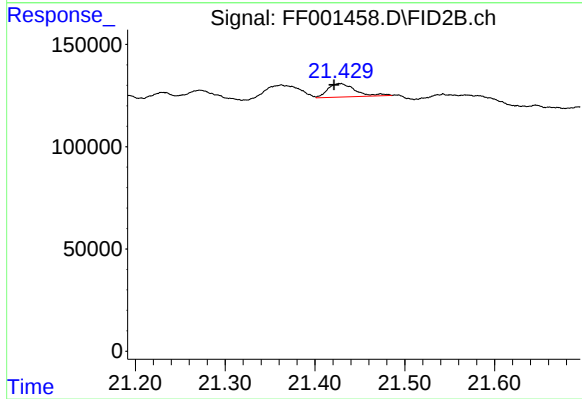

#18 N-TETRACONTANE

R.T.: 21.427 min
Delta R.T.: 0.006 min
Response: 138553
Conc: 1.35 ug/ml