

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072319\
Data File : FF005120.D
Signal(s) : FID2B.ch
Acq On : 23 Jul 2019 17:49
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 24 01:23:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.561	126614	1.091 ug/ml
8)	N-DOCOSANE	13.770	130692	1.162 ug/ml
10)	N-TETRACOSANE	14.857	422179	3.793 ug/ml
13)	N-TRIACONTANE	17.759	102996	0.917 ug/ml
14)	N-DOTRIACONTANE	18.604	194173	1.705 ug/ml
15)	N-TETRATRIACONTANE	19.396	98646	0.909 ug/ml
16)	N-HEXATRIACONTANE	20.177	1730667	16.713 ug/ml
17)	N-OCTATRIACONTANE	20.902	881857	9.246 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072319\
Data File : FF005120.D
Signal(s) : FID2B.ch
Acq On : 23 Jul 2019 17:49
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 24 01:23:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

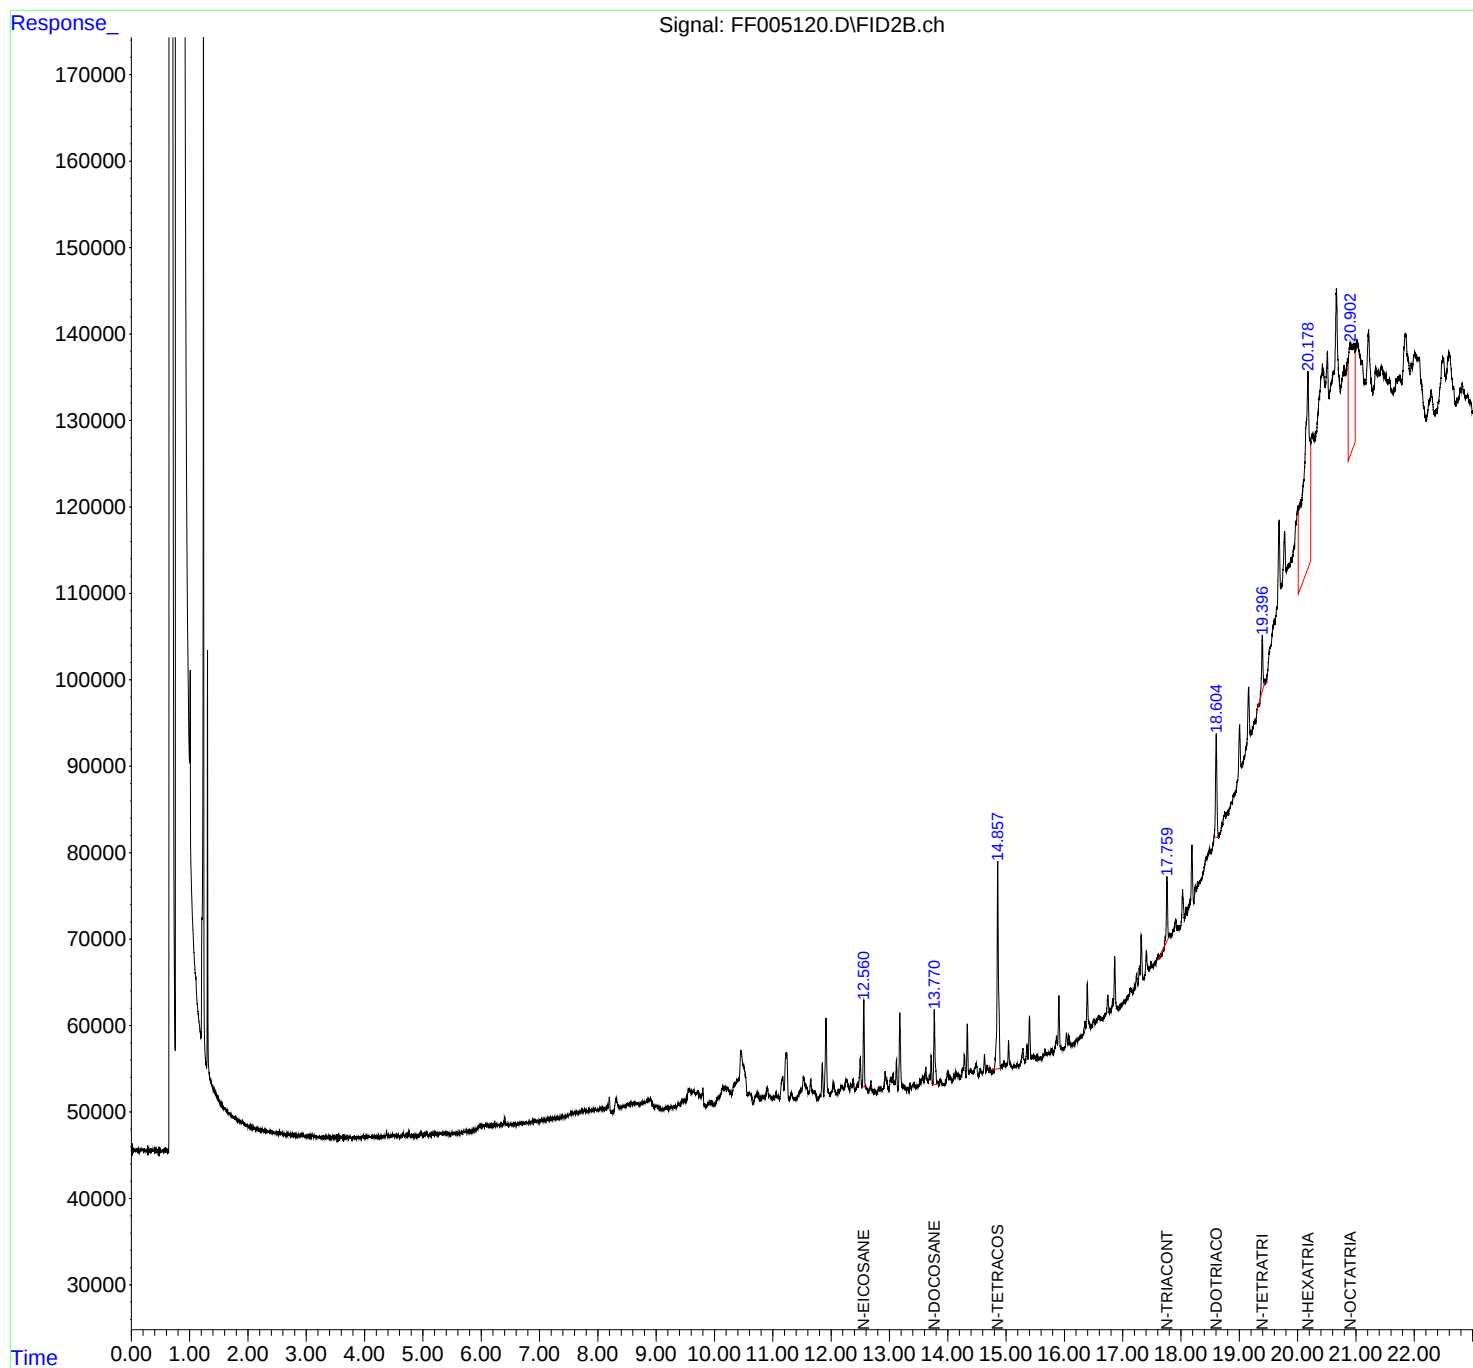

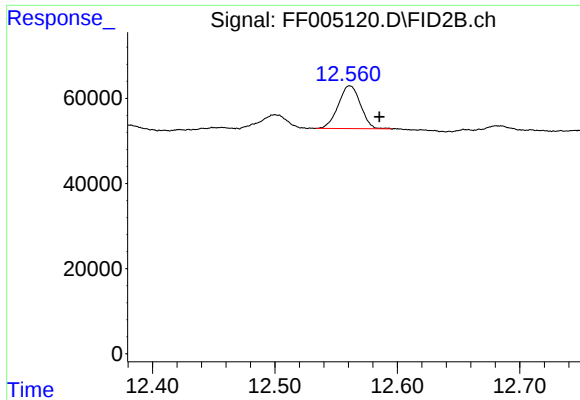


#7 N-EICOSANE

R.T.: 12.561 min
Delta R.T.: -0.024 min
Response: 126614
Conc: 1.09 ug/ml

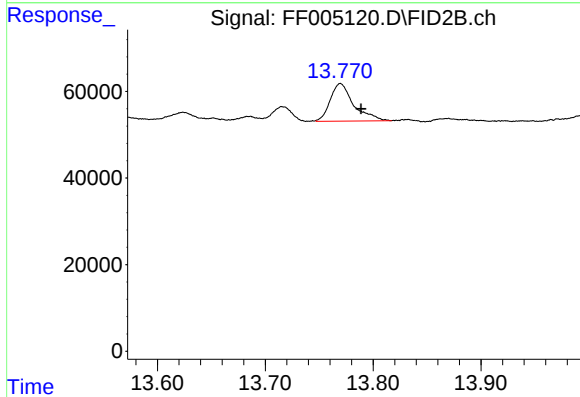


#8 N-DOCOSANE

R.T.: 13.770 min
Delta R.T.: -0.019 min
Response: 130692
Conc: 1.16 ug/ml

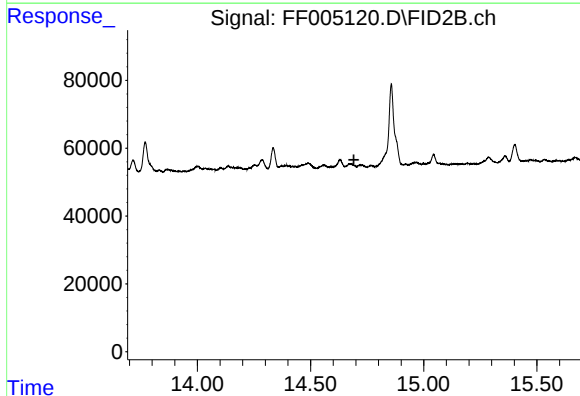


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.692 min
Response: 0
Conc: N.D.

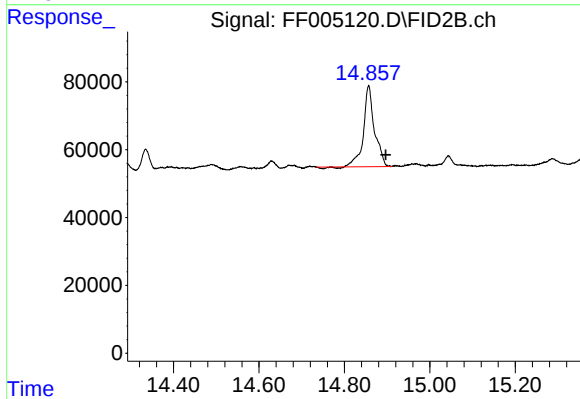


#10 N-TETRACOSANE

R.T.: 14.857 min
Delta R.T.: -0.040 min
Response: 422179
Conc: 3.79 ug/ml

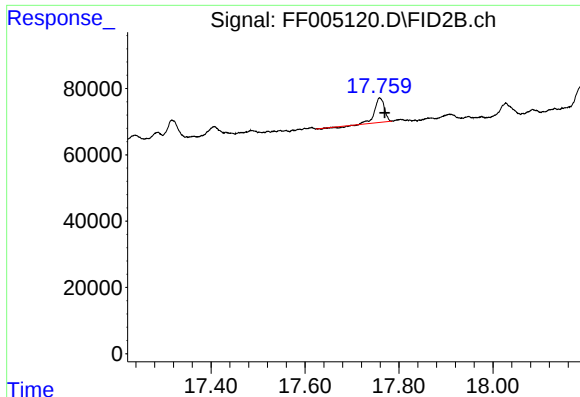


#13 N-TRIACONTANE

R.T.: 17.759 min
Delta R.T.: -0.011 min
Response: 102996
Conc: 0.92 ug/ml

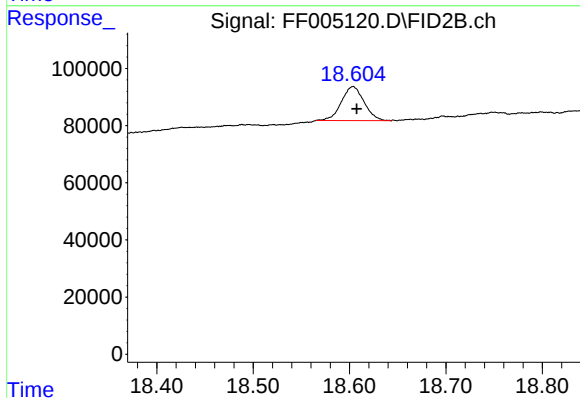


#14 N-DOTRIACONTANE

R.T.: 18.604 min
Delta R.T.: -0.004 min
Response: 194173
Conc: 1.70 ug/ml

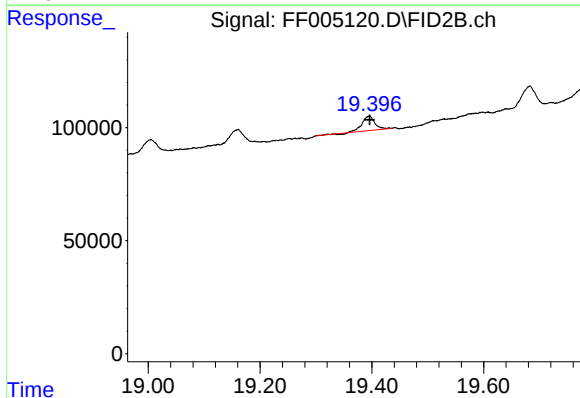


#15 N-TETRATRIACONTANE

R.T.: 19.396 min
Delta R.T.: 0.000 min
Response: 98646
Conc: 0.91 ug/ml

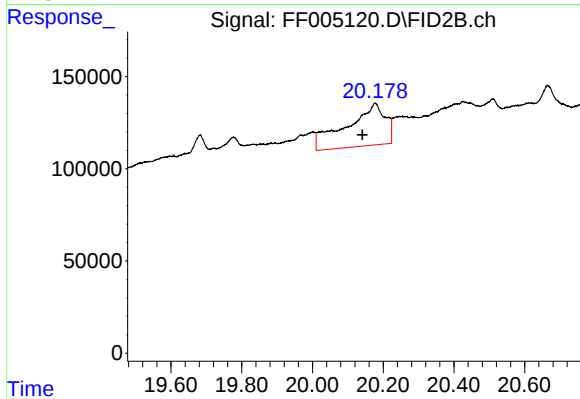

#16 N-HEXATRIACONTANE

R.T.: 20.177 min
Delta R.T.: 0.036 min
Response: 1730667
Conc: 16.71 ug/ml

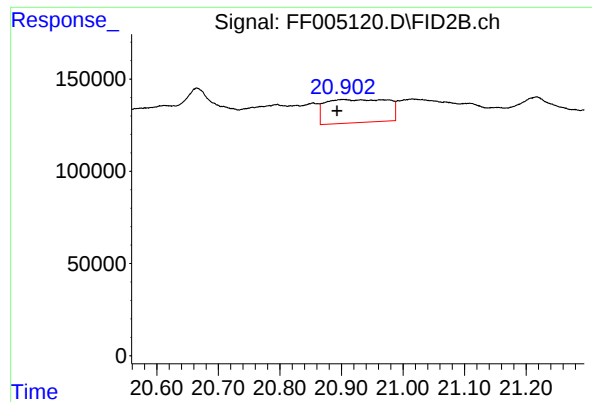

#17 N-OCTATRIACONTANE

R.T.: 20.902 min
Delta R.T.: 0.009 min
Response: 881857
Conc: 9.25 ug/ml