

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
 Data File : FF007229.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jul 2020 12:18
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 25 00:38:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.493	15153588	97.559 ug/ml
11) N-HEXACOSANE	15.977	176637	1.086 ug/ml
12) N-OCTACOSANE	16.940	14339072	87.507 ug/ml
13) N-TRIACONTANE	17.820	1769419	10.704 ug/ml
14) N-DOTRIACONTANE	18.656	1957494	12.464 ug/ml
15) N-TETRATRIACONTANE	19.445	1442993	11.084 ug/ml
16) N-HEXATRIACONTANE	20.189	945979	9.683 ug/ml
17) N-OCTATRIACONTANE	20.950	549513	6.968 ug/ml
18) N-TETRACONTANE	21.899	341248	4.764 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007229.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 12:18
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 00:38:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

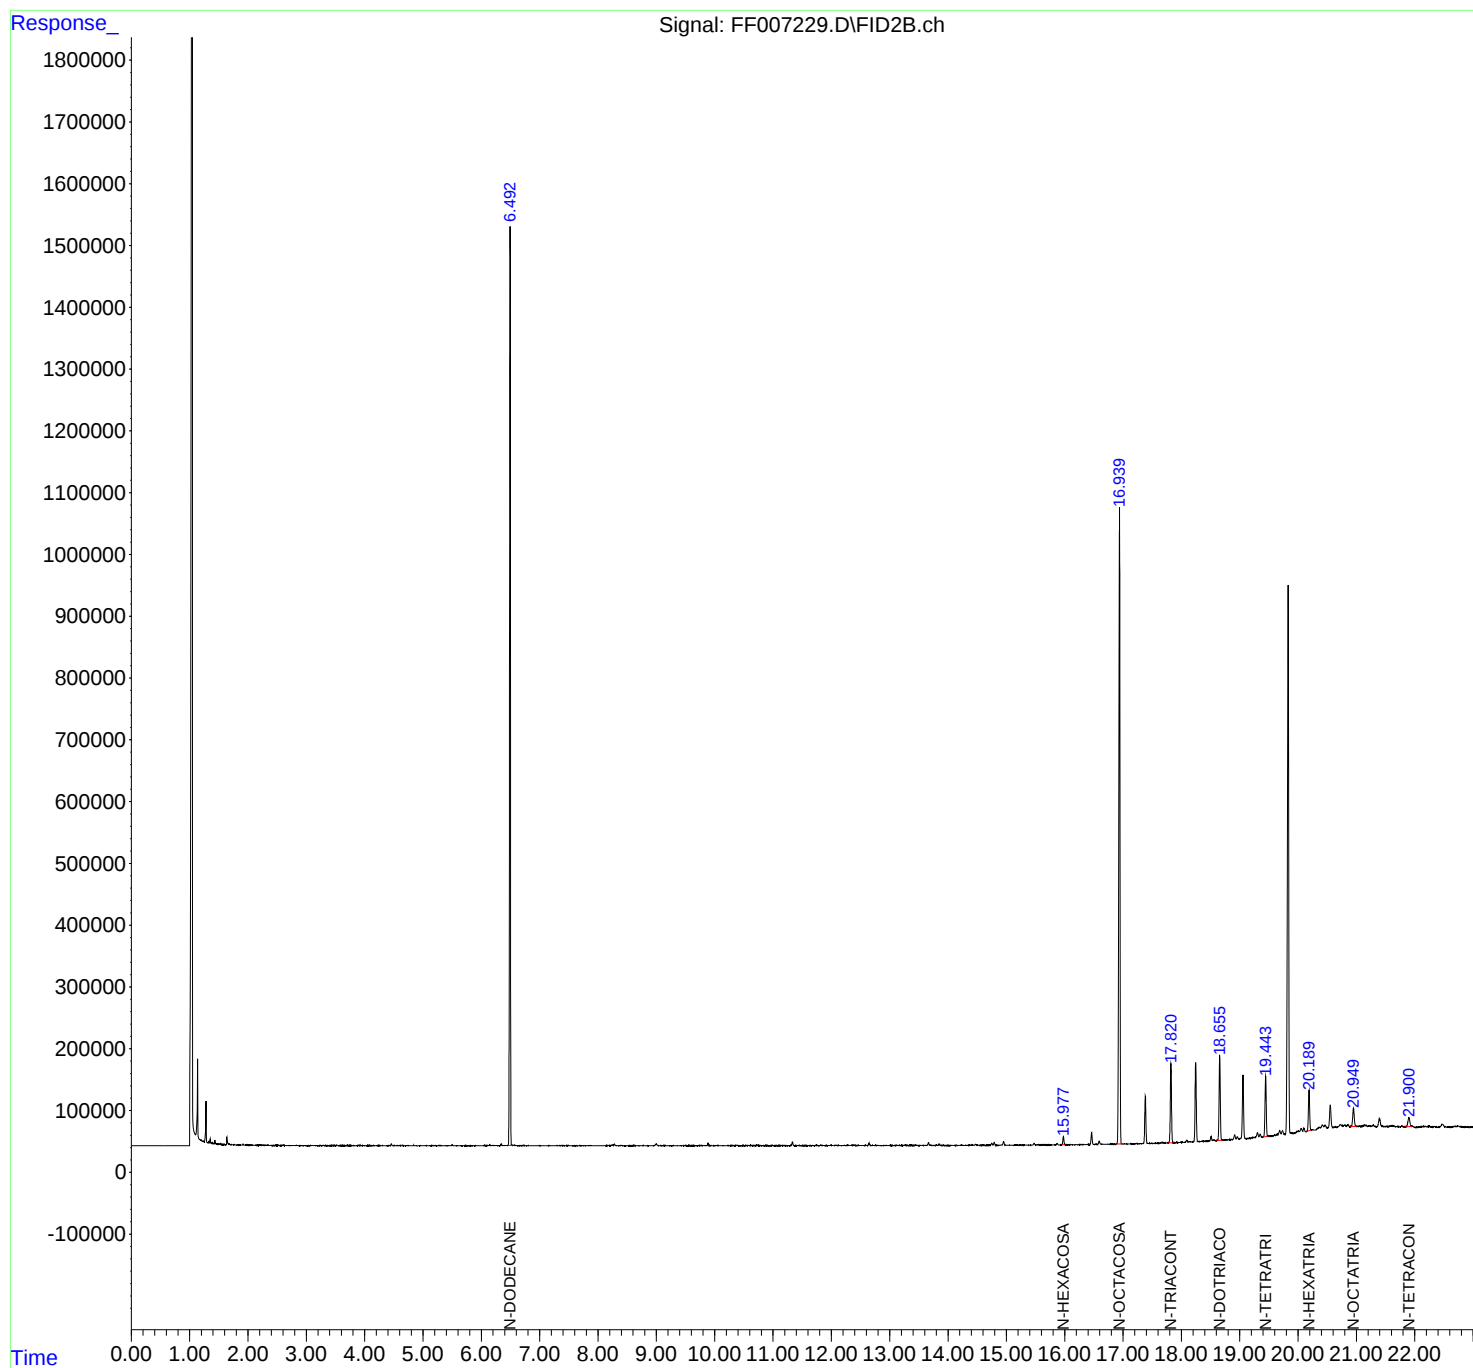


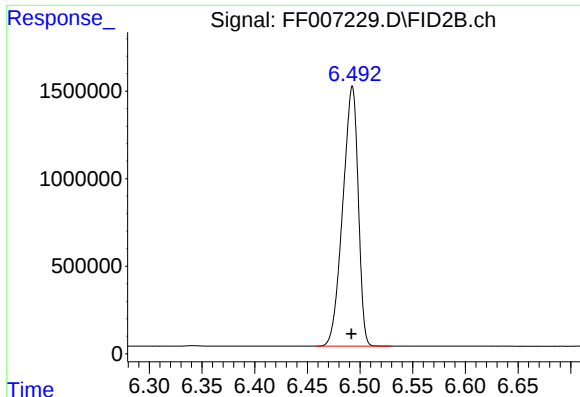

#3 N-DODECANE


R.T.: 6.493 min
Delta R.T.: 0.001 min
Response: 15153588
Conc: 97.56 ug/ml

Instrument :
FID_F
ClientSampleId :

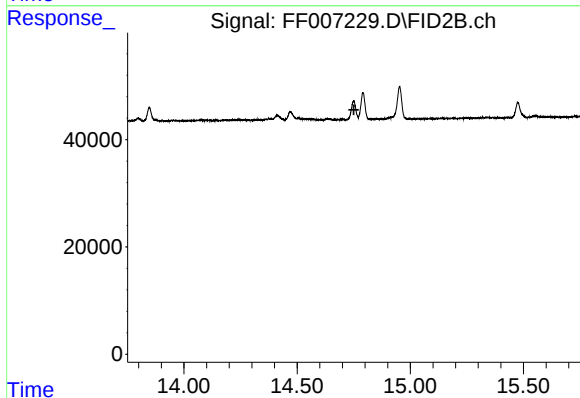


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.751 min
Response: 0
Conc: N.D.

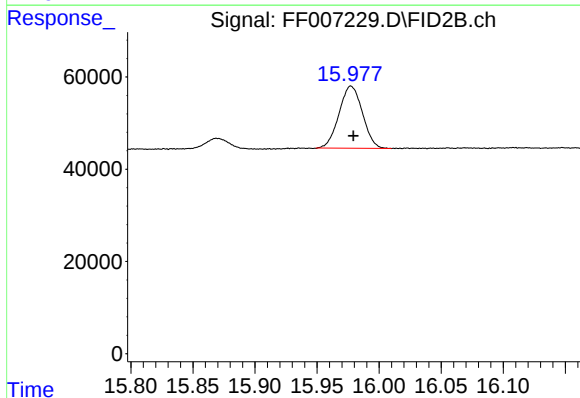


#11 N-HEXACOSANE

R.T.: 15.977 min
Delta R.T.: -0.002 min
Response: 176637
Conc: 1.09 ug/ml

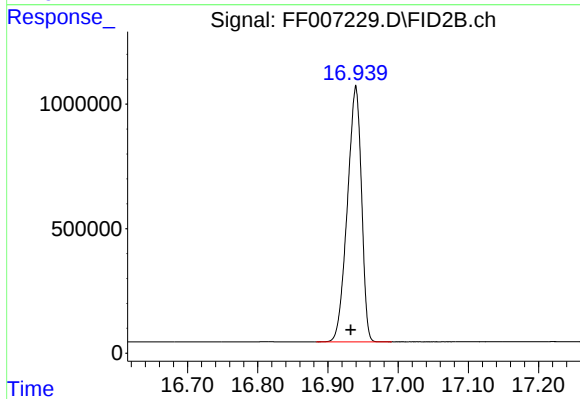

#12 N-OCTACOSANE


R.T.: 16.940 min
Delta R.T.: 0.007 min
Response: 14339072
Conc: 87.51 ug/ml

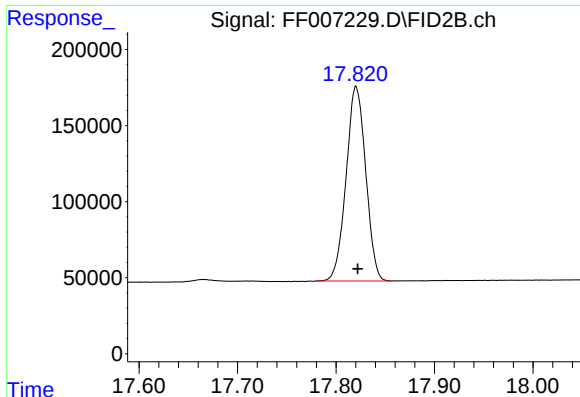

#13 N-TRIACONTANE


R.T.: 17.820 min
Delta R.T.: -0.002 min
Response: 1769419
Conc: 10.70 ug/ml

Instrument :
FID_F
ClientSampleId :

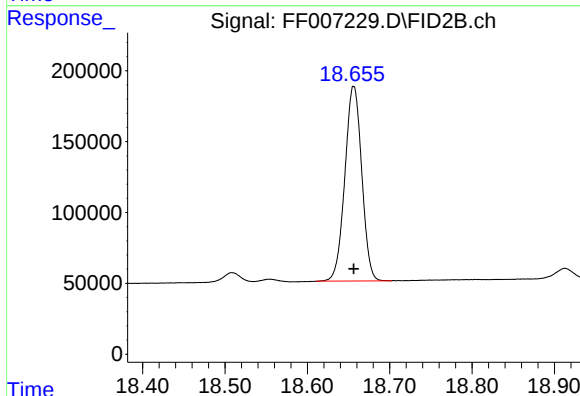


#14 N-DOTRIACONTANE

R.T.: 18.656 min
Delta R.T.: 0.000 min
Response: 1957494
Conc: 12.46 ug/ml

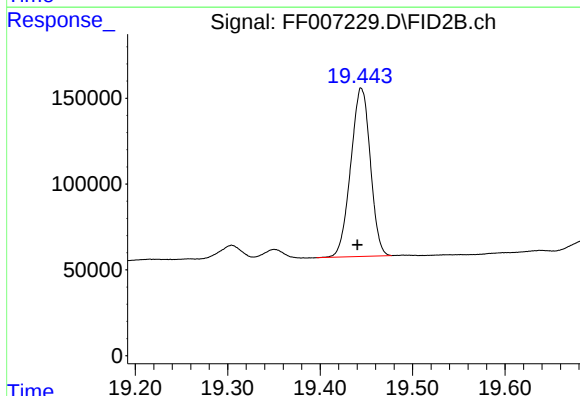


#15 N-TETRATRIACONTANE

R.T.: 19.445 min
Delta R.T.: 0.004 min
Response: 1442993
Conc: 11.08 ug/ml

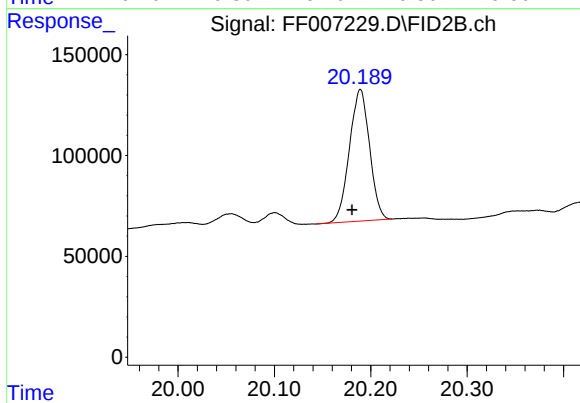

#16 N-HEXATRIACONTANE


R.T.: 20.189 min
Delta R.T.: 0.009 min
Response: 945979
Conc: 9.68 ug/ml

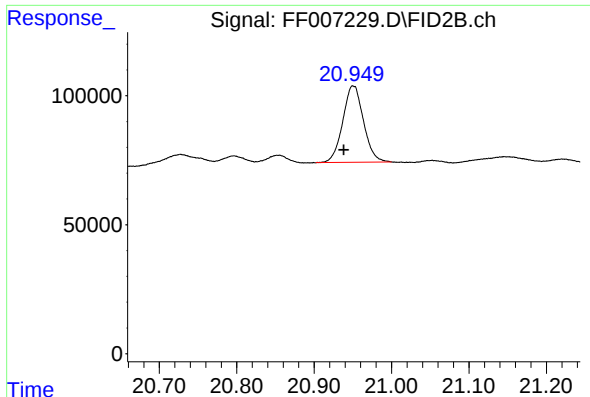

#17 N-OCTATRIACONTANE

R.T.: 20.950 min
Delta R.T.: 0.012 min
Response: 549513
Conc: 6.97 ug/ml

Instrument :
FID_F
ClientSampleId :

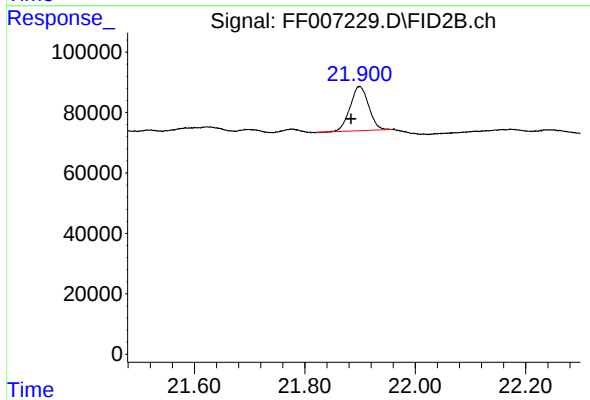

#18 N-TETRACONTANE

R.T.: 21.899 min
Delta R.T.: 0.016 min
Response: 341248
Conc: 4.76 ug/ml