

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007230.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 12:58
Operator : DD\AJ
Sample : L3381-07 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 00:38:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.750	193696	1.374 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.344f	130763	0.845 ug/ml
7)	N-EICOSANE	12.711f	274182	1.698 ug/ml
10)	N-TETRACOSANE	14.935	193858	1.184 ug/ml
14)	N-DOTRIACONTANE	18.639	445883	2.839 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007230.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 12:58
Operator : DD\AJ
Sample : L3381-07 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 00:38:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

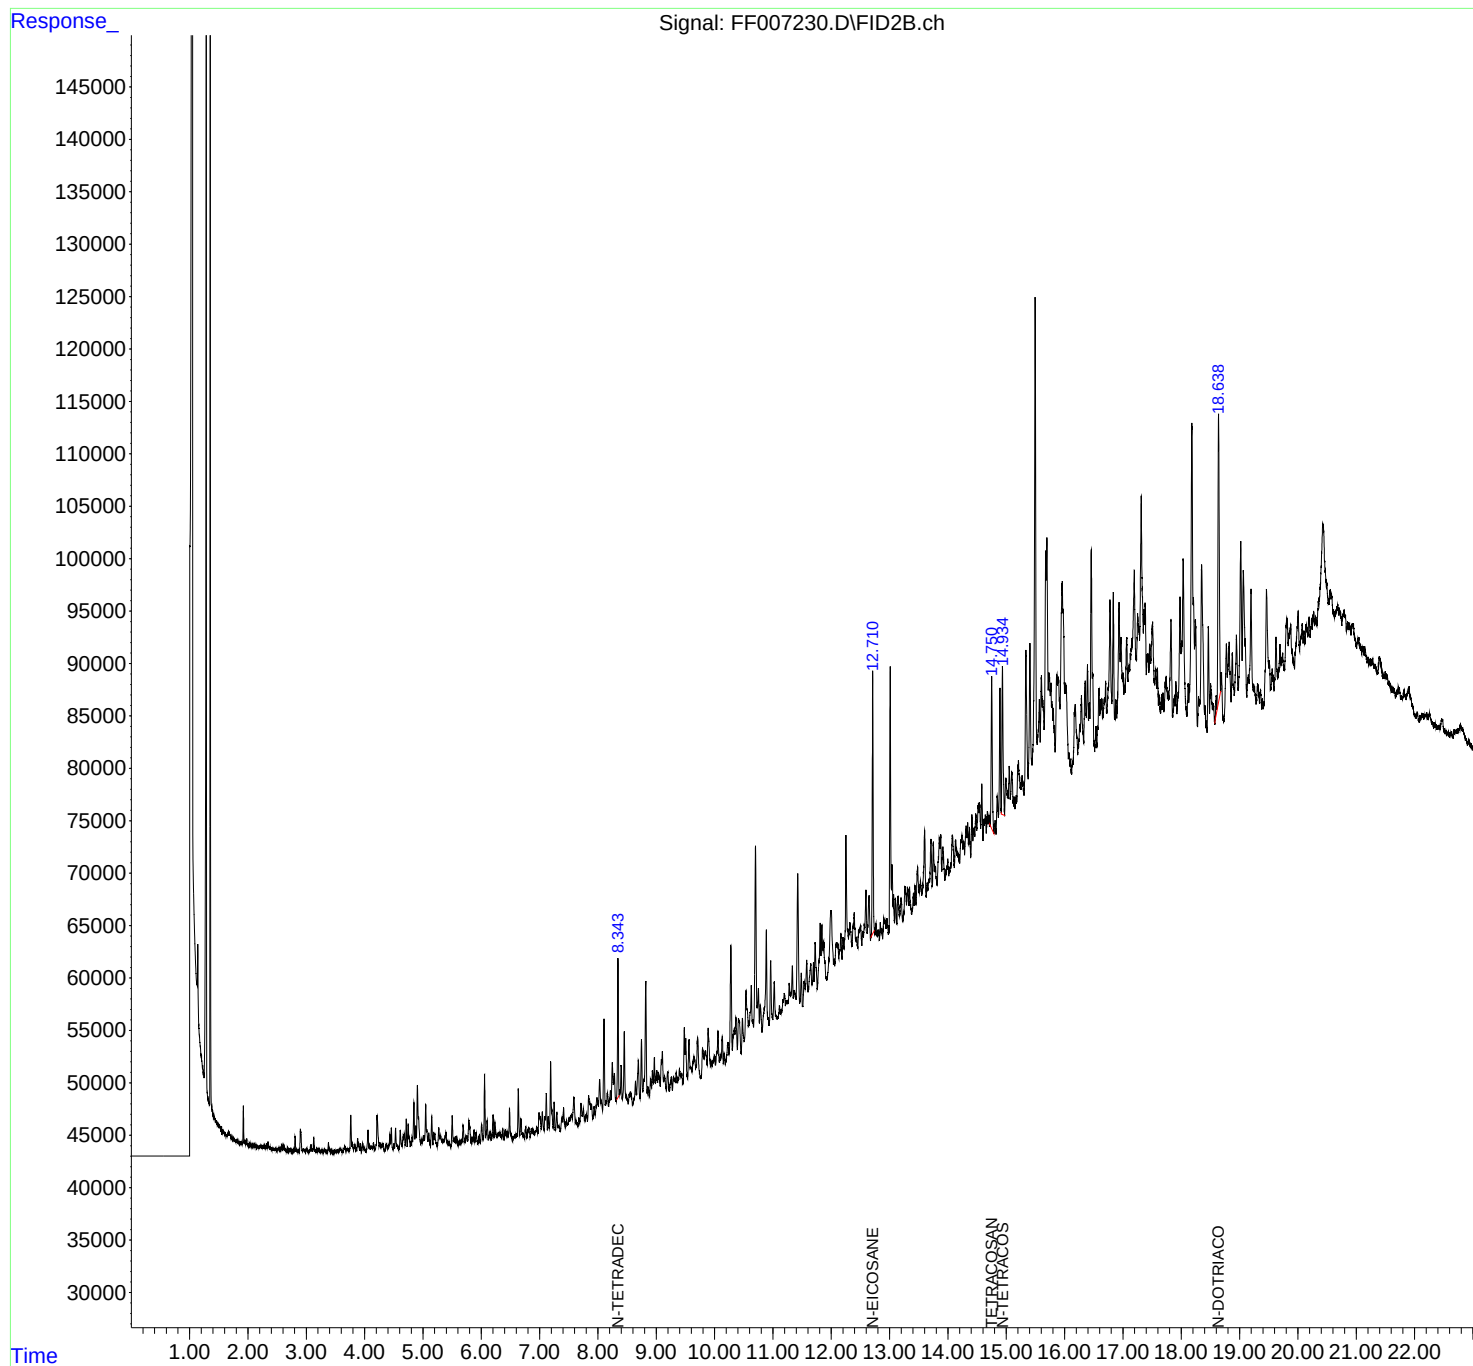


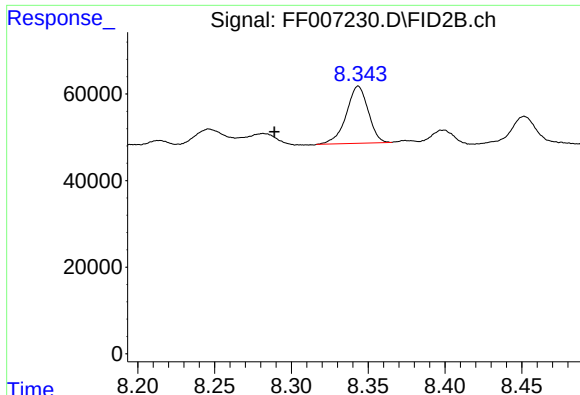

#4 N-TETRADECANE


R.T.: 8.344 min
Delta R.T.: 0.055 min
Response: 130763
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

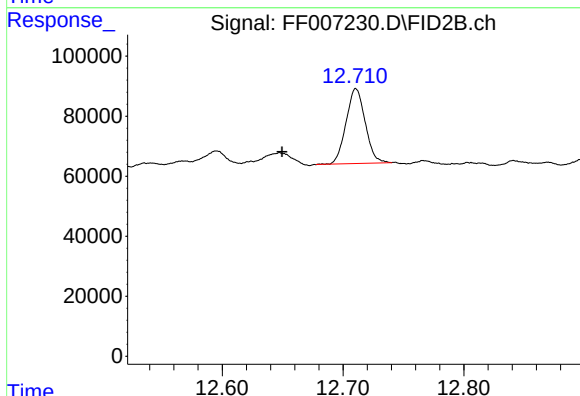


#7 N-EICOSANE

R.T.: 12.711 min
Delta R.T.: 0.061 min
Response: 274182
Conc: 1.70 ug/ml

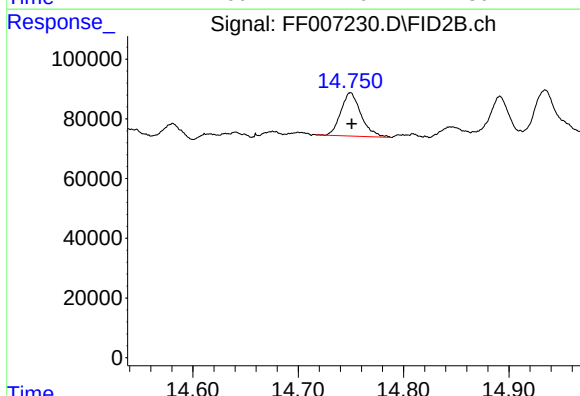


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: -0.001 min
Response: 193696
Conc: 1.37 ug/ml

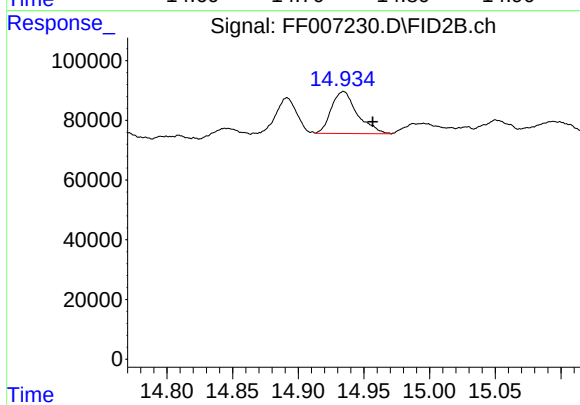

#10 N-TETRACOSANE

R.T.: 14.935 min
Delta R.T.: -0.022 min
Response: 193858
Conc: 1.18 ug/ml

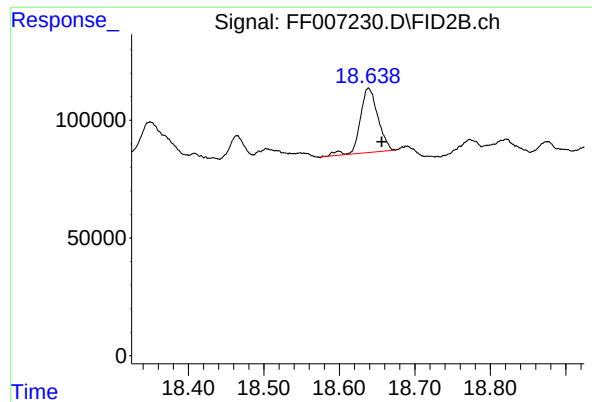

#14 N-DOTRIACONTANE

R.T.: 18.639 min
Delta R.T.: -0.018 min
Response: 445883
Conc: 2.84 ug/ml

Instrument :
FID_F
ClientSampleId :