

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
 Data File : FF007232.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jul 2020 13:59
 Operator : DD\AJ
 Sample : L3381-04 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 25 00:39:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.752	434702	3.084 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.348f	229785	1.484 ug/ml
7)	N-EICOSANE	12.598f	122982	0.762 ug/ml
10)	N-TETRACOSANE	14.938	936732	5.720 ug/ml
12)	N-OCTACOSANE	16.942	368111	2.246 ug/ml
13)	N-TRIACONTANE	17.826	511819	3.096 ug/ml
14)	N-DOTRIACONTANE	18.662	255022	1.624 ug/ml
15)	N-TETRATRIACONTANE	19.450	269398	2.069 ug/ml
16)	N-HEXATRIACONTANE	20.191	105000	1.075 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007232.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 13:59
Operator : DD\AJ
Sample : L3381-04 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 00:39:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

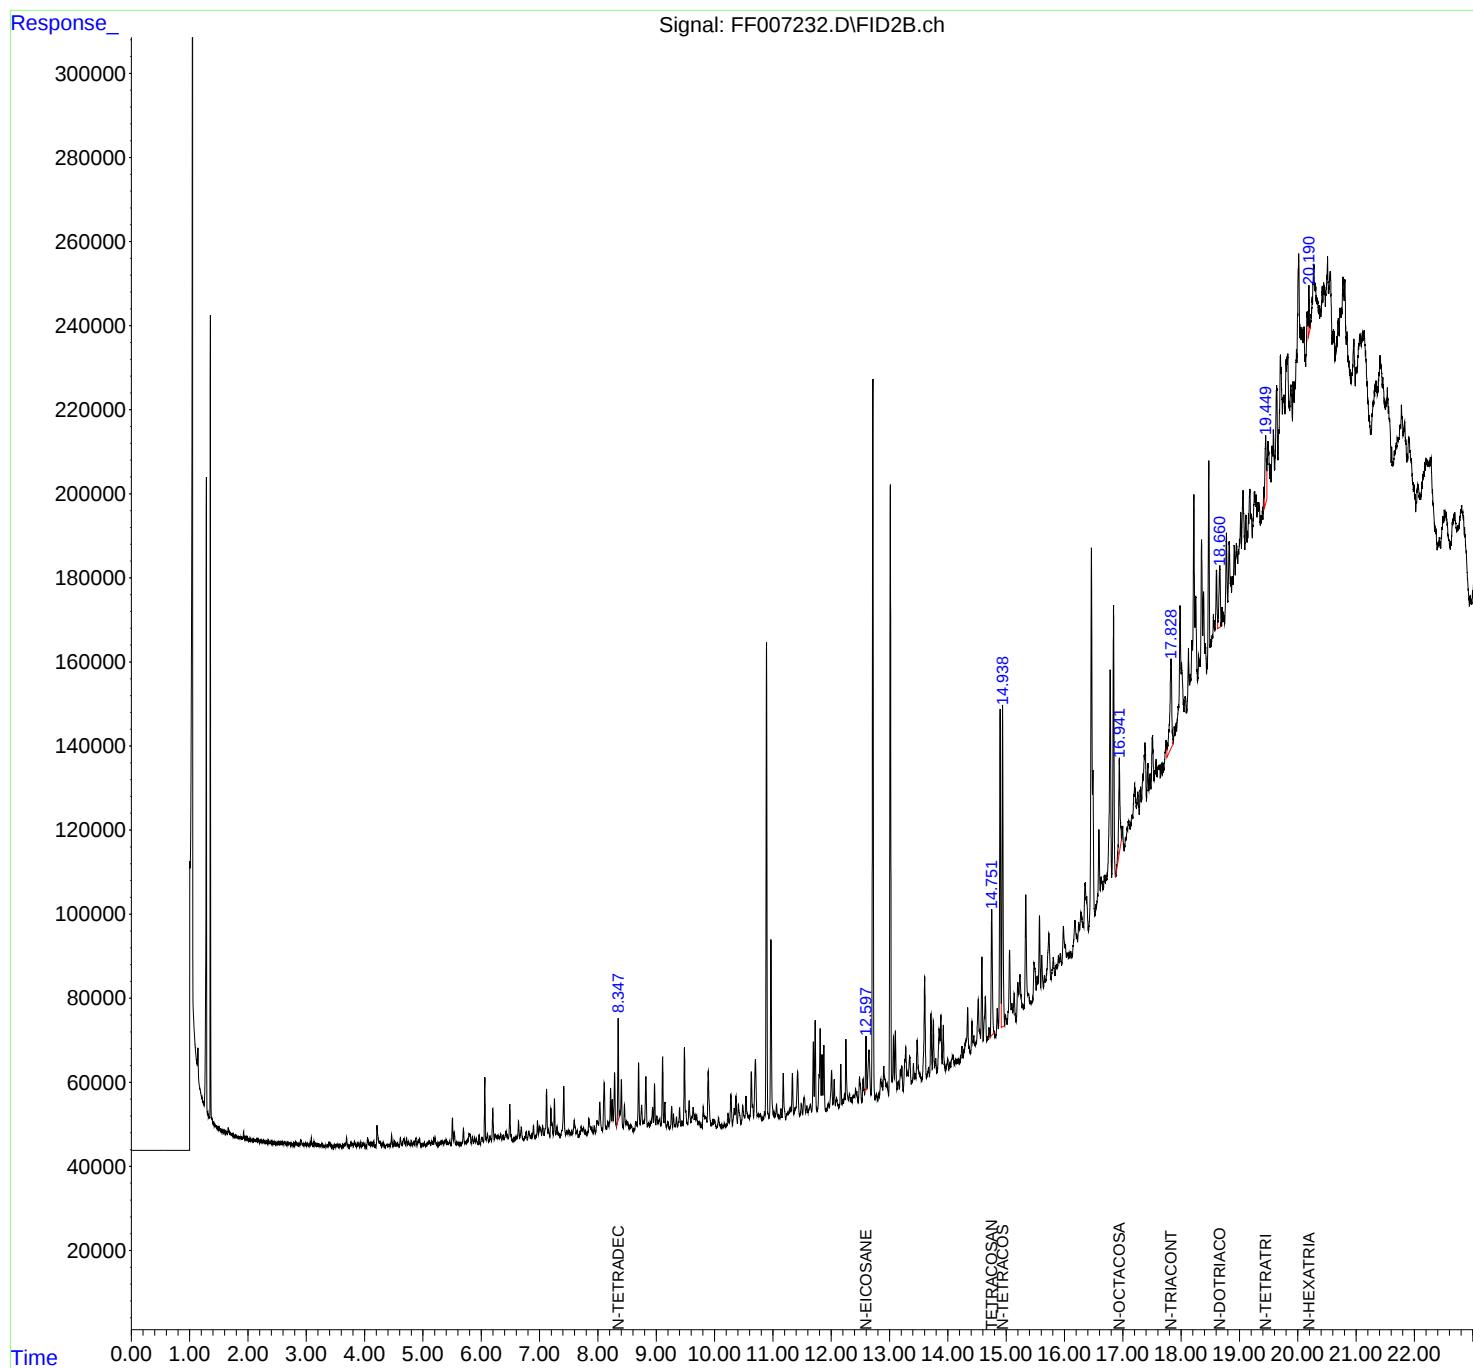


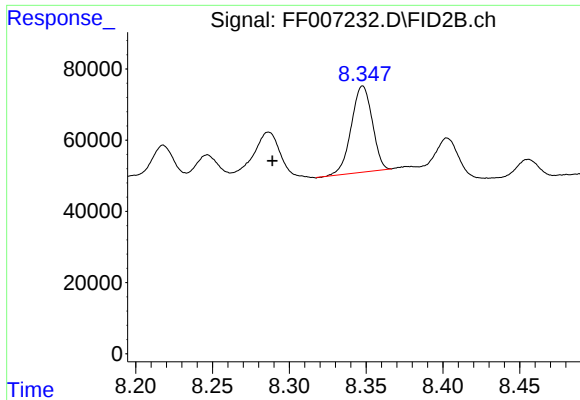

#4 N-TETRADECANE


R.T.: 8.348 min
Delta R.T.: 0.059 min
Response: 229785
Conc: 1.48 ug/ml

Instrument :
FID_F
ClientSampleId :

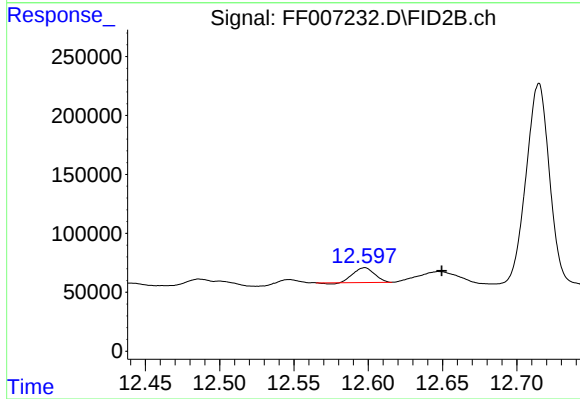


#7 N-EICOSANE

R.T.: 12.598 min
Delta R.T.: -0.052 min
Response: 122982
Conc: 0.76 ug/ml

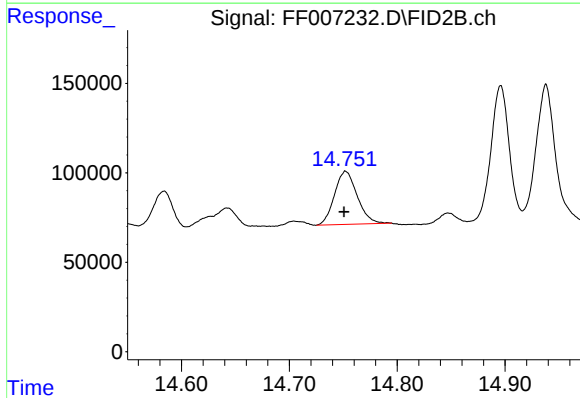


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.752 min
Delta R.T.: 0.002 min
Response: 434702
Conc: 3.08 ug/ml

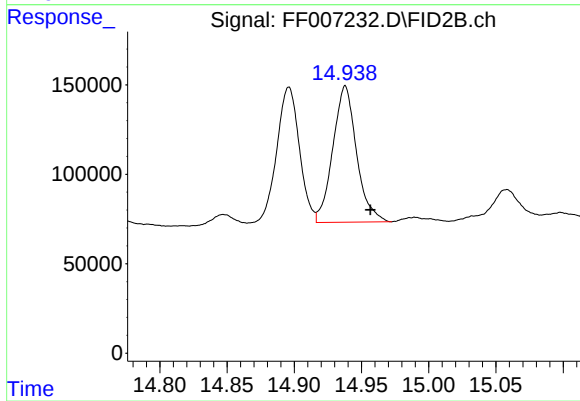

#10 N-TETRACOSANE


R.T.: 14.938 min
Delta R.T.: -0.019 min
Response: 936732
Conc: 5.72 ug/ml

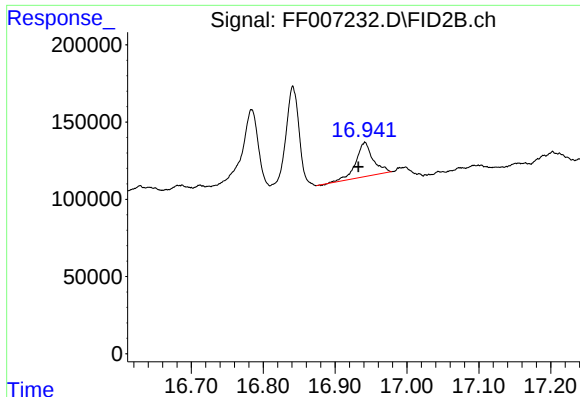

#12 N-OCTACOSANE


R.T.: 16.942 min
Delta R.T.: 0.009 min
Response: 368111
Conc: 2.25 ug/ml

Instrument :
FID_F
ClientSampleId :

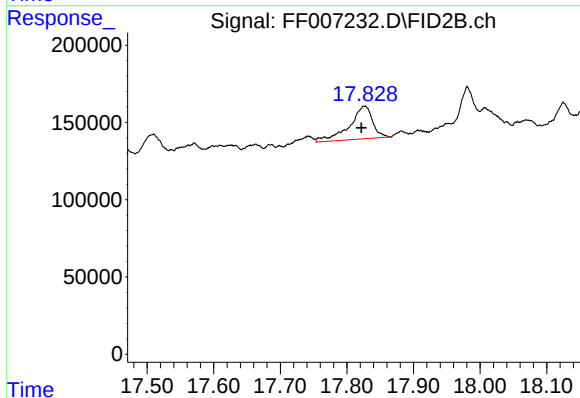


#13 N-TRIACONTANE

R.T.: 17.826 min
Delta R.T.: 0.004 min
Response: 511819
Conc: 3.10 ug/ml

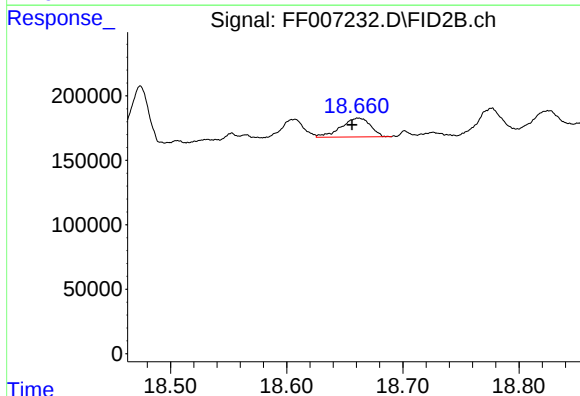


#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: 0.005 min
Response: 255022
Conc: 1.62 ug/ml

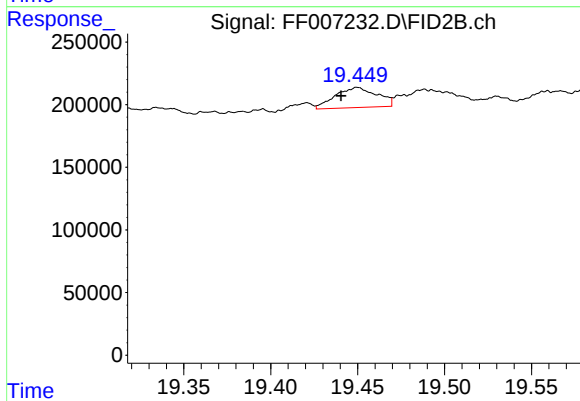

#15 N-TETRATRIACONTANE

R.T.: 19.450 min
Delta R.T.: 0.010 min
Response: 269398
Conc: 2.07 ug/ml

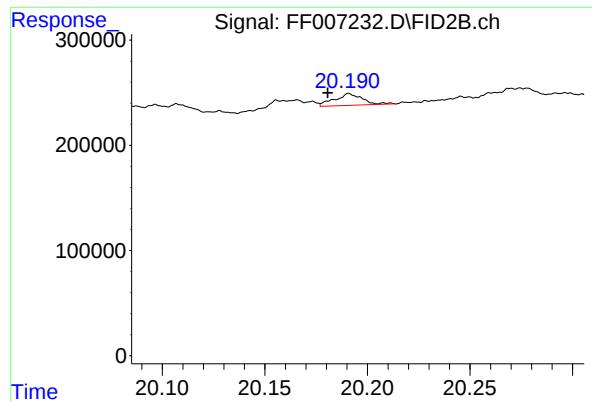

#16 N-HEXATRIACONTANE

R.T.: 20.191 min
Delta R.T.: 0.011 min
Response: 105000
Conc: 1.07 ug/ml

Instrument :
FID_F
ClientSampleId :