

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
 Data File : FF007236.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jul 2020 16:35
 Operator : DD\AJ
 Sample : L3418-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 25 00:39:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.754	1996030	14.159 ug/ml
Target Compounds			
4) N-TETRADECANE	8.349f	567496	3.665 ug/ml
7) N-EICOSANE	12.715f	1268537	7.855 ug/ml
10) N-TETRACOSANE	14.937	602950	3.682 ug/ml
14) N-DOTRIACONTANE	18.705	2966789	18.891 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007236.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 16:35
Operator : DD\AJ
Sample : L3418-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 00:39:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

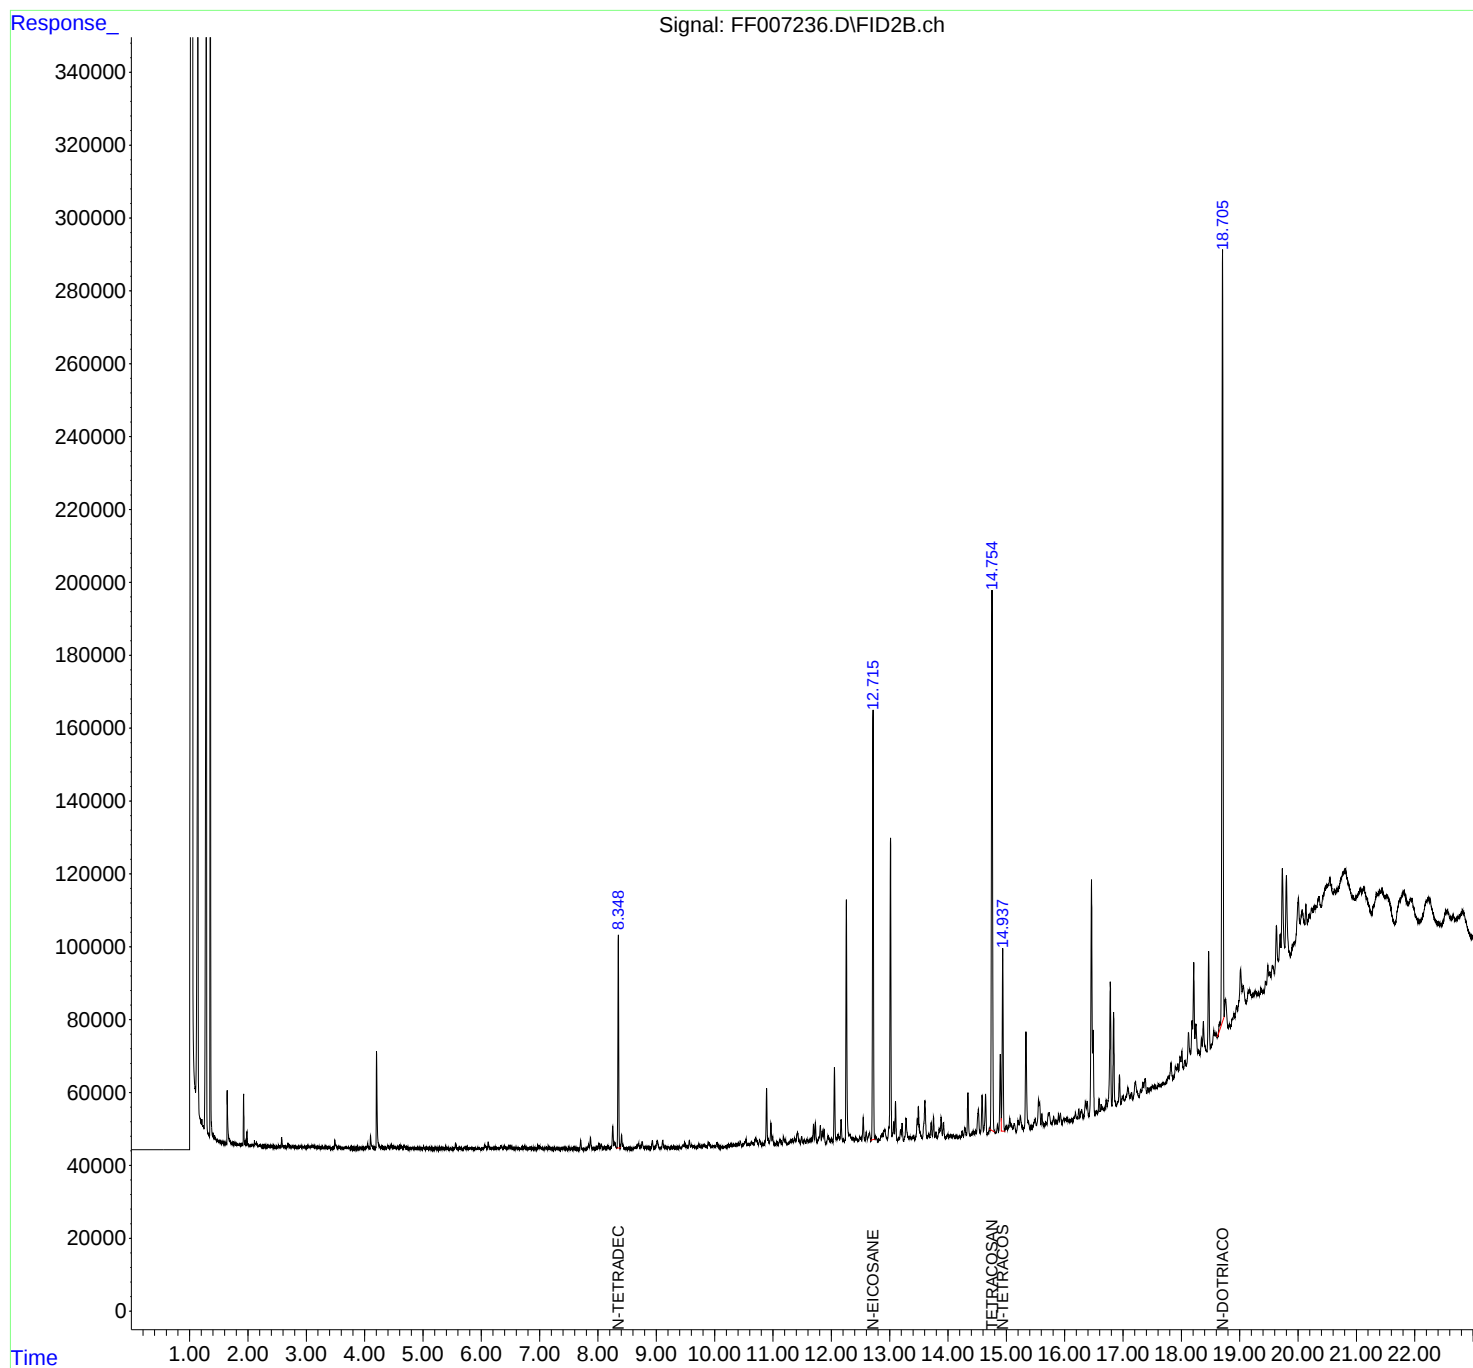


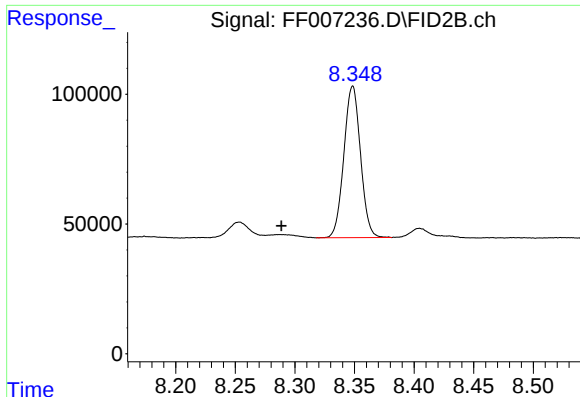

#4 N-TETRADECANE


R.T.: 8.349 min
Delta R.T.: 0.060 min
Response: 567496
Conc: 3.67 ug/ml

Instrument :
FID_F
ClientSampleId :

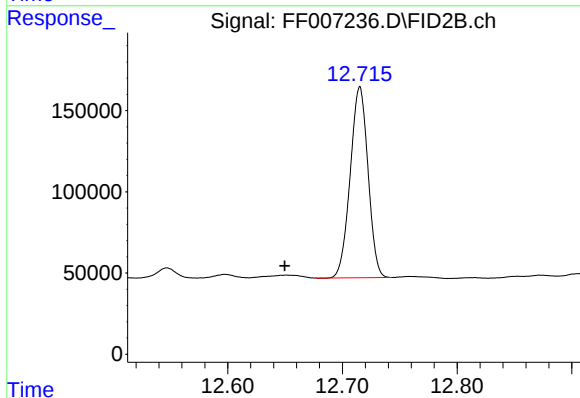


#7 N-EICOSANE

R.T.: 12.715 min
Delta R.T.: 0.066 min
Response: 1268537
Conc: 7.86 ug/ml

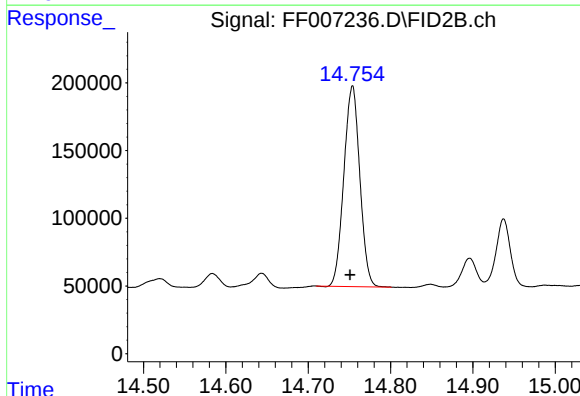


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.754 min
Delta R.T.: 0.003 min
Response: 1996030
Conc: 14.16 ug/ml

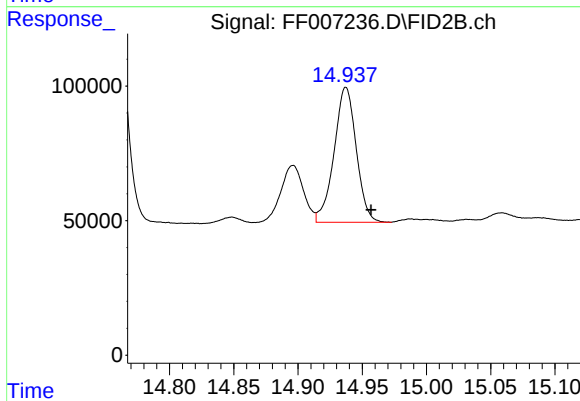

#10 N-TETRACOSANE

R.T.: 14.937 min
Delta R.T.: -0.019 min
Response: 602950
Conc: 3.68 ug/ml

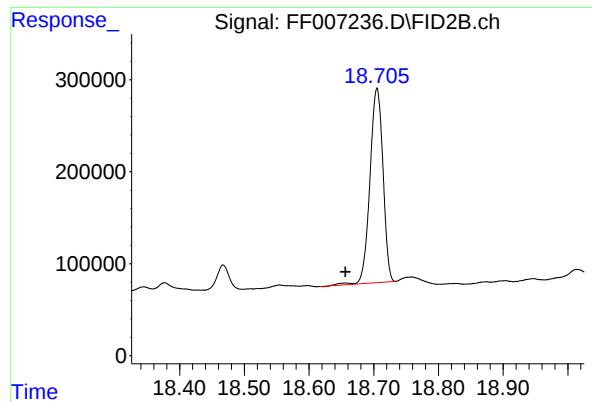

#14 N-DOTRIACONTANE

R.T.: 18.705 min
Delta R.T.: 0.049 min
Response: 2966789
Conc: 18.89 ug/ml

Instrument :
FID_F
ClientSampleId :