

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007238.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 17:37
Operator : DD\AJ
Sample : L3418-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 00:40:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.752	2403455	17.049 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.348f	611760	3.951 ug/ml
8)	N-DOCOSANE	13.815	308728	1.904 ug/ml
10)	N-TETRACOSANE	14.970	411479	2.513 ug/ml
13)	N-TRIACONTANE	17.824	363472	2.199 ug/ml
14)	N-DOTRIACONTANE	18.650	569099	3.624 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007238.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 17:37
Operator : DD\AJ
Sample : L3418-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 00:40:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

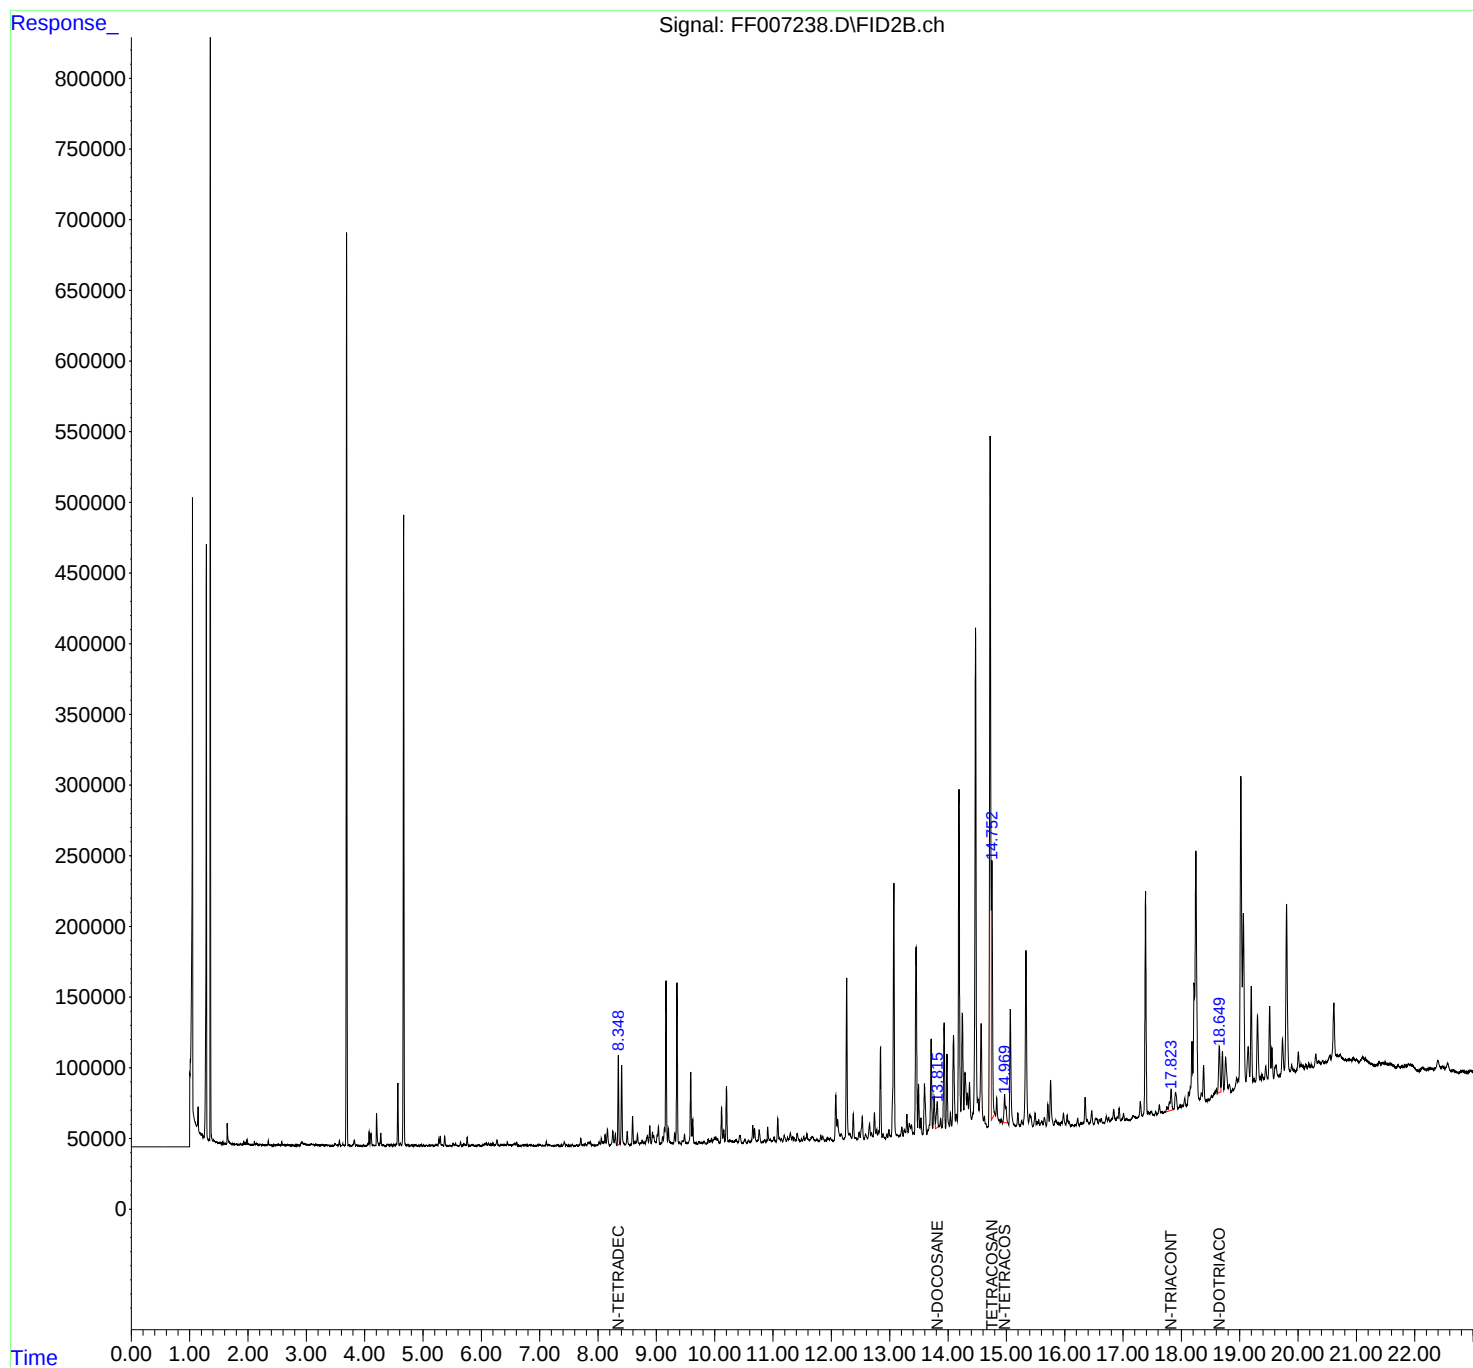


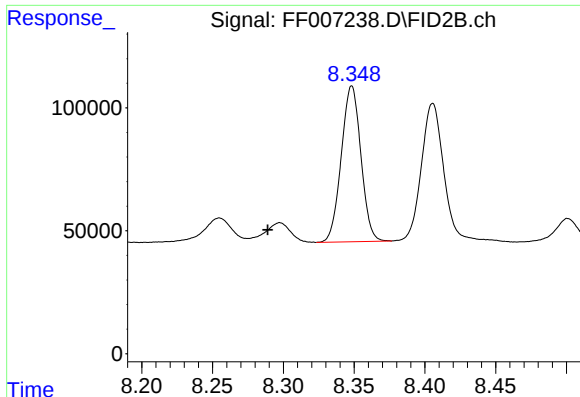

#4 N-TETRADECANE


R.T.: 8.348 min
Delta R.T.: 0.060 min
Response: 611760
Conc: 3.95 ug/ml

Instrument :
FID_F
ClientSampleId :

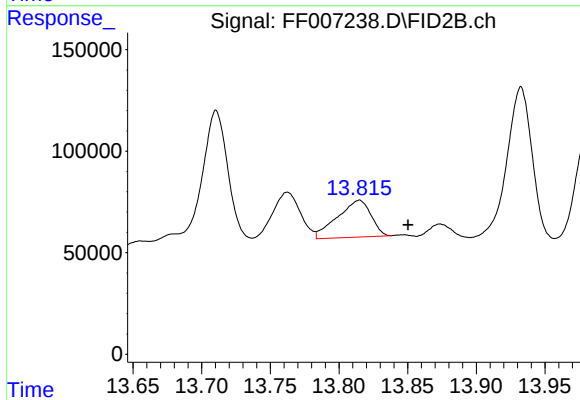


#8 N-DOCOSANE

R.T.: 13.815 min
Delta R.T.: -0.035 min
Response: 308728
Conc: 1.90 ug/ml

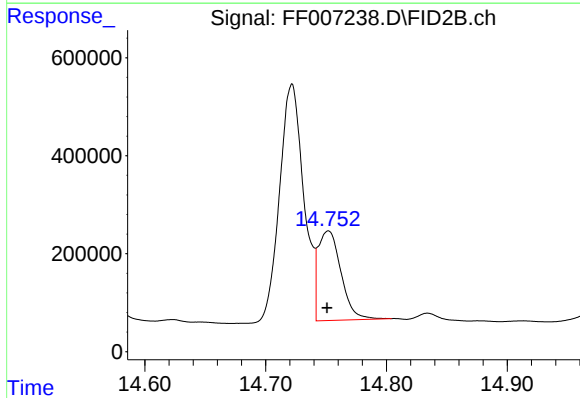


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.752 min
Delta R.T.: 0.001 min
Response: 2403455
Conc: 17.05 ug/ml

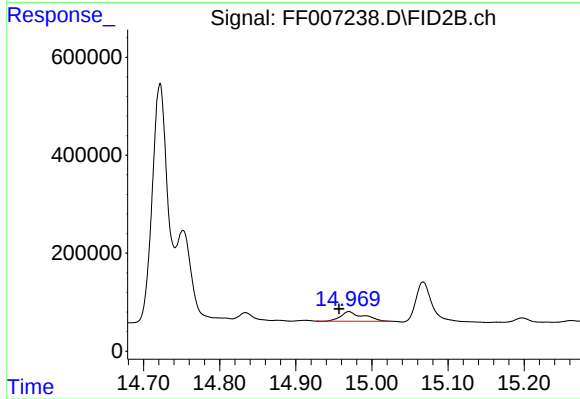

#10 N-TETRACOSANE


R.T.: 14.970 min
Delta R.T.: 0.013 min
Response: 411479
Conc: 2.51 ug/ml

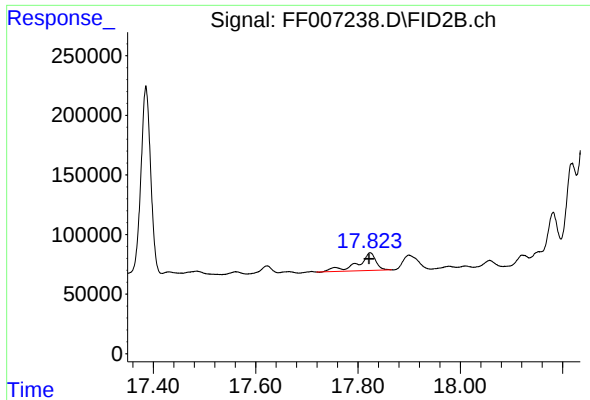

#13 N-TRIACONTANE

R.T.: 17.824 min
Delta R.T.: 0.002 min
Response: 363472
Conc: 2.20 ug/ml

Instrument :
FID_F
ClientSampleId :

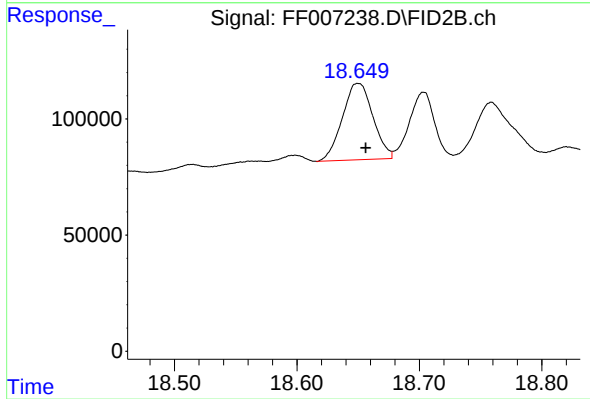

#14 N-DOTRIACONTANE

R.T.: 18.650 min
Delta R.T.: -0.006 min
Response: 569099
Conc: 3.62 ug/ml