

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
 Data File : FF007239.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jul 2020 18:08
 Operator : DD\AJ
 Sample : L3418-04
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 25 00:40:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.751	3521047	24.976 ug/ml
Target Compounds			
3) N-DODECANE	6.444	269069	1.732 ug/ml
4) N-TETRADECANE	8.297	174026	1.124 ug/ml
6) N-OCTADECANE	11.296	204996	1.272 ug/ml
7) N-EICOSANE	12.651	167515	1.037 ug/ml
8) N-DOCOSANE	13.814	939969	5.796 ug/ml
10) N-TETRACOSANE	14.995	4595312	28.059 ug/ml
11) N-HEXACOSANE	16.042f	441908	2.718 ug/ml
14) N-DOTRIACONTANE	18.652	1001303	6.376 ug/ml
15) N-TETRATRIACONTANE	19.446	798549	6.134 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007239.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 18:08
Operator : DD\AJ
Sample : L3418-04
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 00:40:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

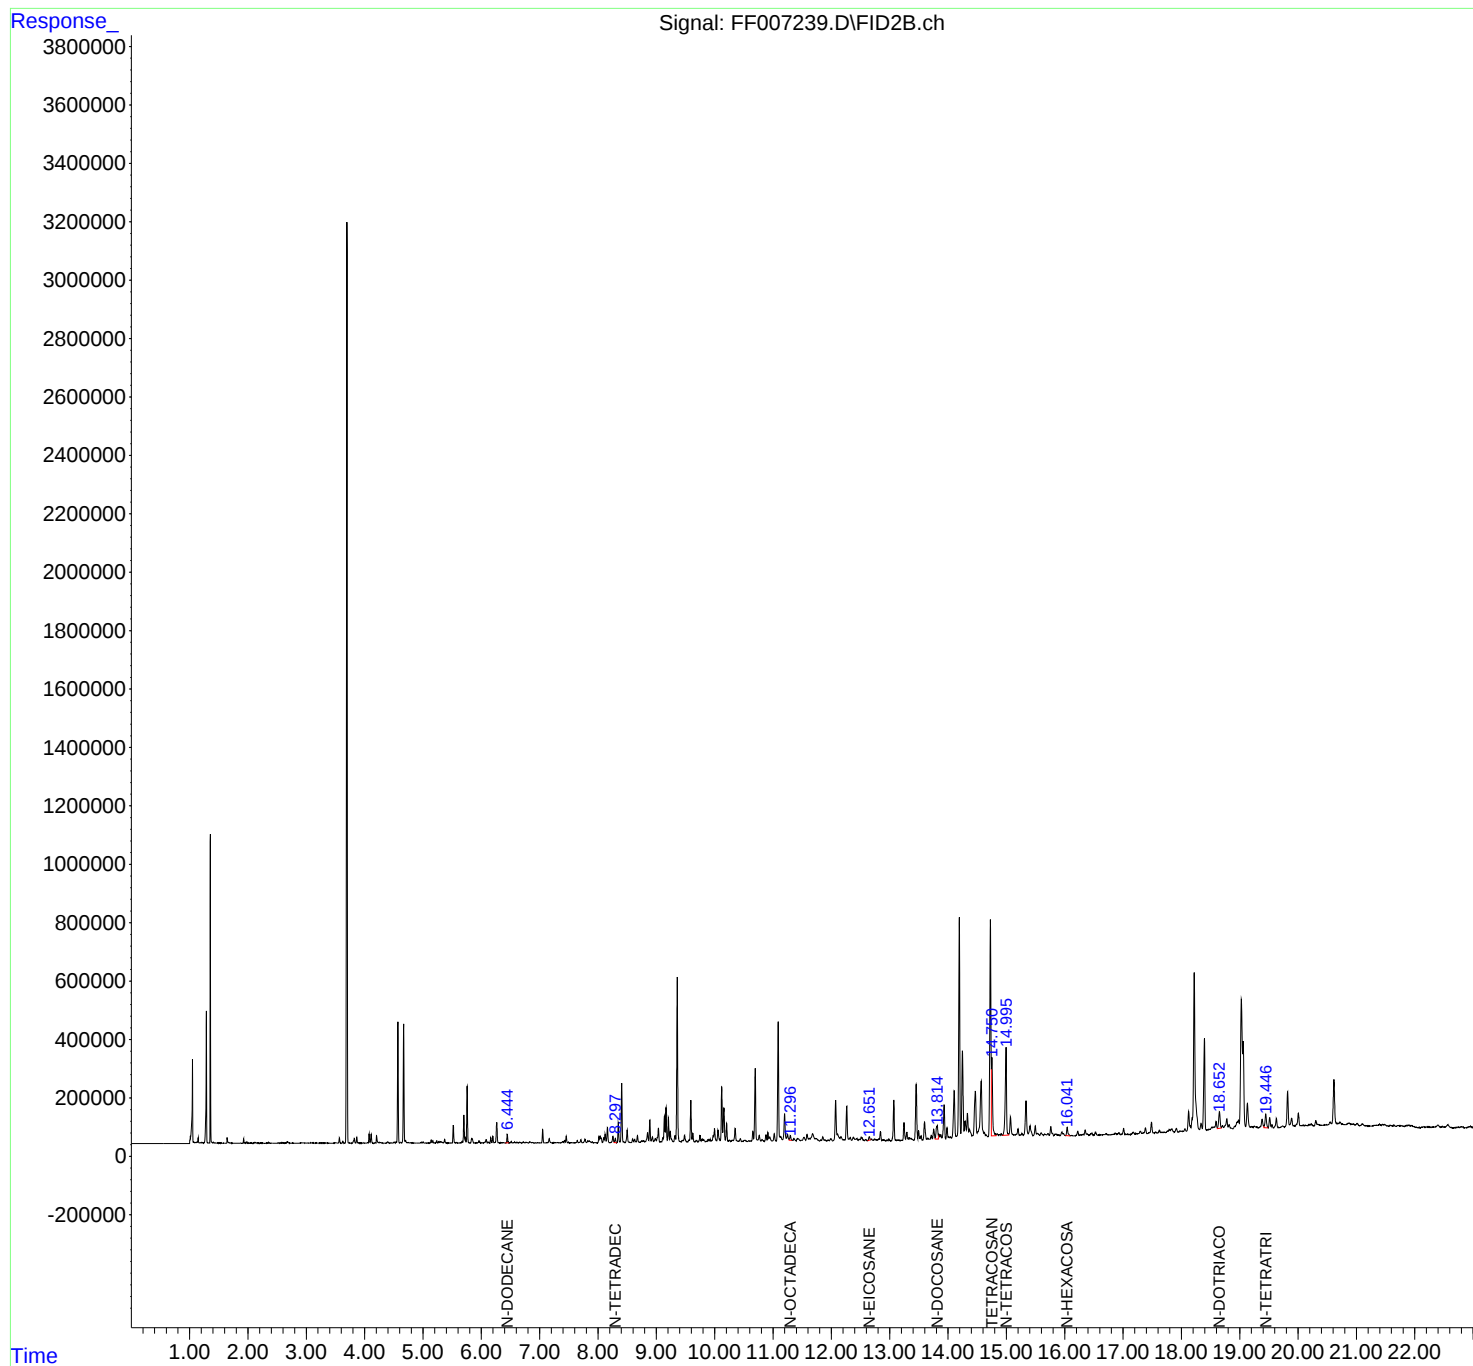


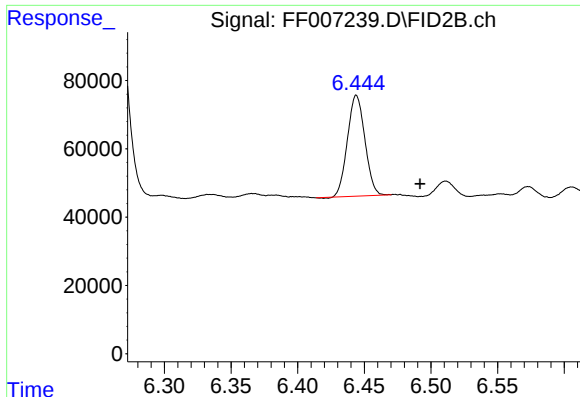

#3 N-DODECANE


R.T.: 6.444 min
Delta R.T.: -0.048 min
Response: 269069
Conc: 1.73 ug/ml

Instrument :
FID_F
ClientSampleId :

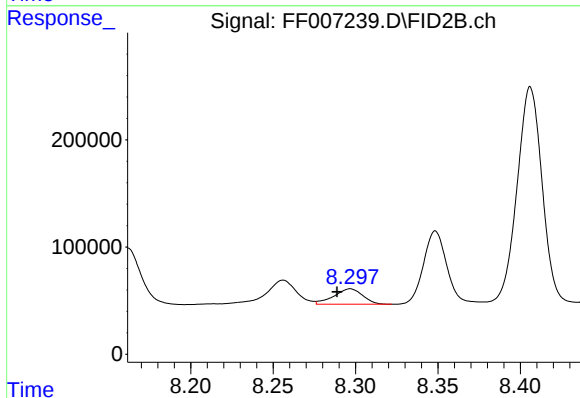


#4 N-TETRADECANE

R.T.: 8.297 min
Delta R.T.: 0.008 min
Response: 174026
Conc: 1.12 ug/ml

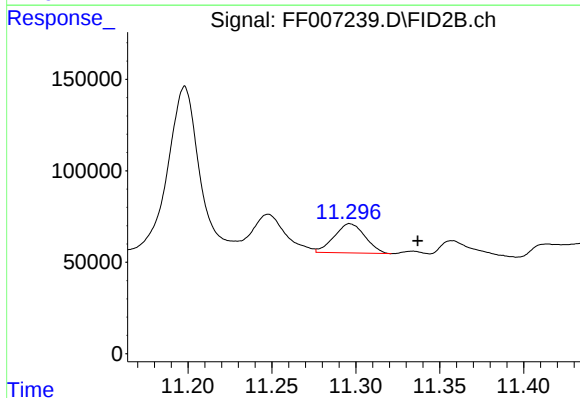


#6 N-OCTADECANE

R.T.: 11.296 min
Delta R.T.: -0.040 min
Response: 204996
Conc: 1.27 ug/ml

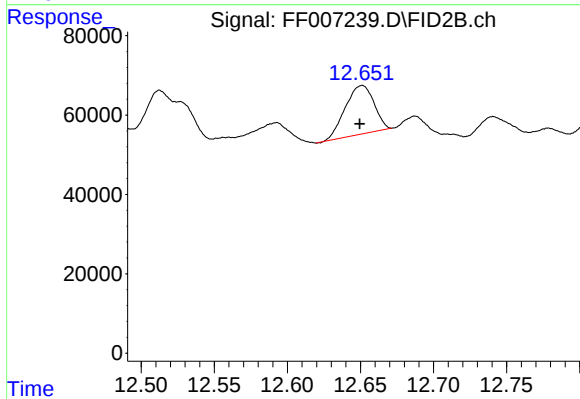

#7 N-EICOSANE


R.T.: 12.651 min
Delta R.T.: 0.002 min
Response: 167515
Conc: 1.04 ug/ml

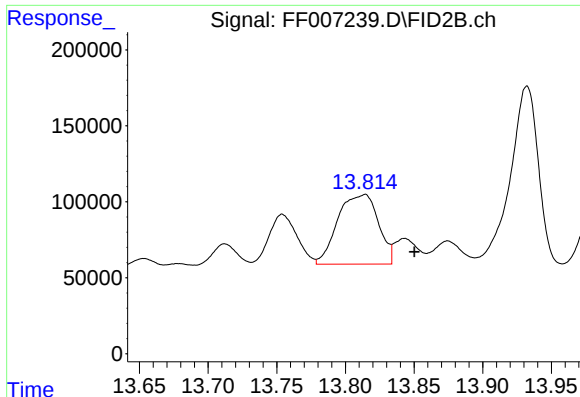

#8 N-DOCOSANE


R.T.: 13.814 min
Delta R.T.: -0.036 min
Response: 939969
Conc: 5.80 ug/ml

Instrument :
FID_F
ClientSampleId :

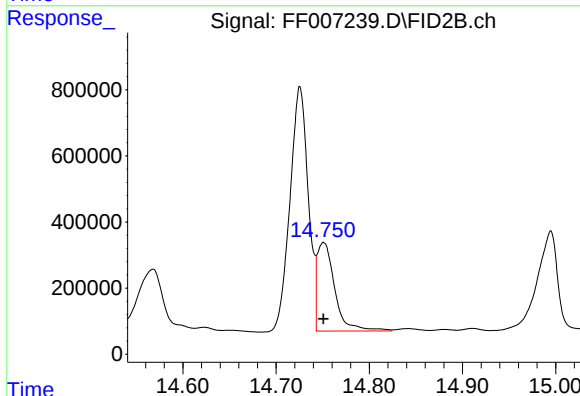


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.751 min
Delta R.T.: 0.000 min
Response: 3521047
Conc: 24.98 ug/ml

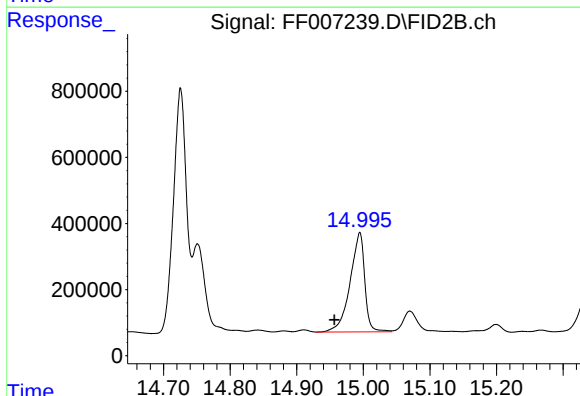


#10 N-TETRACOSANE

R.T.: 14.995 min
Delta R.T.: 0.038 min
Response: 4595312
Conc: 28.06 ug/ml

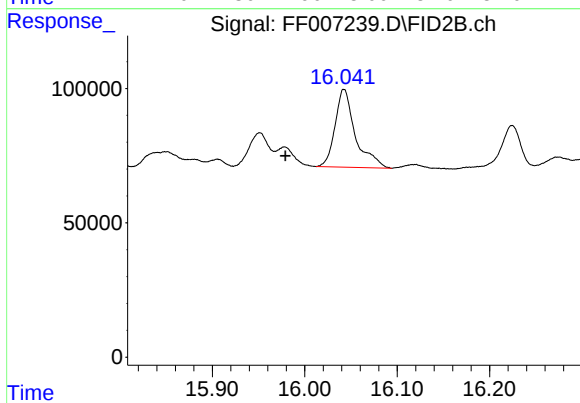

#11 N-HEXACOSANE


R.T.: 16.042 min
Delta R.T.: 0.063 min
Response: 441908
Conc: 2.72 ug/ml

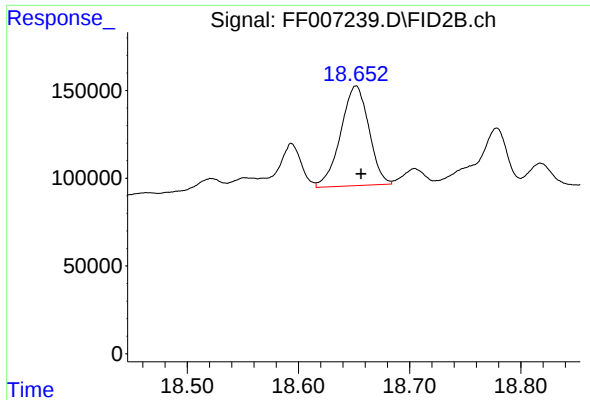

#14 N-DOTRIACONTANE

R.T.: 18.652 min
Delta R.T.: -0.005 min
Response: 1001303
Conc: 6.38 ug/ml

Instrument :
FID_F
ClientSampleId :

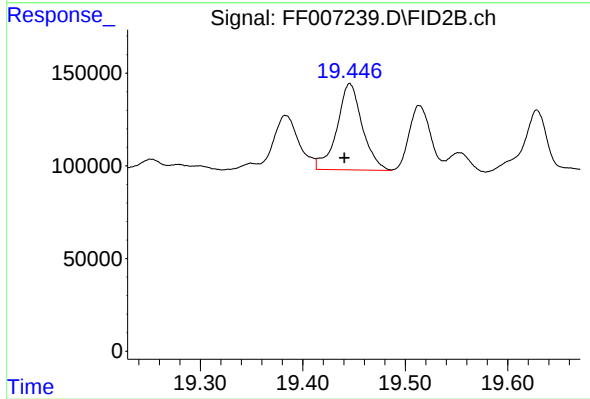

#15 N-TETRATRIACONTANE

R.T.: 19.446 min
Delta R.T.: 0.005 min
Response: 798549
Conc: 6.13 ug/ml