

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
 Data File : FF007244.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jul 2020 20:44
 Operator : DD\AJ
 Sample : L3418-07MSD
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 C0AF8MSD

Integration File: autoint1.e
 Quant Time: Jul 25 00:41:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	1756950	12.463 ug/ml
Target Compounds			
2) N-DECANE	4.463	2302346	14.968 ug/ml
3) N-DODECANE	6.489	2361734	15.205 ug/ml
4) N-TETRADECANE	8.287	2405156	15.534 ug/ml
5) N-HEXADECANE	9.890	2422039	15.363 ug/ml
6) N-OCTADECANE	11.334	2443865	15.161 ug/ml
7) N-EICOSANE	12.648	2419460	14.982 ug/ml
8) N-DOCOSANE	13.848	2408299	14.850 ug/ml
10) N-TETRACOSANE	14.955	2562230	15.645 ug/ml
11) N-HEXACOSANE	15.978	2247002	13.819 ug/ml
12) N-OCTACOSANE	16.931	2239895	13.669 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072420\
Data File : FF007244.D
Signal(s) : FID2B.ch
Acq On : 24 Jul 2020 20:44
Operator : DD\AJ
Sample : L3418-07MSD
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
C0AF8MSD

Integration File: autoint1.e
Quant Time: Jul 25 00:41:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

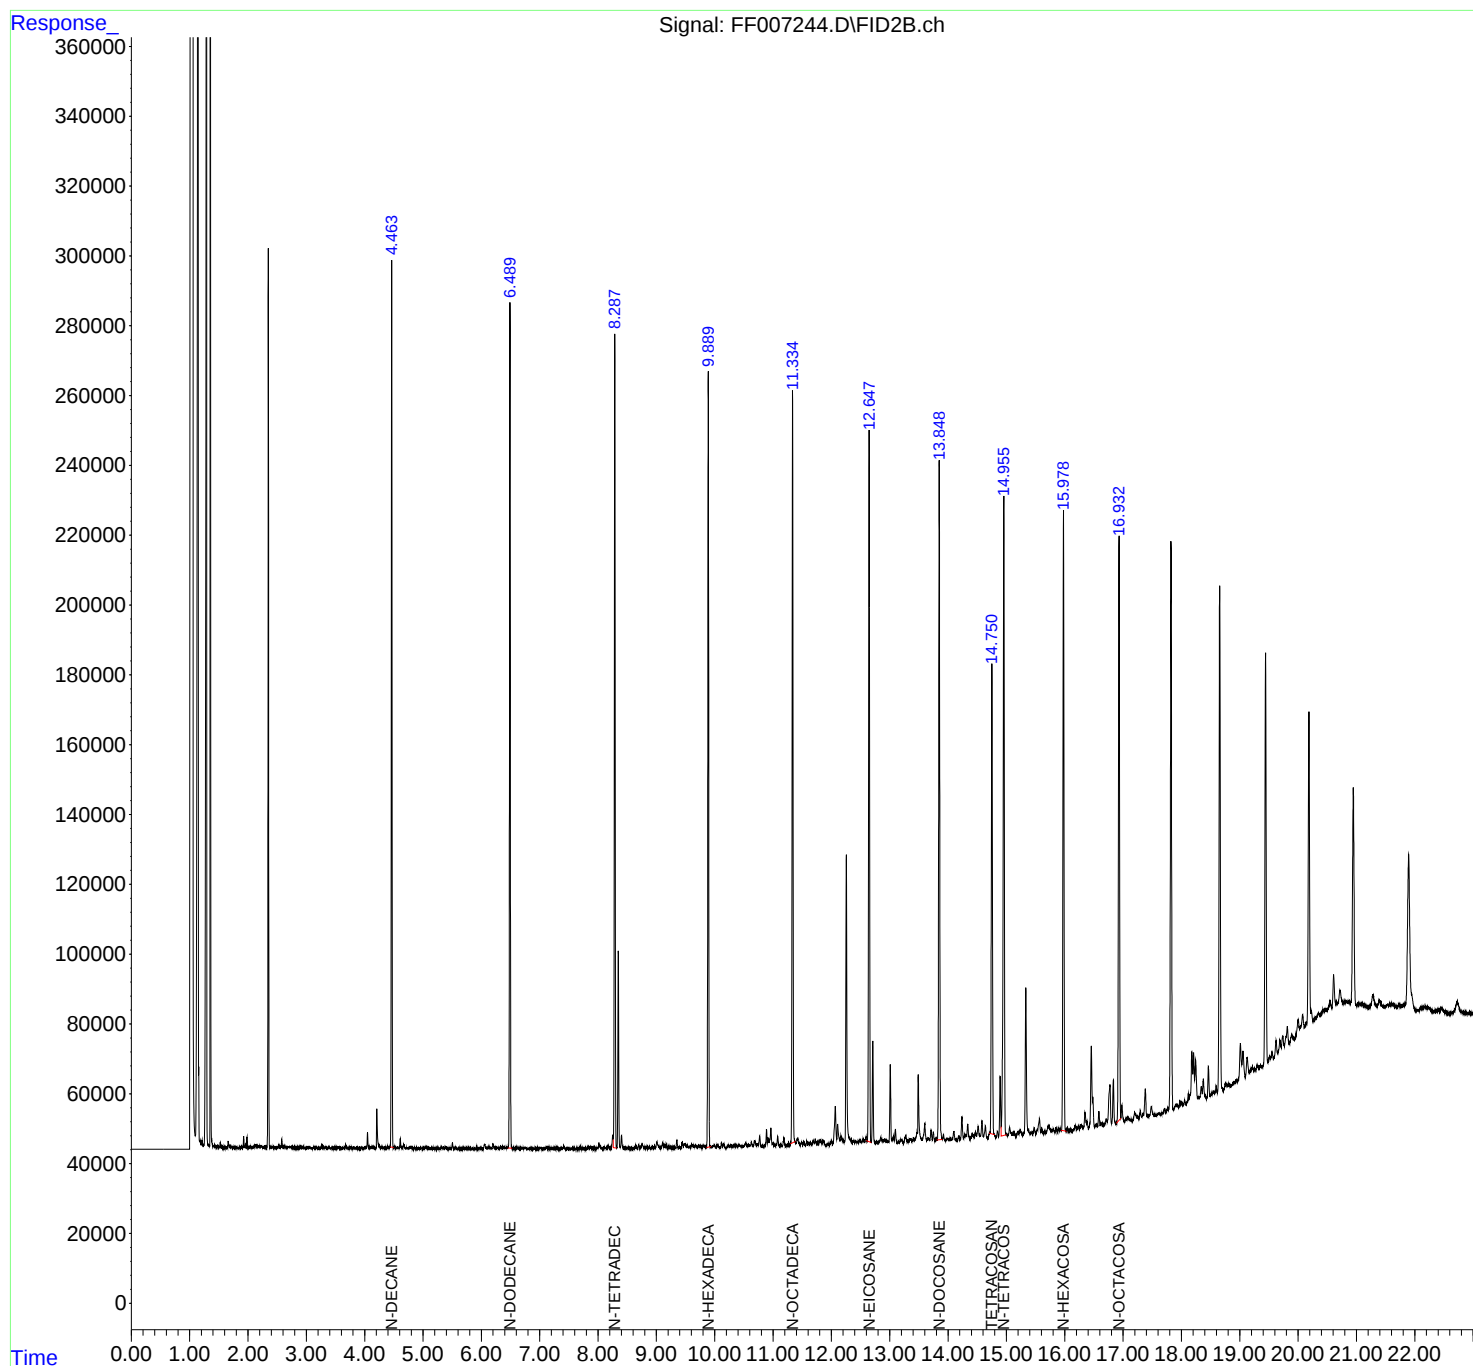


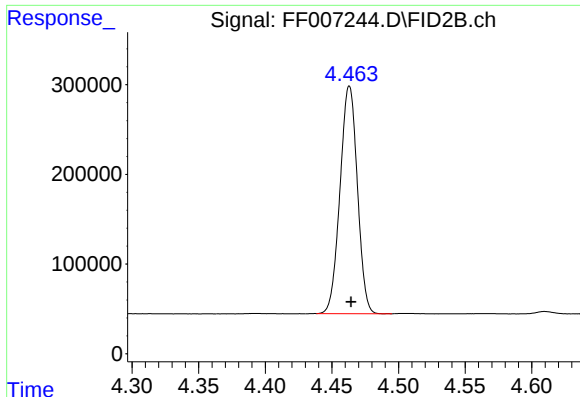

#2 N-DECANE


R.T.: 4.463 min
Delta R.T.: -0.001 min
Response: 2302346
Conc: 14.97 ug/ml

Instrument :
FID_F
ClientSampleId :
C0AF8MSD

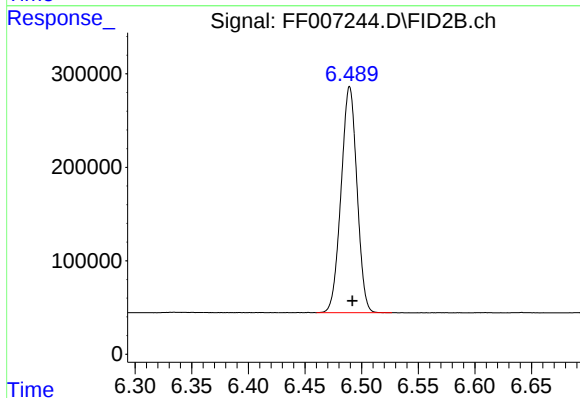


#3 N-DODECANE

R.T.: 6.489 min
Delta R.T.: -0.002 min
Response: 2361734
Conc: 15.20 ug/ml

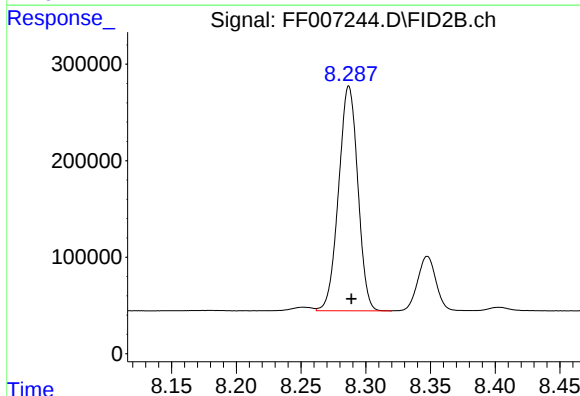


#4 N-TETRADECANE

R.T.: 8.287 min
Delta R.T.: -0.002 min
Response: 2405156
Conc: 15.53 ug/ml

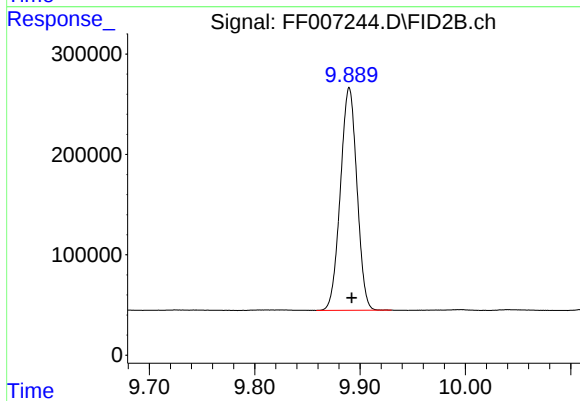

#5 N-HEXADECANE


R.T.: 9.890 min
Delta R.T.: -0.002 min
Response: 2422039
Conc: 15.36 ug/ml

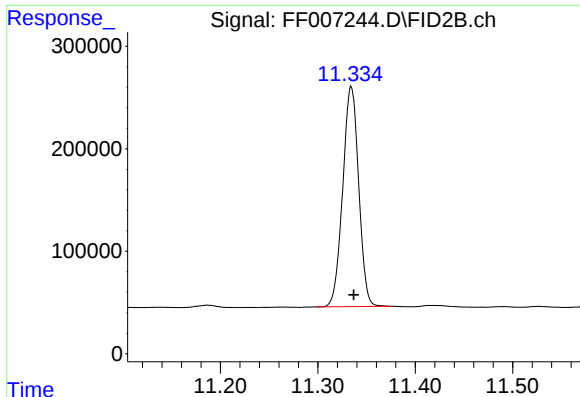

#6 N-OCTADECANE


R.T.: 11.334 min
Delta R.T.: -0.003 min
Response: 2443865
Conc: 15.16 ug/ml

Instrument :
FID_F
ClientSampleId :
C0AF8MSD

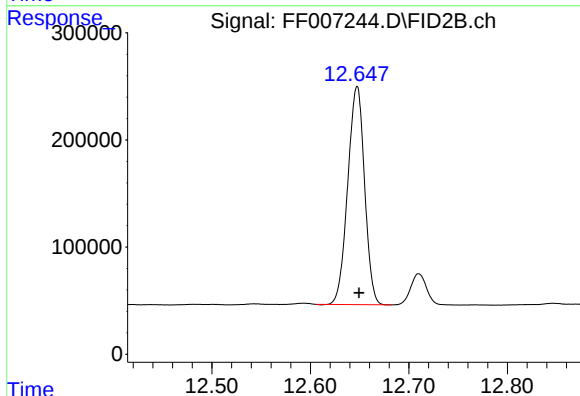


#7 N-EICOSANE

R.T.: 12.648 min
Delta R.T.: -0.002 min
Response: 2419460
Conc: 14.98 ug/ml

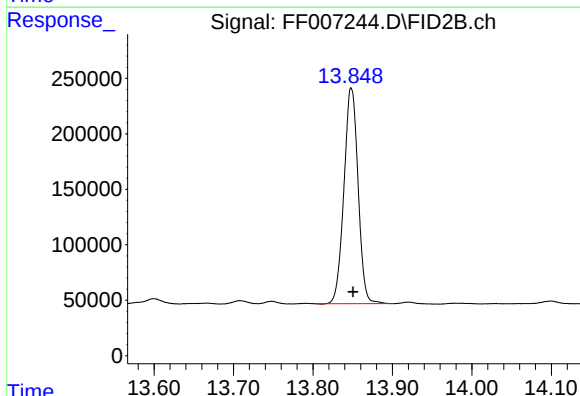


#8 N-DOCOSANE

R.T.: 13.848 min
Delta R.T.: -0.002 min
Response: 2408299
Conc: 14.85 ug/ml

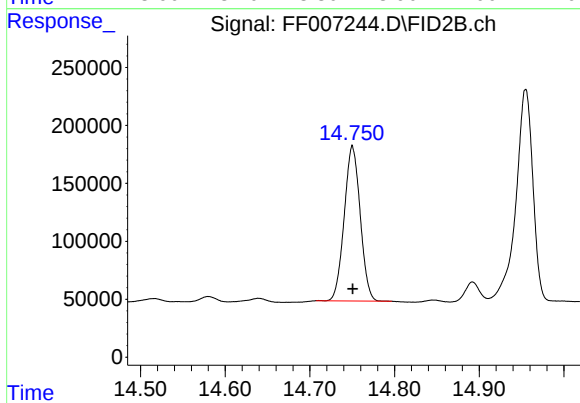

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.750 min
Delta R.T.: 0.000 min
Response: 1756950
Conc: 12.46 ug/ml

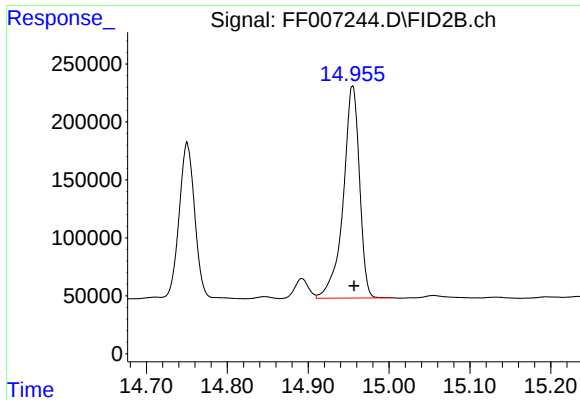

#10 N-TETRACOSANE


R.T.: 14.955 min
Delta R.T.: -0.002 min
Response: 2562230
Conc: 15.65 ug/ml

Instrument :
FID_F
ClientSampleId :
C0AF8MSD

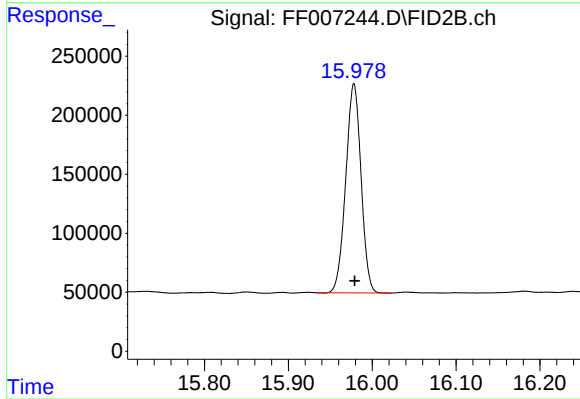

#11 N-HEXACOSANE

R.T.: 15.978 min
Delta R.T.: 0.000 min
Response: 2247002
Conc: 13.82 ug/ml

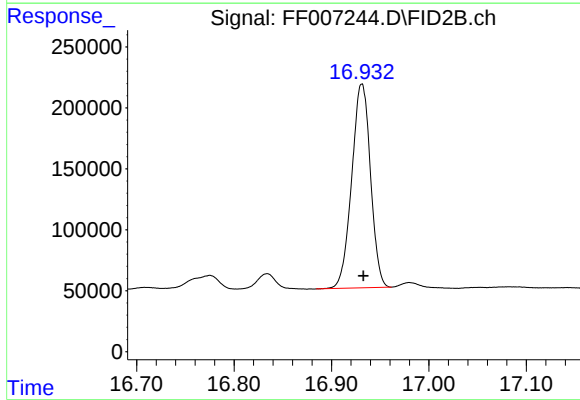

#12 N-OCTACOSANE

R.T.: 16.931 min
Delta R.T.: -0.001 min
Response: 2239895
Conc: 13.67 ug/ml