

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072518\
 Data File : FF001491.D
 Signal(s) : FID2B.ch
 Acq On : 25 Jul 2018 18:57
 Operator : AJ\SJ
 Sample : J4135-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 26 08:09:26 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.443	1528169	14.186 ug/ml
Target Compounds			
4) N-TETRADECANE	8.071	322113	2.561 ug/ml
7) N-EICOSANE	12.348	112434	0.904 ug/ml
8) N-DOCOSANE	13.566	197260	1.600 ug/ml
10) N-TETRACOSANE	14.621	946665	7.765 ug/ml
11) N-HEXACOSANE	15.708	125750	1.037 ug/ml
12) N-OCTACOSANE	16.623	610478	5.067 ug/ml
13) N-TRIACONTANE	17.490	499953	4.159 ug/ml
14) N-DOTRIACONTANE	18.322	538705	4.569 ug/ml
15) N-TETRATRIACONTANE	19.119	187626	1.596 ug/ml
16) N-HEXATRIACONTANE	19.853	191812	1.689 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072518\
Data File : FF001491.D
Signal(s) : FID2B.ch
Acq On : 25 Jul 2018 18:57
Operator : AJ\SJ
Sample : J4135-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 26 08:09:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

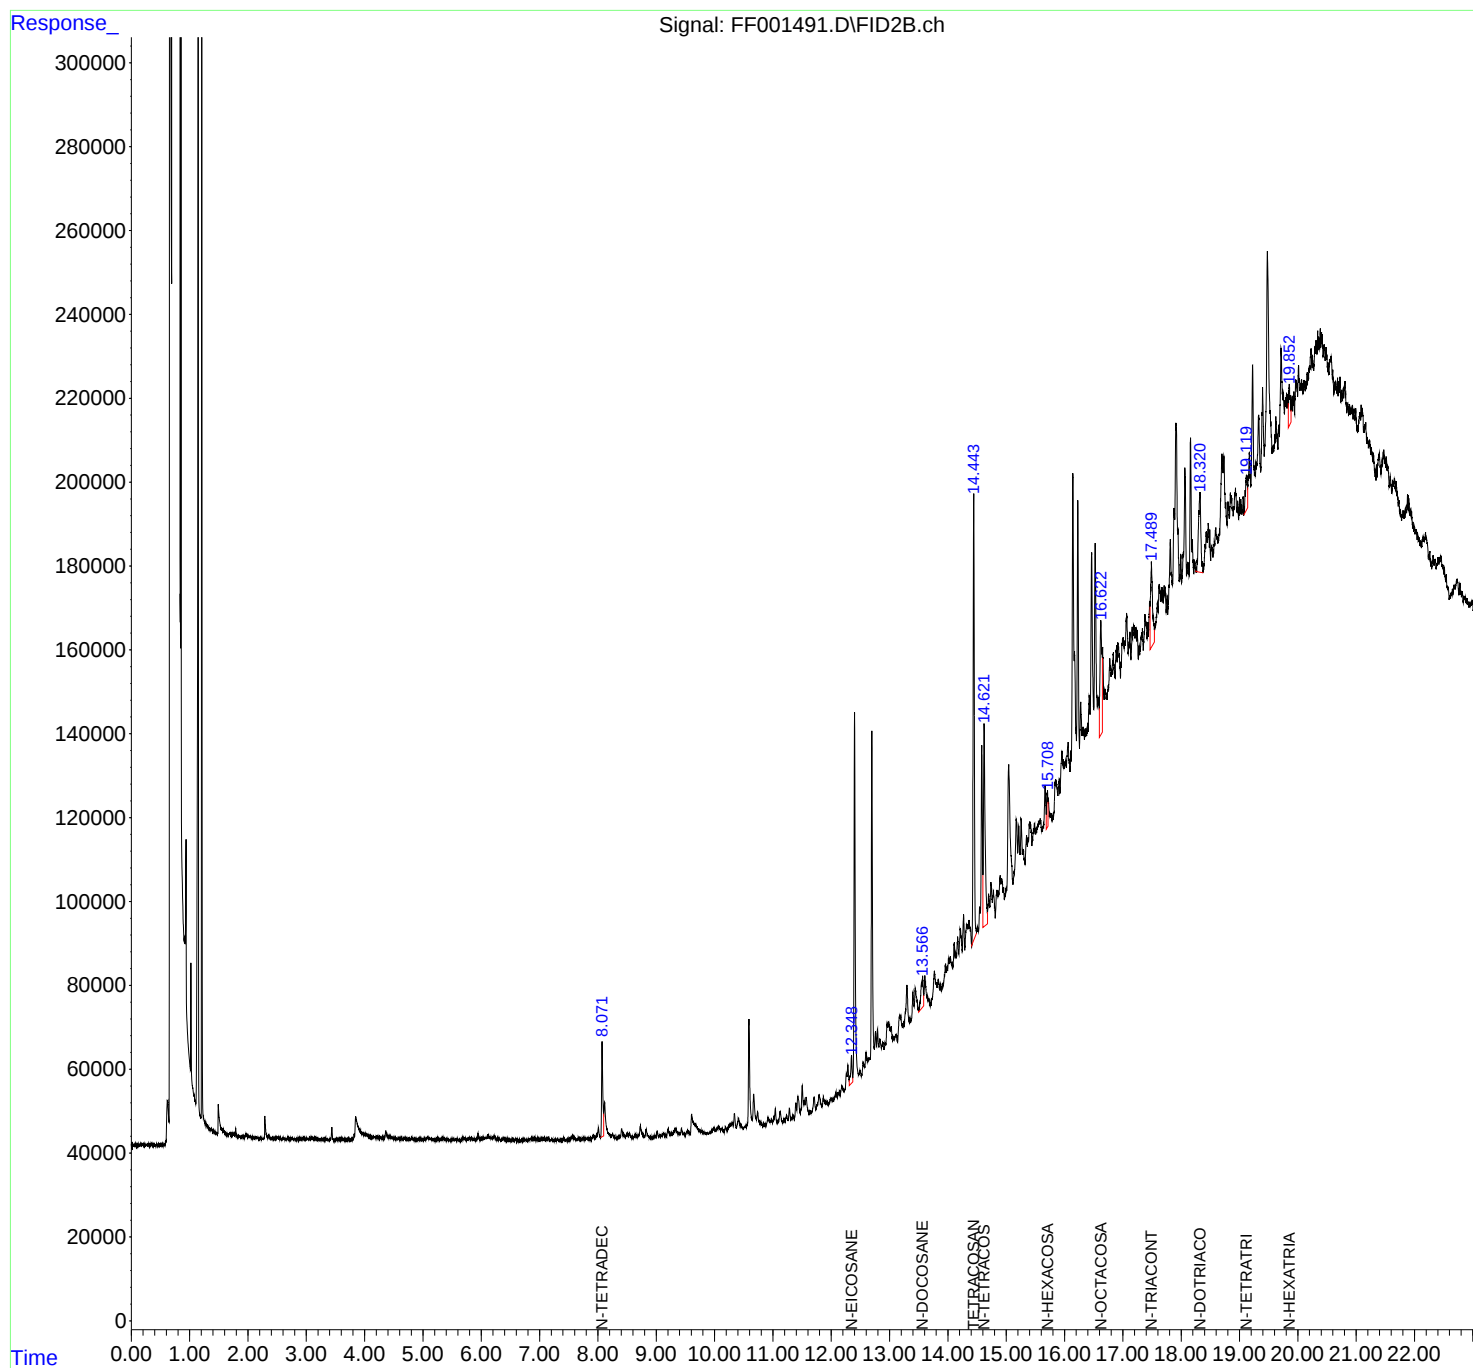

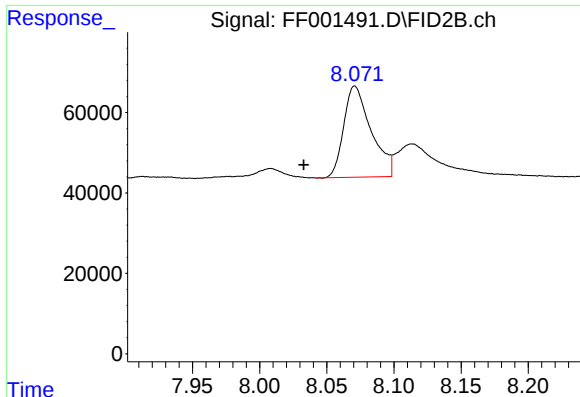


#4 N-TETRADECANE

R.T.: 8.071 min
Delta R.T.: 0.038 min
Response: 322113
Conc: 2.56 ug/ml

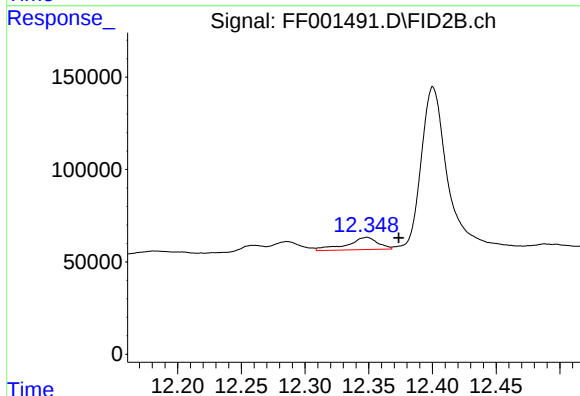


#7 N-EICOSANE

R.T.: 12.348 min
Delta R.T.: -0.025 min
Response: 112434
Conc: 0.90 ug/ml

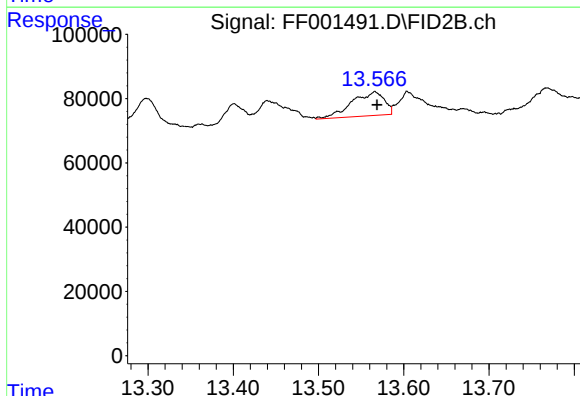


#8 N-DOCOSANE

R.T.: 13.566 min
Delta R.T.: -0.002 min
Response: 197260
Conc: 1.60 ug/ml

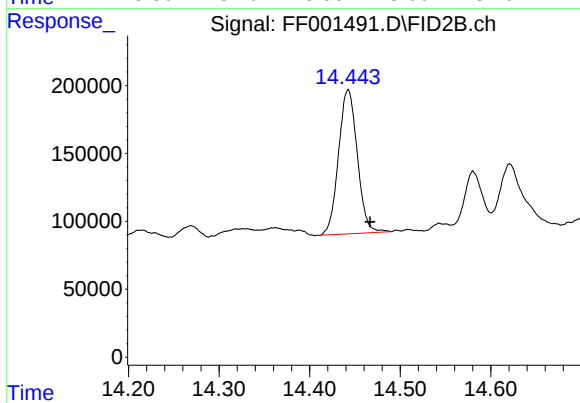


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.443 min
Delta R.T.: -0.024 min
Response: 1528169
Conc: 14.19 ug/ml

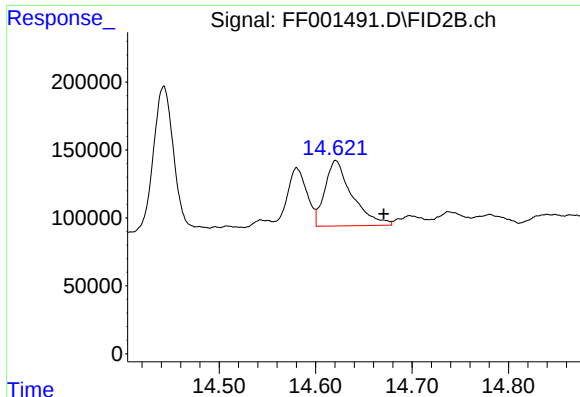


#10 N-TETRACOSANE

R.T.: 14.621 min
Delta R.T.: -0.050 min
Response: 946665
Conc: 7.77 ug/ml

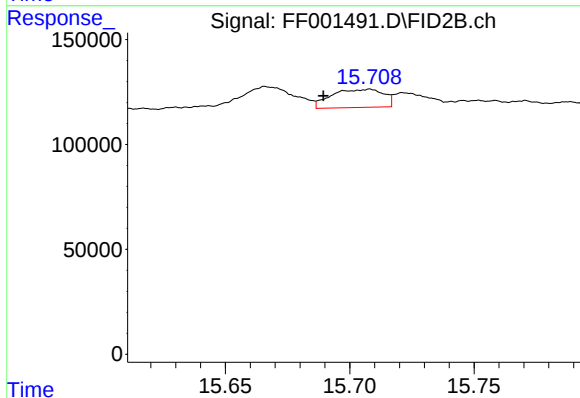


#11 N-HEXACOSANE

R.T.: 15.708 min
Delta R.T.: 0.019 min
Response: 125750
Conc: 1.04 ug/ml

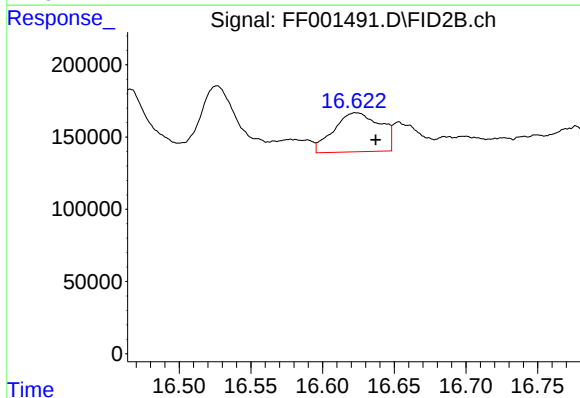


#12 N-OCTACOSANE

R.T.: 16.623 min
Delta R.T.: -0.014 min
Response: 610478
Conc: 5.07 ug/ml

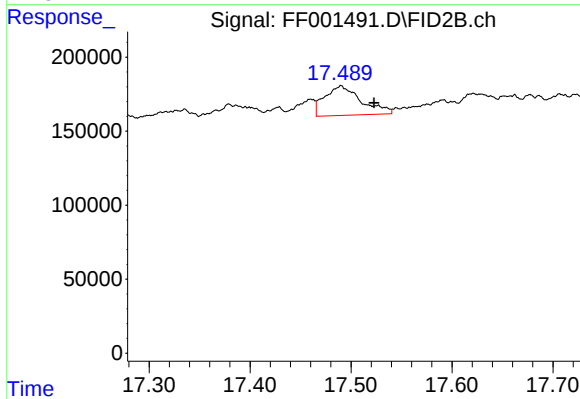


#13 N-TRIACONTANE

R.T.: 17.490 min
Delta R.T.: -0.033 min
Response: 499953
Conc: 4.16 ug/ml

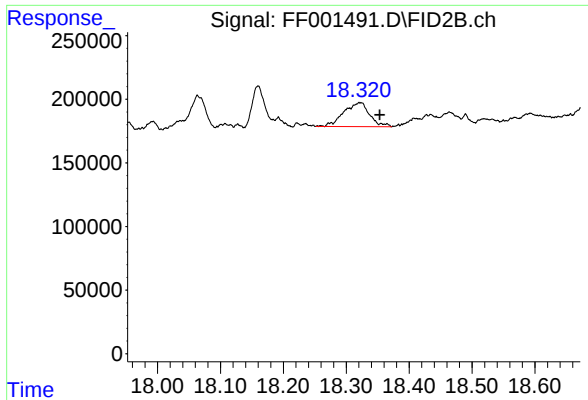


#14 N-DOTRIACONTANE

R.T.: 18.322 min
Delta R.T.: -0.032 min
Response: 538705
Conc: 4.57 ug/ml

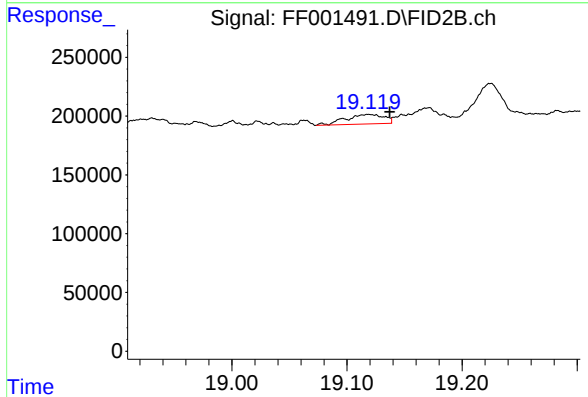

#15 N-TETRATRIACONTANE

R.T.: 19.119 min
Delta R.T.: -0.018 min
Response: 187626
Conc: 1.60 ug/ml

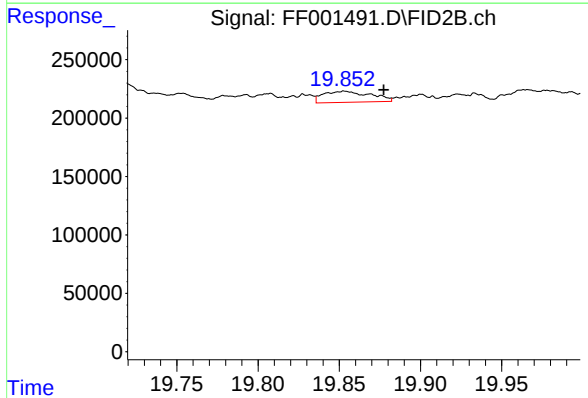

#16 N-HEXATRIACONTANE

R.T.: 19.853 min
Delta R.T.: -0.024 min
Response: 191812
Conc: 1.69 ug/ml