

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072518\
 Data File : FF001493.D
 Signal(s) : FID2B.ch
 Acq On : 25 Jul 2018 19:58
 Operator : AJ\SJ
 Sample : J4126-03 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 26 08:09:42 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.442	370641	3.441 ug/ml
Target Compounds			
4) N-TETRADECANE	8.074	71955	0.572 ug/ml
7) N-EICOSANE	12.402	1162438	9.345 ug/ml
10) N-TETRACOSANE	14.691	307584	2.523 ug/ml
12) N-OCTACOSANE	16.625	237784	1.974 ug/ml
13) N-TRIACONTANE	17.495	182692	1.520 ug/ml
14) N-DOTRIACONTANE	18.328	408784	3.467 ug/ml
15) N-TETRATRIACONTANE	19.114	171333	1.458 ug/ml
16) N-HEXATRIACONTANE	19.852	381577	3.359 ug/ml
17) N-OCTATRIACONTANE	20.561	151117	1.464 ug/ml
18) N-TETRACONTANE	21.382	157539	1.538 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072518\
Data File : FF001493.D
Signal(s) : FID2B.ch
Acq On : 25 Jul 2018 19:58
Operator : AJ\SJ
Sample : J4126-03 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 26 08:09:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

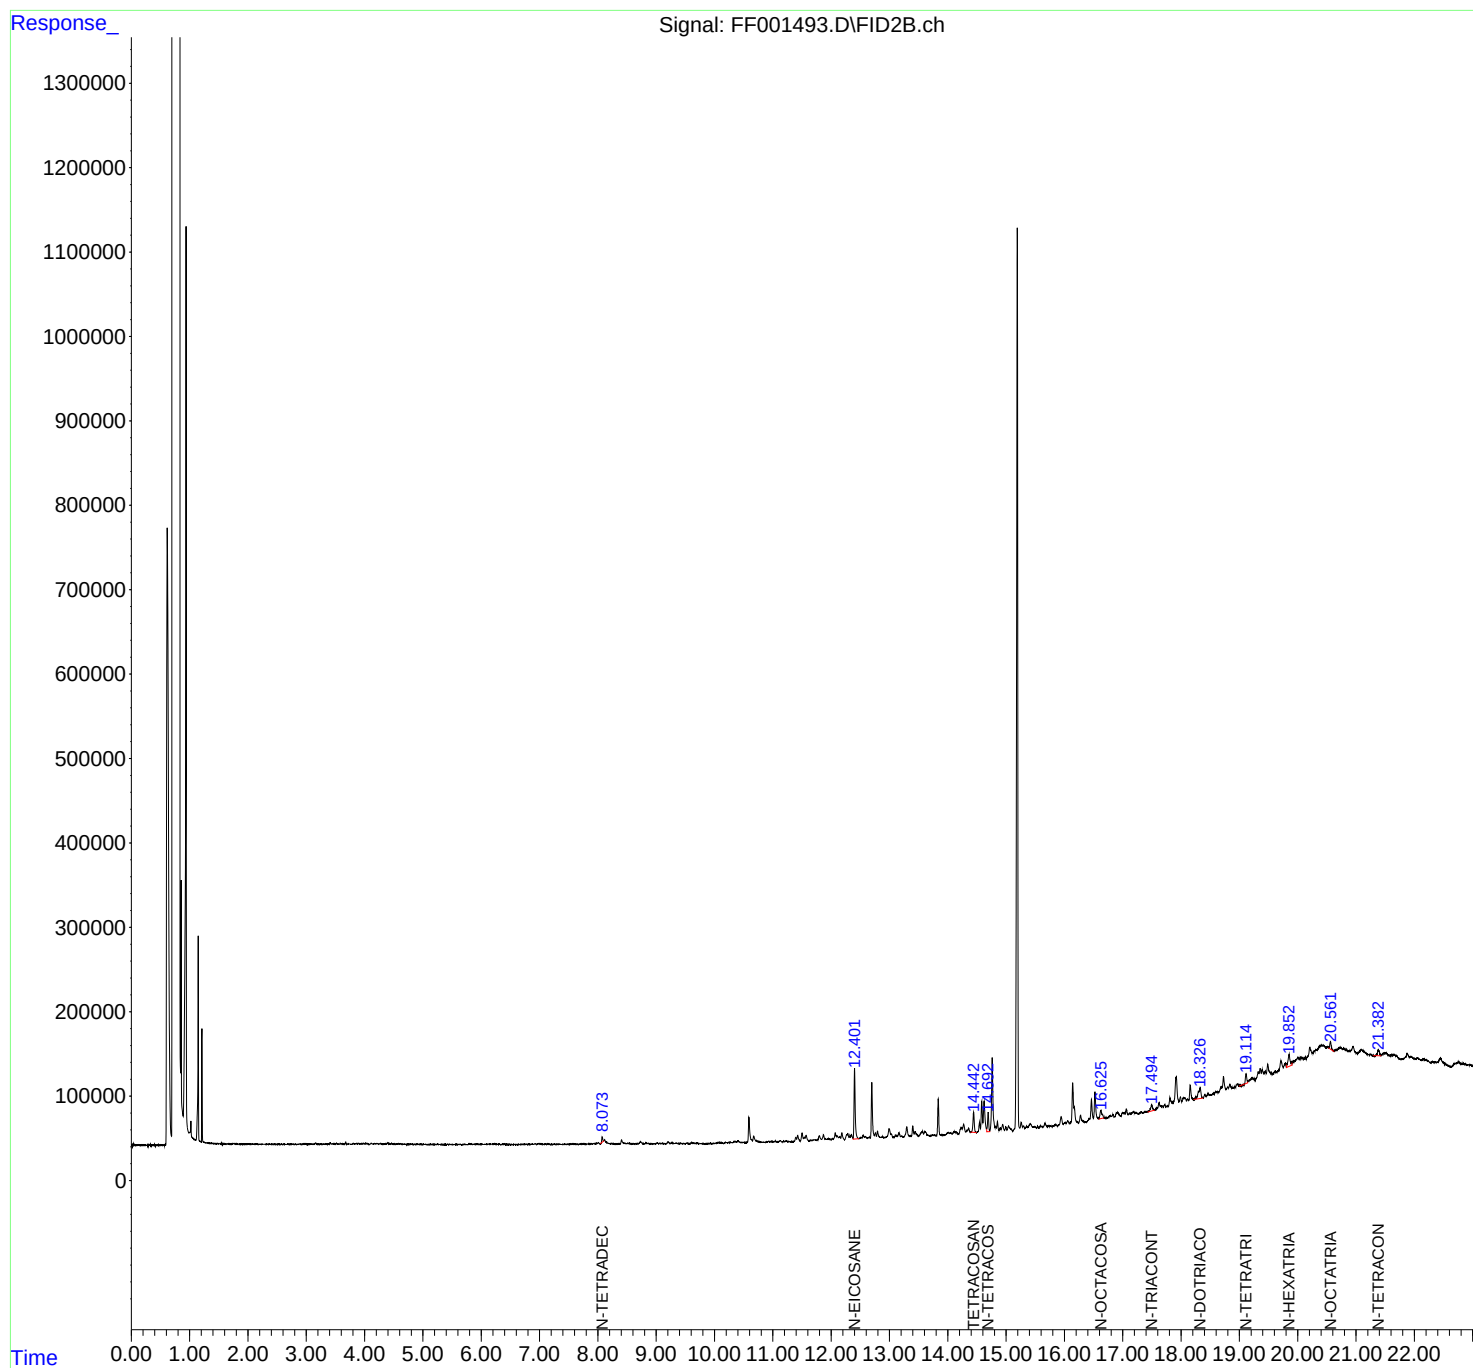

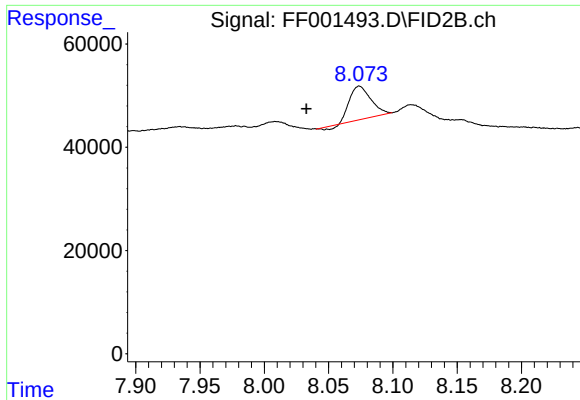


#4 N-TETRADECANE

R.T.: 8.074 min
Delta R.T.: 0.041 min
Response: 71955
Conc: 0.57 ug/ml

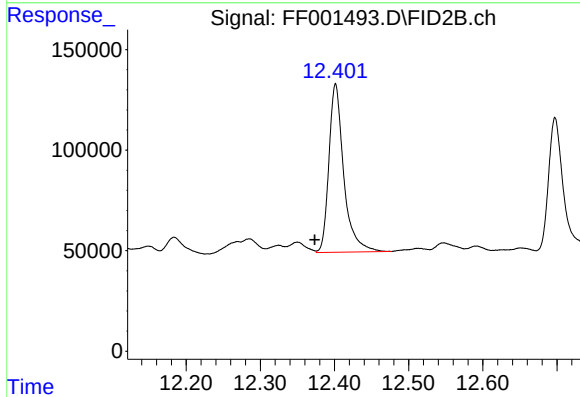


#7 N-EICOSANE

R.T.: 12.402 min
Delta R.T.: 0.028 min
Response: 1162438
Conc: 9.35 ug/ml

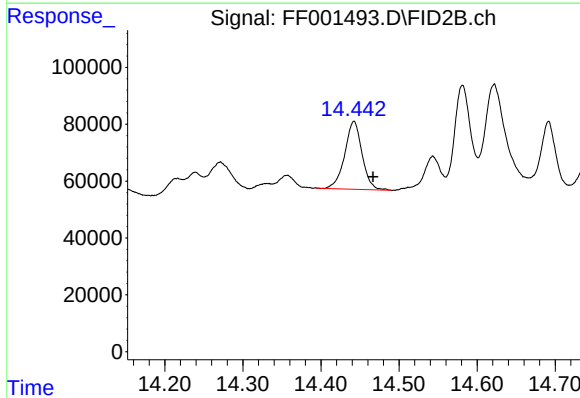


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.442 min
Delta R.T.: -0.024 min
Response: 370641
Conc: 3.44 ug/ml

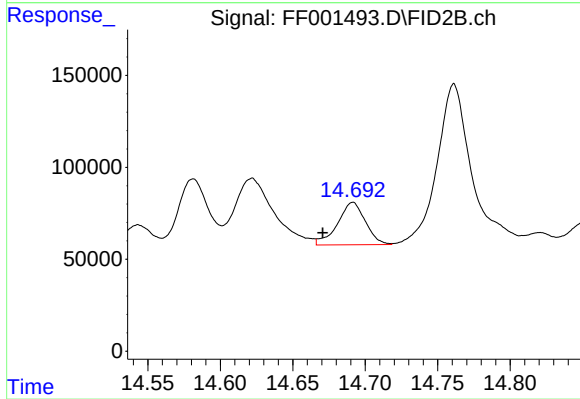


#10 N-TETRACOSANE

R.T.: 14.691 min
Delta R.T.: 0.021 min
Response: 307584
Conc: 2.52 ug/ml

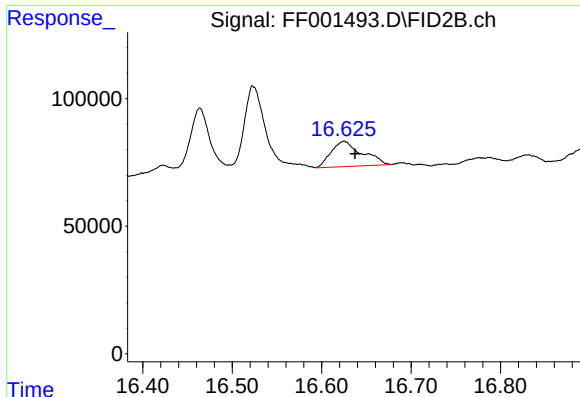


#12 N-OCTACOSANE

R.T.: 16.625 min
Delta R.T.: -0.012 min
Response: 237784
Conc: 1.97 ug/ml

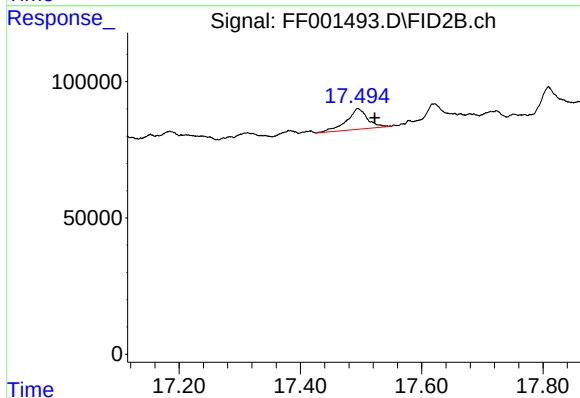


#13 N-TRIACONTANE

R.T.: 17.495 min
Delta R.T.: -0.028 min
Response: 182692
Conc: 1.52 ug/ml

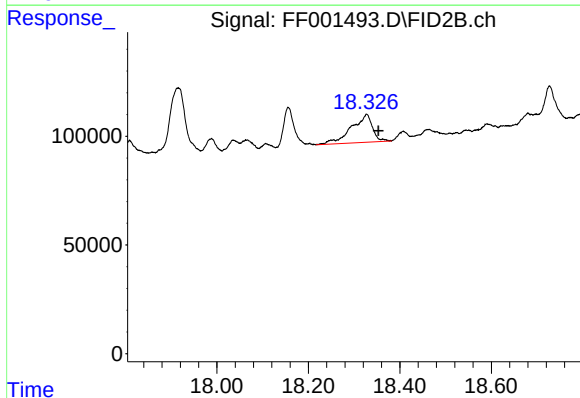


#14 N-DOTRIACONTANE

R.T.: 18.328 min
Delta R.T.: -0.026 min
Response: 408784
Conc: 3.47 ug/ml

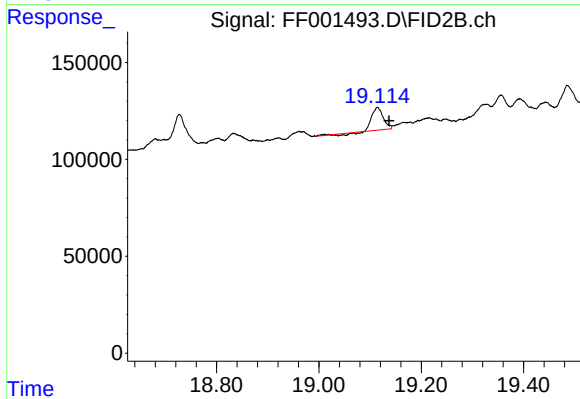


#15 N-TETRATRIACONTANE

R.T.: 19.114 min
Delta R.T.: -0.023 min
Response: 171333
Conc: 1.46 ug/ml

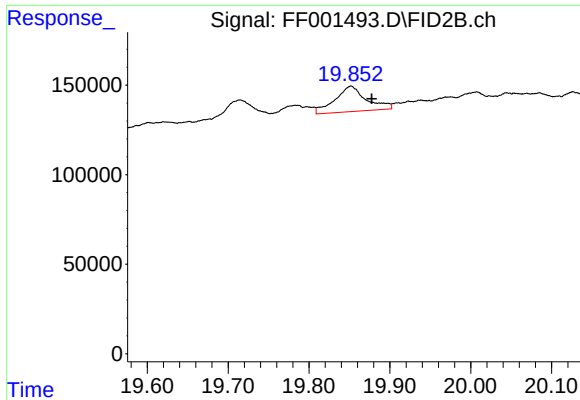


#16 N-HEXATRIACONTANE

R.T.: 19.852 min
Delta R.T.: -0.025 min
Response: 381577
Conc: 3.36 ug/ml

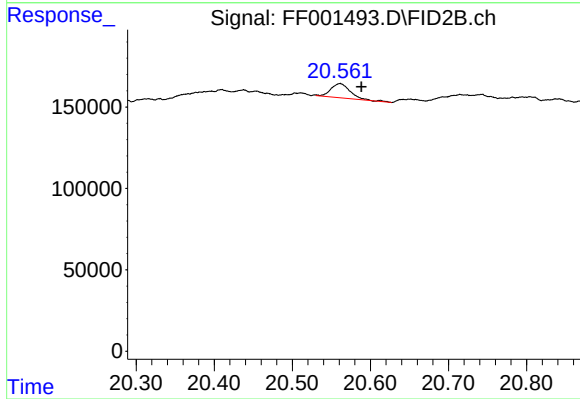

#17 N-OCTATRIACONTANE

R.T.: 20.561 min
Delta R.T.: -0.028 min
Response: 151117
Conc: 1.46 ug/ml

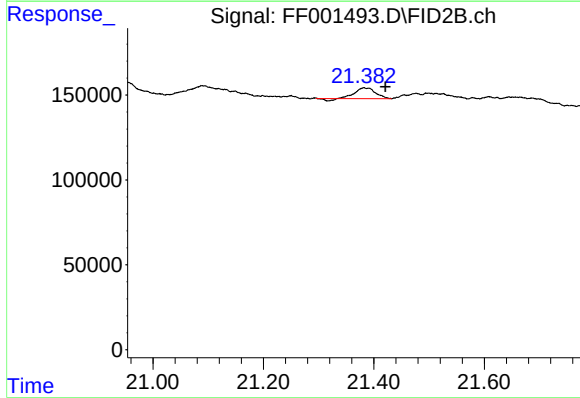

#18 N-TETRACONTANE

R.T.: 21.382 min
Delta R.T.: -0.039 min
Response: 157539
Conc: 1.54 ug/ml