

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072518\
 Data File : FF001497.D
 Signal(s) : FID2B.ch
 Acq On : 25 Jul 2018 22:00
 Operator : AJ\SJ
 Sample : J4126-11 5X
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 26 08:10:12 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.442	629470	5.843 ug/ml
Target Compounds			
4) N-TETRADECANE	7.990	224170	1.782 ug/ml
6) N-OCTADECANE	11.117f	681609	5.439 ug/ml
7) N-EICOSANE	12.348	289667	2.329 ug/ml
8) N-DOCOSANE	13.562	608933	4.938 ug/ml
10) N-TETRACOSANE	14.618f	2825310	23.176 ug/ml
11) N-HEXACOSANE	15.646	294270	2.428 ug/ml
12) N-OCTACOSANE	16.621	539035	4.474 ug/ml
13) N-TRIACONTANE	17.495	247557	2.059 ug/ml
14) N-DOTRIACONTANE	18.289f	1275665	10.820 ug/ml
16) N-HEXATRIACONTANE	19.845	421710	3.712 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072518\
Data File : FF001497.D
Signal(s) : FID2B.ch
Acq On : 25 Jul 2018 22:00
Operator : AJ\SJ
Sample : J4126-11 5X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 26 08:10:12 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

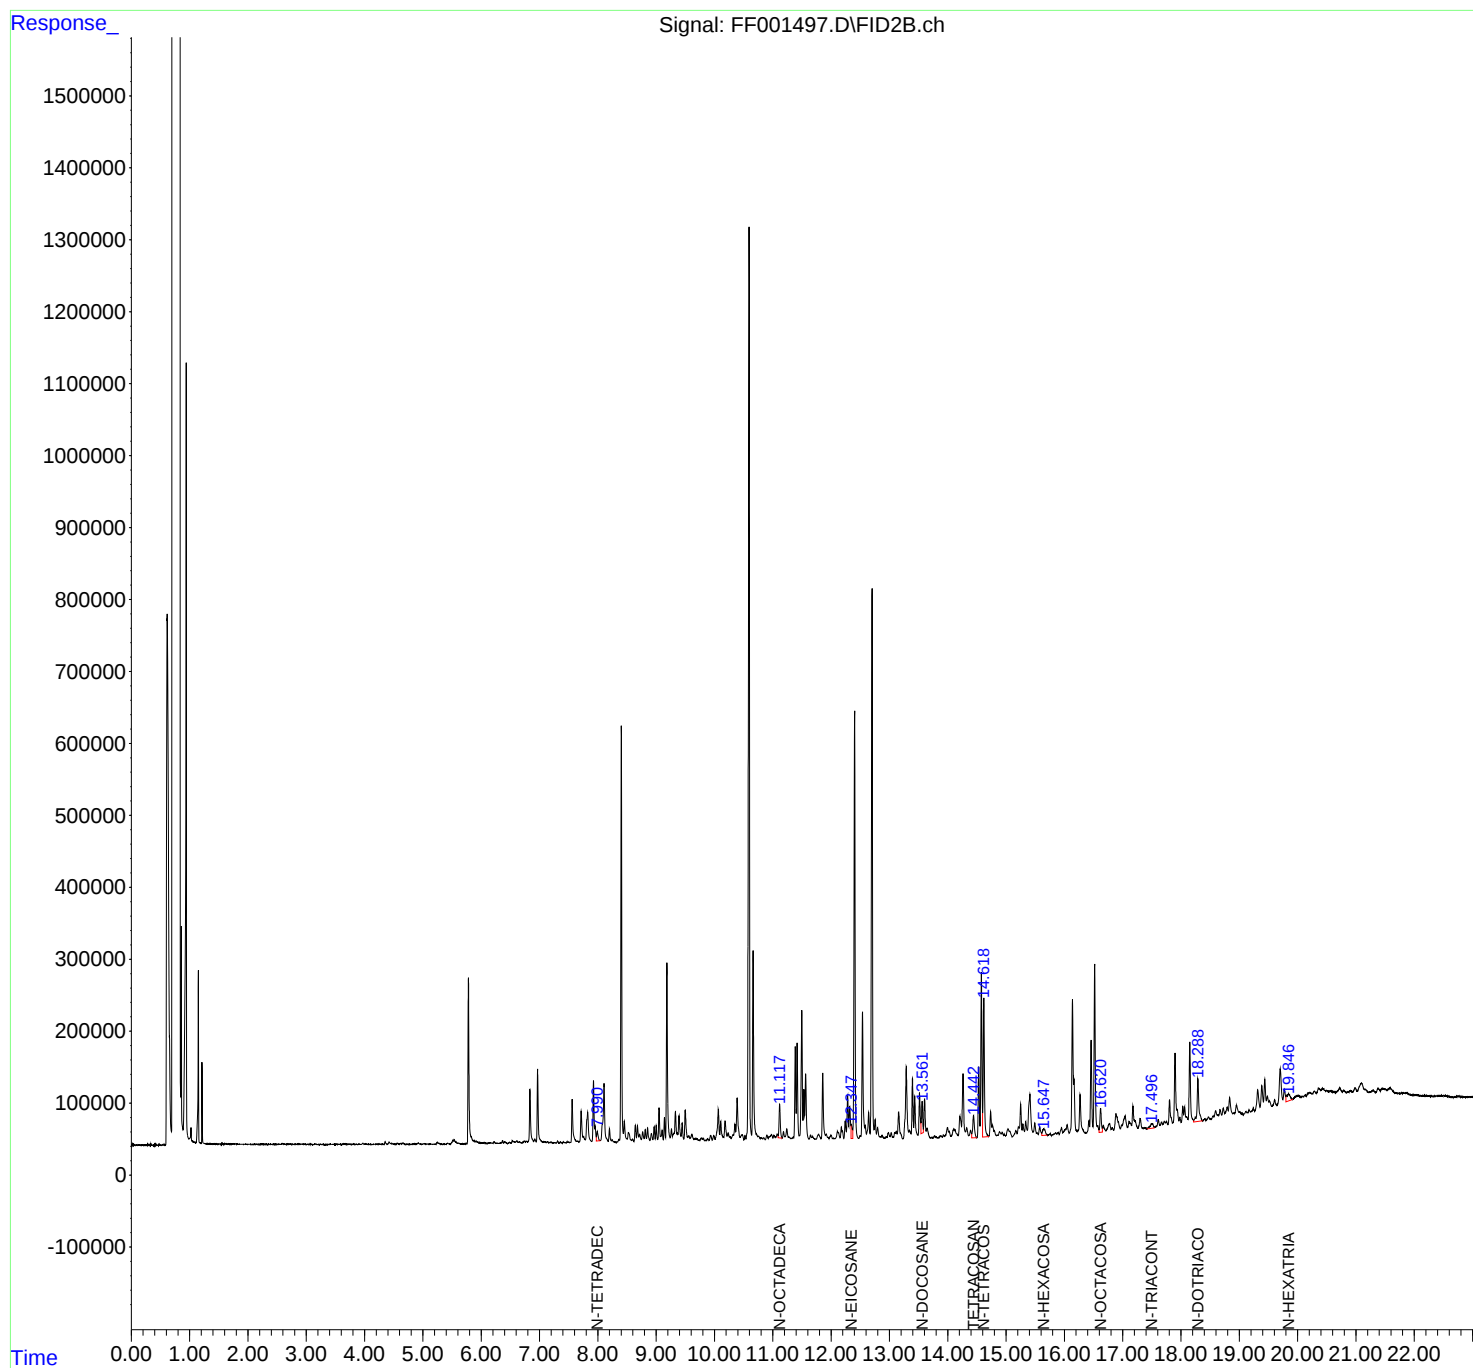

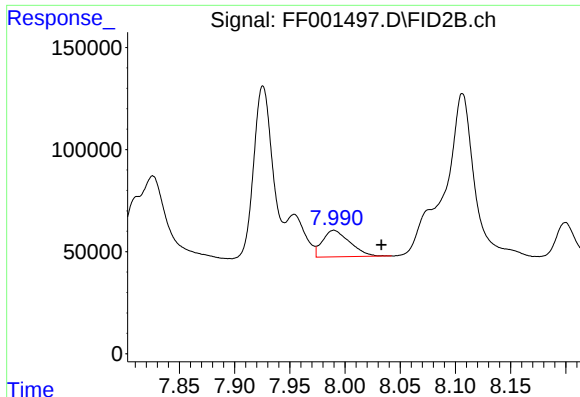


#4 N-TETRADECANE

R.T.: 7.990 min
Delta R.T.: -0.043 min
Response: 224170
Conc: 1.78 ug/ml

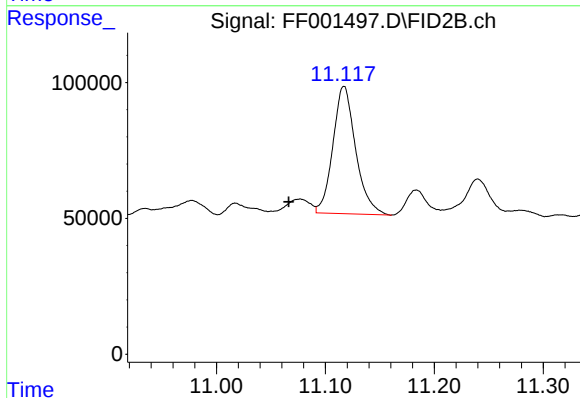


#6 N-OCTADECANE

R.T.: 11.117 min
Delta R.T.: 0.051 min
Response: 681609
Conc: 5.44 ug/ml

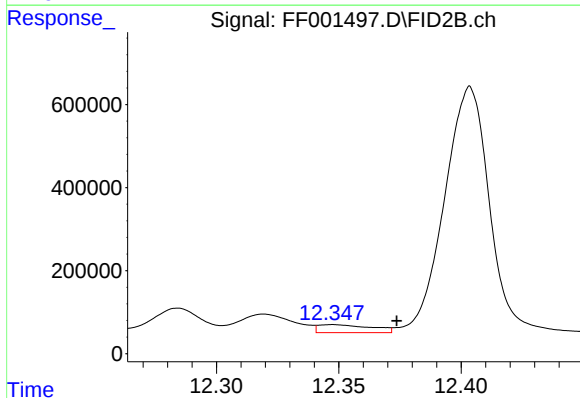


#7 N-EICOSANE

R.T.: 12.348 min
Delta R.T.: -0.026 min
Response: 289667
Conc: 2.33 ug/ml

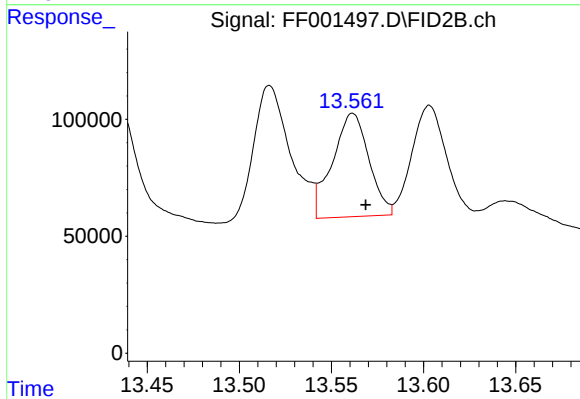


#8 N-DOCOSANE

R.T.: 13.562 min
Delta R.T.: -0.007 min
Response: 608933
Conc: 4.94 ug/ml

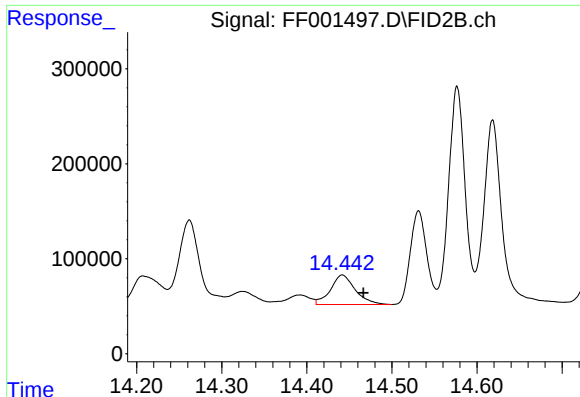


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.442 min
Delta R.T.: -0.025 min
Response: 629470
Conc: 5.84 ug/ml

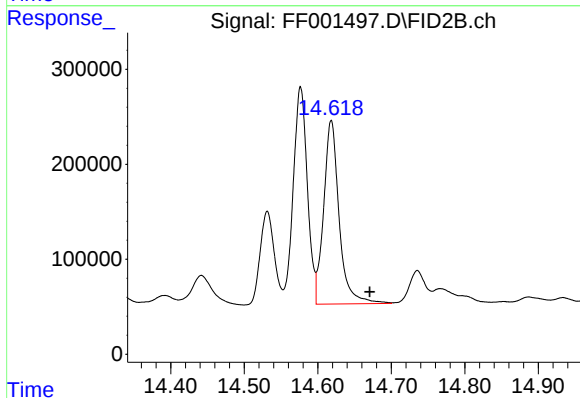


#10 N-TETRACOSANE

R.T.: 14.618 min
Delta R.T.: -0.052 min
Response: 2825310
Conc: 23.18 ug/ml

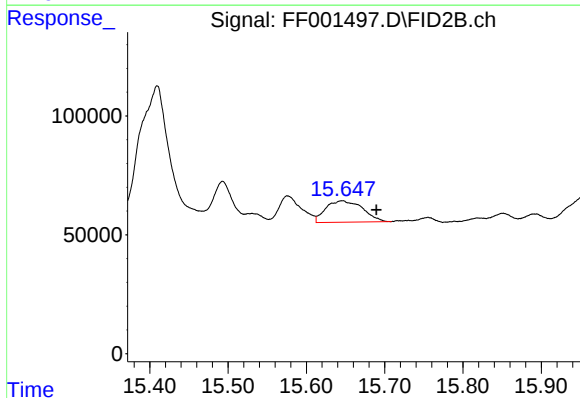


#11 N-HEXACOSANE

R.T.: 15.646 min
Delta R.T.: -0.044 min
Response: 294270
Conc: 2.43 ug/ml

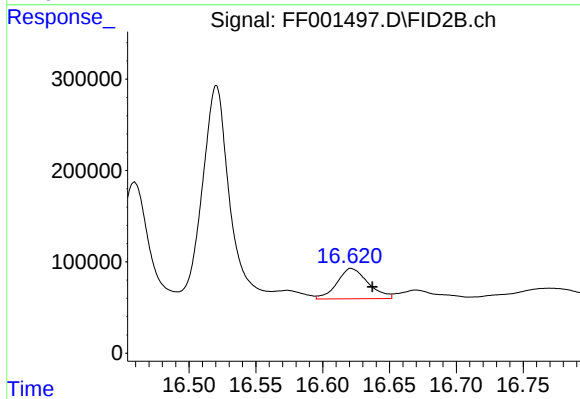


#12 N-OCTACOSANE

R.T.: 16.621 min
Delta R.T.: -0.016 min
Response: 539035
Conc: 4.47 ug/ml

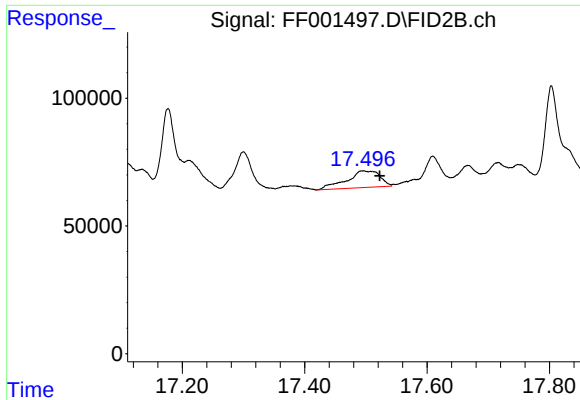


#13 N-TRIACONTANE

R.T.: 17.495 min
Delta R.T.: -0.027 min
Response: 247557
Conc: 2.06 ug/ml

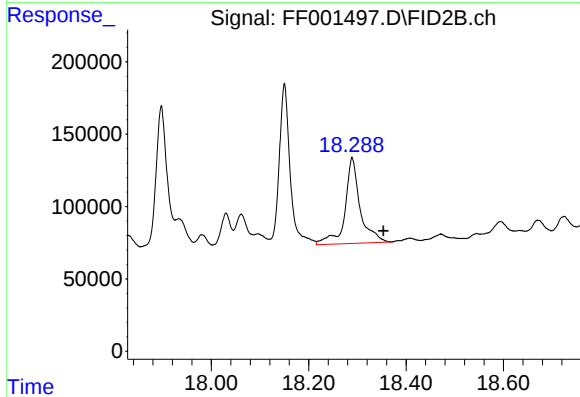

#14 N-DOTRIACONTANE

R.T.: 18.289 min
Delta R.T.: -0.064 min
Response: 1275665
Conc: 10.82 ug/ml

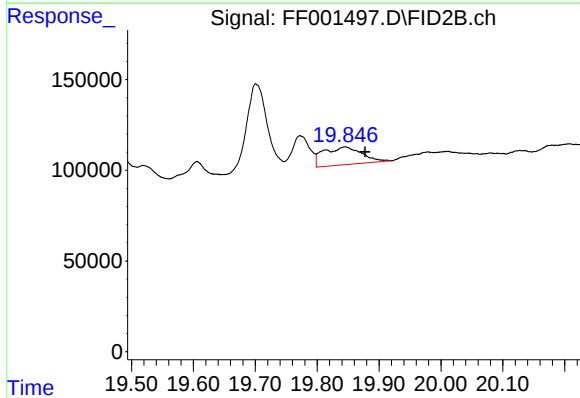

#16 N-HEXATRIACONTANE

R.T.: 19.845 min
Delta R.T.: -0.032 min
Response: 421710
Conc: 3.71 ug/ml