

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
 Data File : FF001500.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jul 2018 08:46
 Operator : AJ\SJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jul 27 05:01:31 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.481	173261	1.608 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.641	17882	0.147 ug/ml
11)	N-HEXACOSANE	15.661	93190	0.769 ug/ml
12)	N-OCTACOSANE	16.609	297784	2.472 ug/ml
13)	N-TRIACONTANE	17.494	572665	4.764 ug/ml
14)	N-DOTRIACONTANE	18.325	1095873	9.295 ug/ml
15)	N-TETRATRIACONTANE	19.108	1201696	10.224 ug/ml
16)	N-HEXATRIACONTANE	19.848	2537045	22.335 ug/ml
17)	N-OCTATRIACONTANE	20.557	9985663	96.708 ug/ml
18)	N-TETRACONTANE	21.381	2321534	22.671 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
Data File : FF001500.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2018 08:46
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jul 27 05:01:31 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

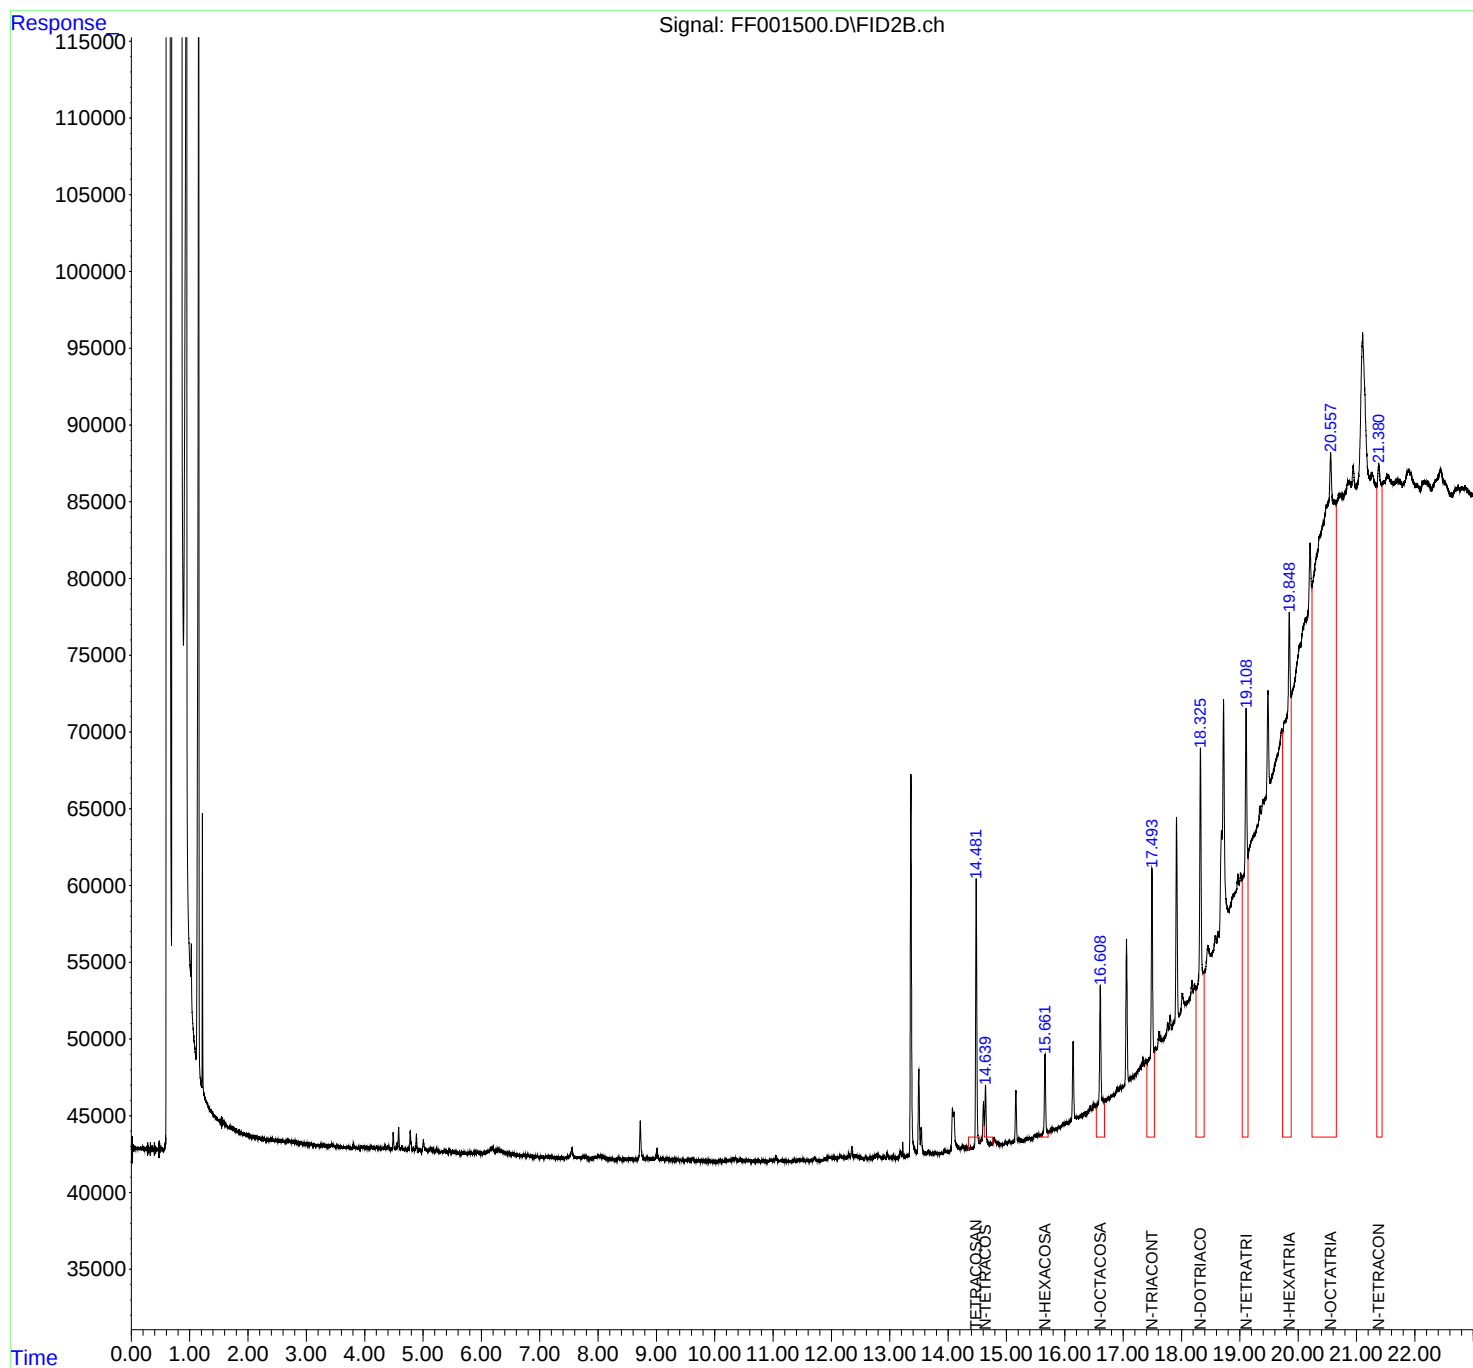


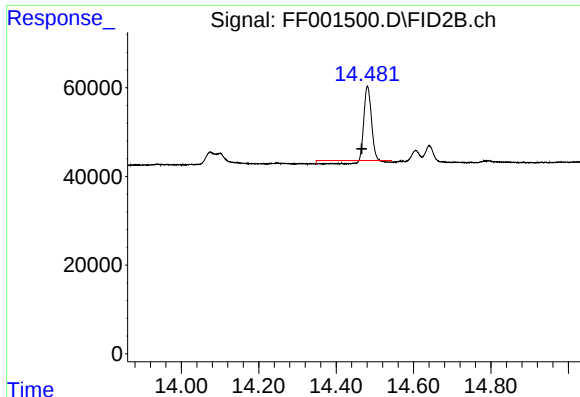

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.481 min
Delta R.T.: 0.015 min
Response: 173261
Conc: 1.61 ug/ml

Instrument :
FID_F
ClientSampleId :

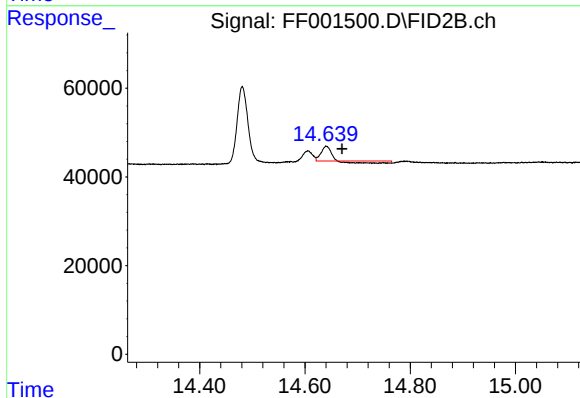


#10 N-TETRACOSANE

R.T.: 14.641 min
Delta R.T.: -0.030 min
Response: 17882
Conc: 0.15 ug/ml

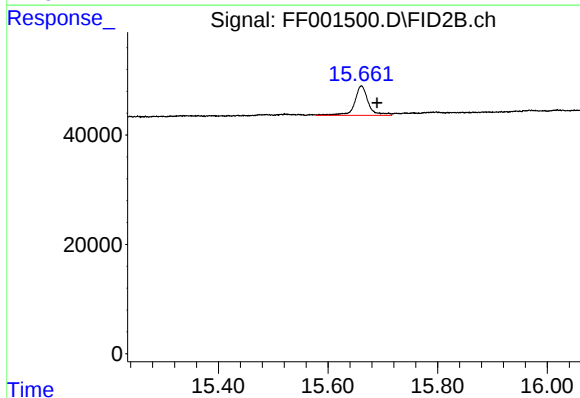


#11 N-HEXACOSANE

R.T.: 15.661 min
Delta R.T.: -0.028 min
Response: 93190
Conc: 0.77 ug/ml

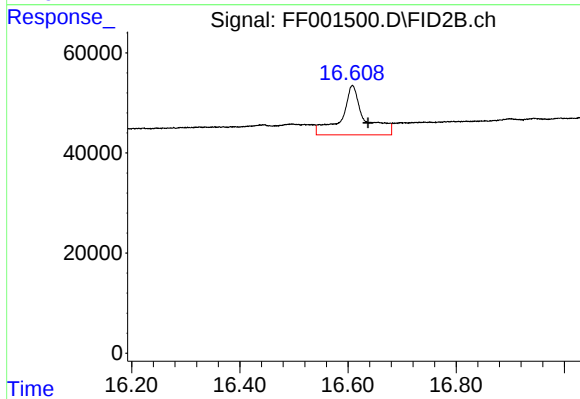

#12 N-OCTACOSANE


R.T.: 16.609 min
Delta R.T.: -0.029 min
Response: 297784
Conc: 2.47 ug/ml

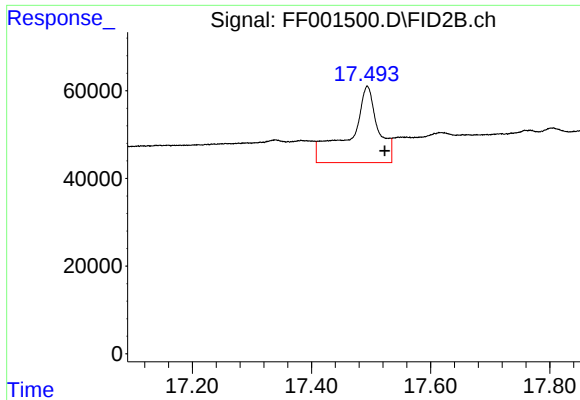

#13 N-TRIACONTANE


R.T.: 17.494 min
Delta R.T.: -0.029 min
Response: 572665
Conc: 4.76 ug/ml

Instrument :
FID_F
ClientSampleId :

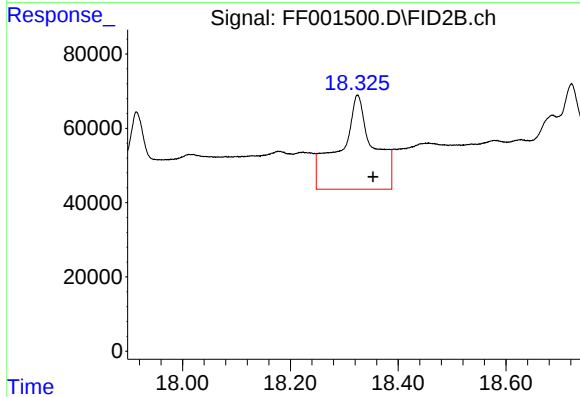


#14 N-DOTRIACONTANE

R.T.: 18.325 min
Delta R.T.: -0.028 min
Response: 1095873
Conc: 9.29 ug/ml

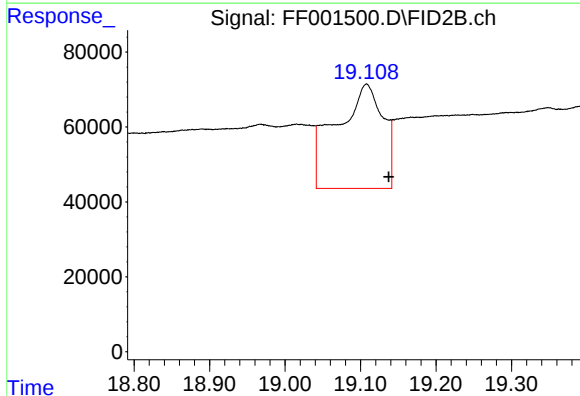


#15 N-TETRATRIACONTANE

R.T.: 19.108 min
Delta R.T.: -0.029 min
Response: 1201696
Conc: 10.22 ug/ml

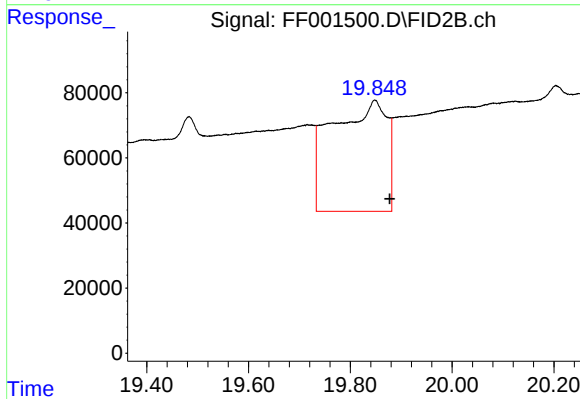

#16 N-HEXATRIACONTANE


R.T.: 19.848 min
Delta R.T.: -0.029 min
Response: 2537045
Conc: 22.33 ug/ml

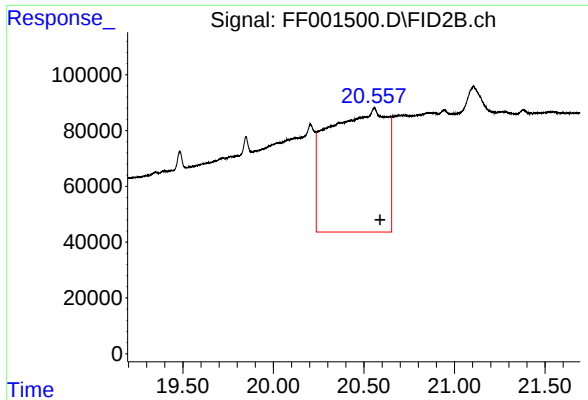

#17 N-OCTATRIACONTANE

R.T.: 20.557 min
Delta R.T.: -0.032 min
Response: 9985663
Conc: 96.71 ug/ml

Instrument :
FID_F
ClientSampleId :

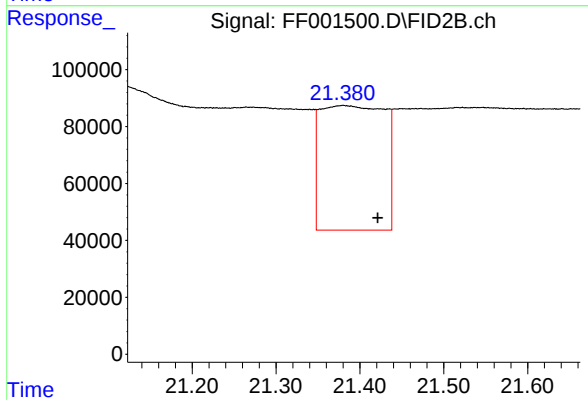

#18 N-TETRACONTANE

R.T.: 21.381 min
Delta R.T.: -0.041 min
Response: 2321534
Conc: 22.67 ug/ml