

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
 Data File : FF001501.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jul 2018 09:16
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jul 27 05:01:43 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.440	2665315	24.742 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.665	12465	0.103 ug/ml
12) N-OCTACOSANE	16.611	143710	1.193 ug/ml
13) N-TRIACONTANE	17.497	927677	7.717 ug/ml
14) N-DOTRIACONTANE	18.328	1018125	8.635 ug/ml
15) N-TETRATRIACONTANE	19.110	3405589	28.976 ug/ml
16) N-HEXATRIACONTANE	19.850	5337013	46.984 ug/ml
17) N-OCTATRIACONTANE	20.558	10004829	96.894 ug/ml
18) N-TETRACONTANE	21.383	2649696	25.876 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
Data File : FF001501.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2018 09:16
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jul 27 05:01:43 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

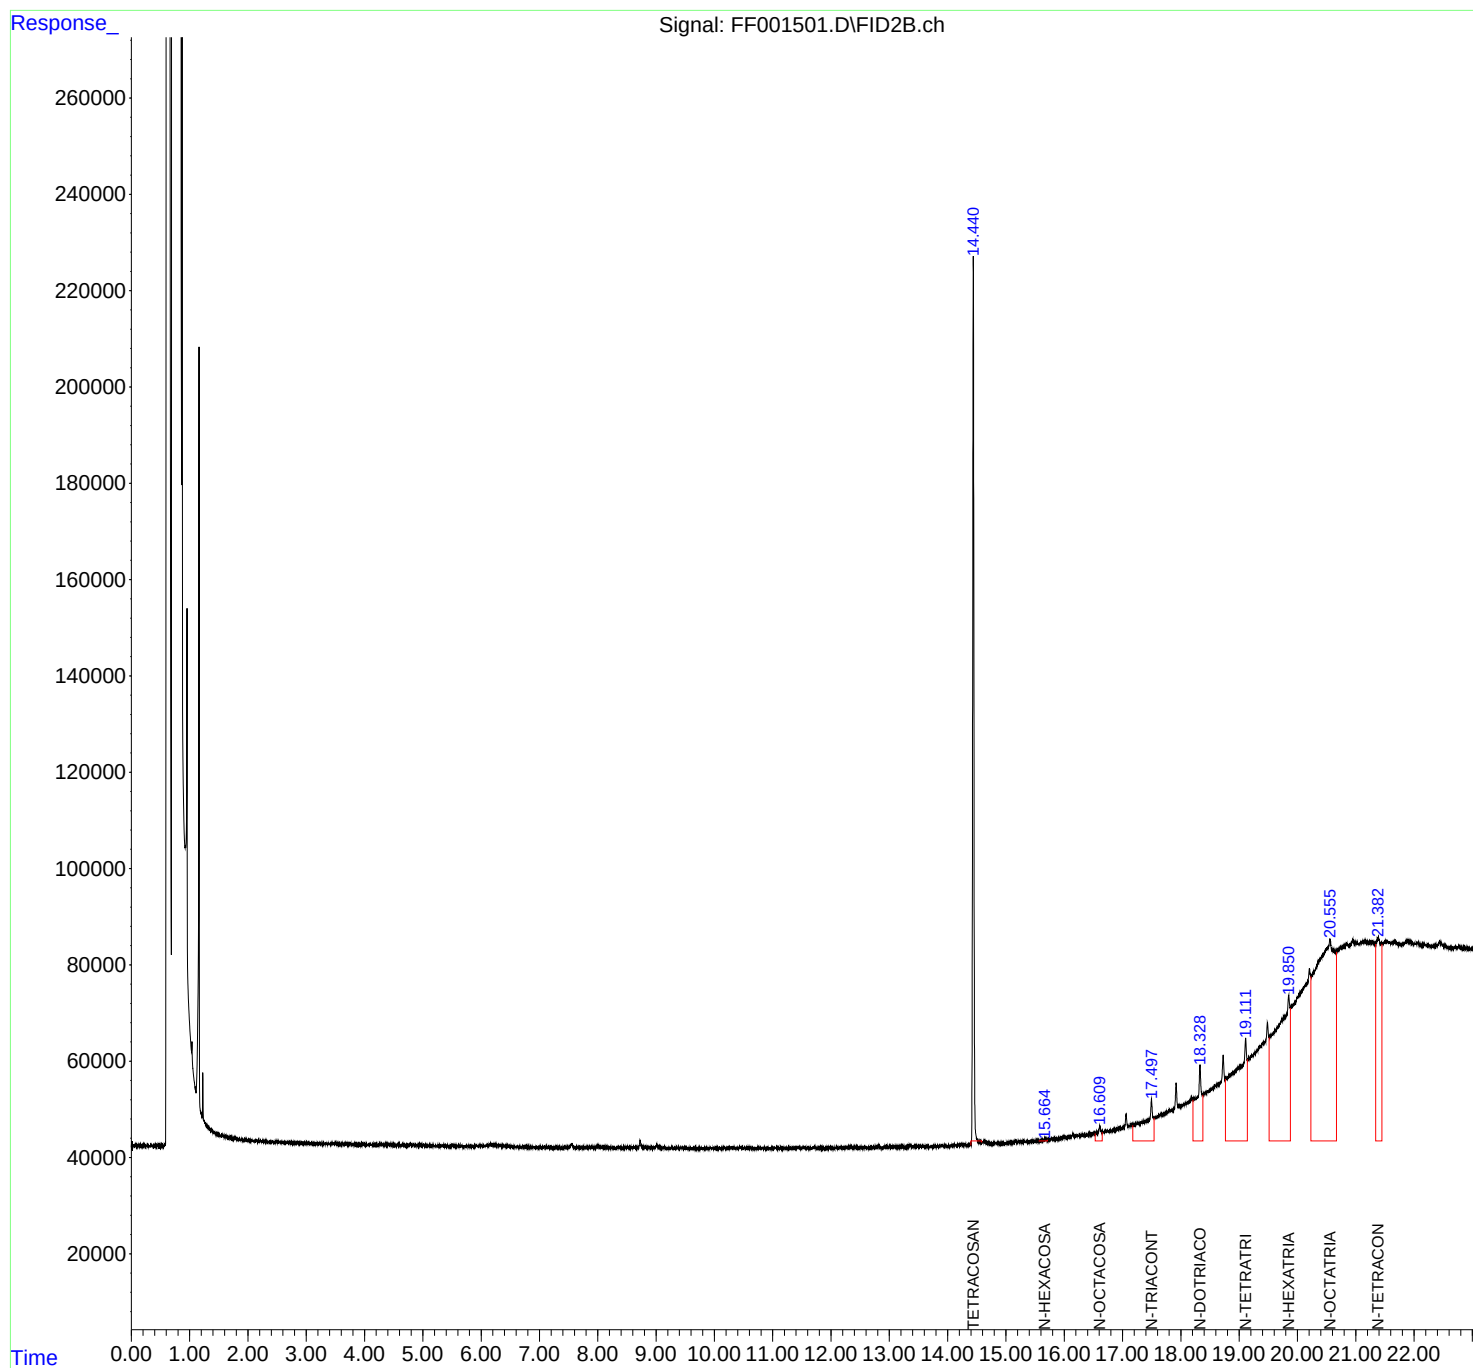


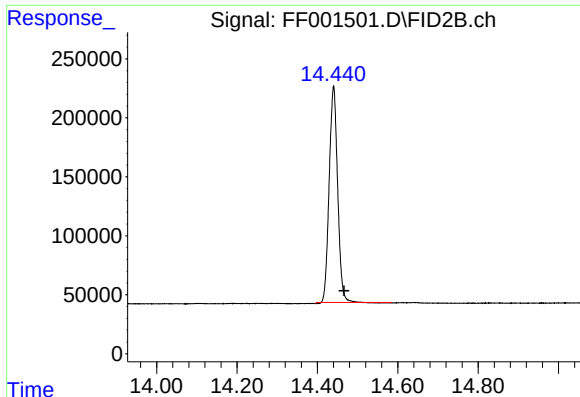

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.440 min
Delta R.T.: -0.026 min
Response: 2665315
Conc: 24.74 ug/ml

Instrument :
FID_F
ClientSampleId :

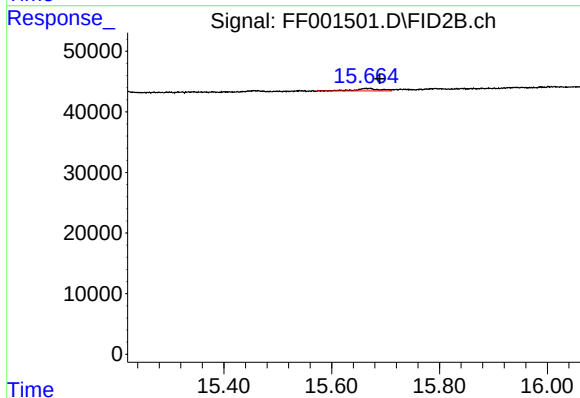


#11 N-HEXACOSANE

R.T.: 15.665 min
Delta R.T.: -0.024 min
Response: 12465
Conc: 0.10 ug/ml

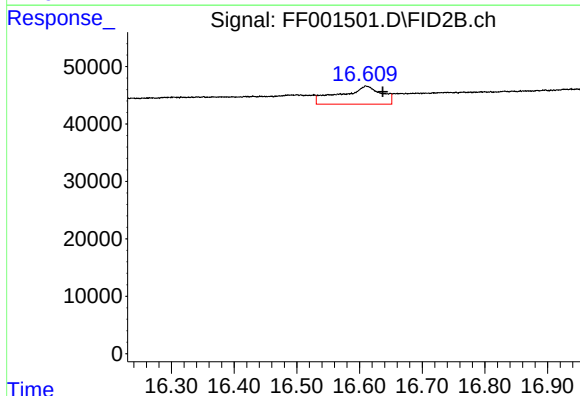


#12 N-OCTACOSANE

R.T.: 16.611 min
Delta R.T.: -0.026 min
Response: 143710
Conc: 1.19 ug/ml

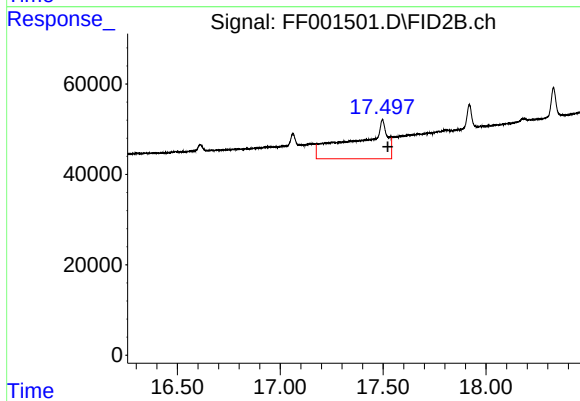

#13 N-TRIACONTANE


R.T.: 17.497 min
Delta R.T.: -0.026 min
Response: 927677
Conc: 7.72 ug/ml

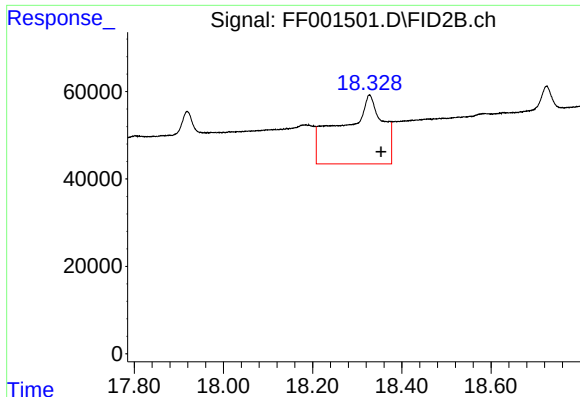

#14 N-DOTRIACONTANE


R.T.: 18.328 min
Delta R.T.: -0.026 min
Response: 1018125
Conc: 8.64 ug/ml

Instrument :
FID_F
ClientSampleId :

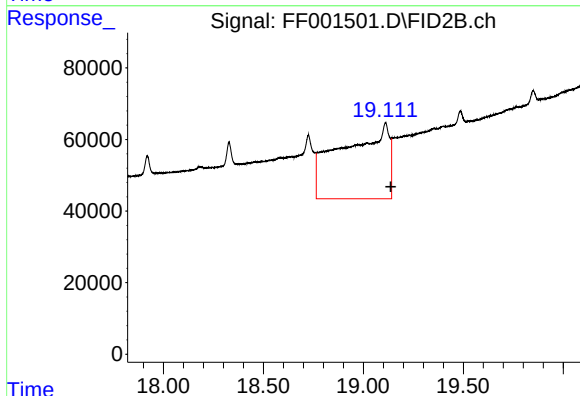


#15 N-TETRATRIACONTANE

R.T.: 19.110 min
Delta R.T.: -0.027 min
Response: 3405589
Conc: 28.98 ug/ml

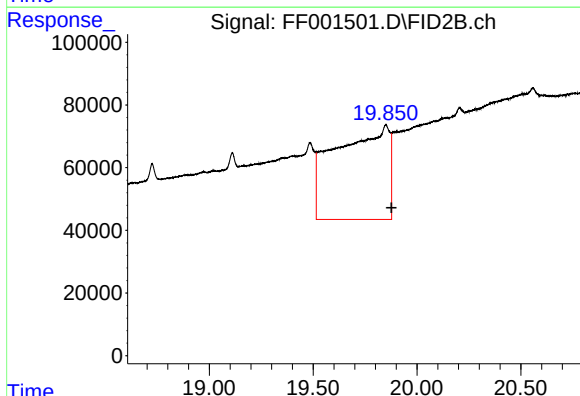


#16 N-HEXATRIACONTANE

R.T.: 19.850 min
Delta R.T.: -0.028 min
Response: 5337013
Conc: 46.98 ug/ml

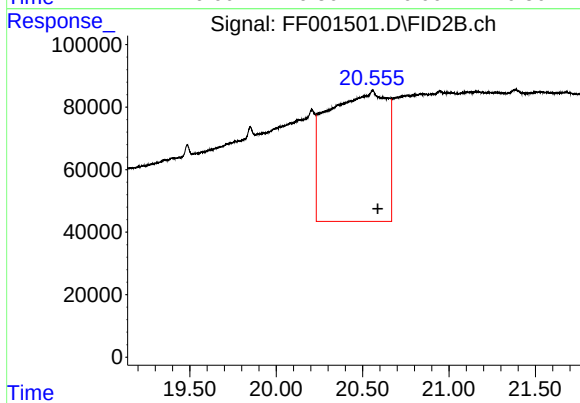

#17 N-OCTATRIACONTANE

R.T.: 20.558 min
Delta R.T.: -0.031 min
Response: 10004829
Conc: 96.89 ug/ml

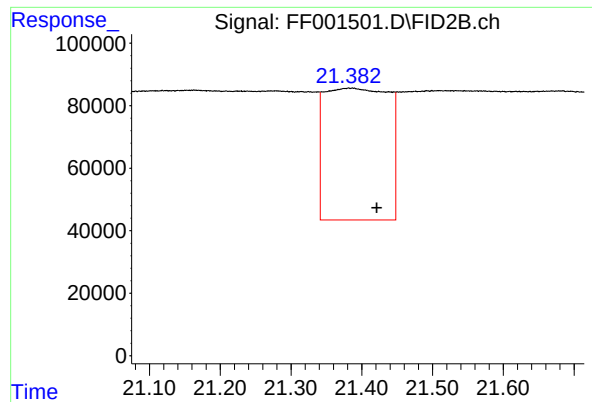

#18 N-TETRACONTANE

R.T.: 21.383 min
Delta R.T.: -0.038 min
Response: 2649696
Conc: 25.88 ug/ml

Instrument :
FID_F
ClientSampleId :