

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
 Data File : FF001505.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jul 2018 13:14
 Operator : AJ\SJ
 Sample : J4135-02 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jul 27 05:02:21 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.484	260365	2.417 ug/ml
Target Compounds			
7) N-EICOSANE	12.345	79659	0.640 ug/ml
8) N-DOCOSANE	13.568	97048	0.787 ug/ml
10) N-TETRACOSANE	14.691	269897	2.214 ug/ml
11) N-HEXACOSANE	15.696	142420	1.175 ug/ml
12) N-OCTACOSANE	16.651	907714	7.535 ug/ml
13) N-TRIACONTANE	17.494	1761091	14.650 ug/ml
14) N-DOTRIACONTANE	18.325	2024218	17.168 ug/ml
15) N-TETRATRIACONTANE	19.113	1508168	12.832 ug/ml
16) N-HEXATRIACONTANE	19.901	1150655	10.130 ug/ml
17) N-OCTATRIACONTANE	20.563	6958841	67.395 ug/ml
18) N-TETRACONTANE	21.444	1102259	10.764 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
Data File : FF001505.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2018 13:14
Operator : AJ\SJ
Sample : J4135-02 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jul 27 05:02:21 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

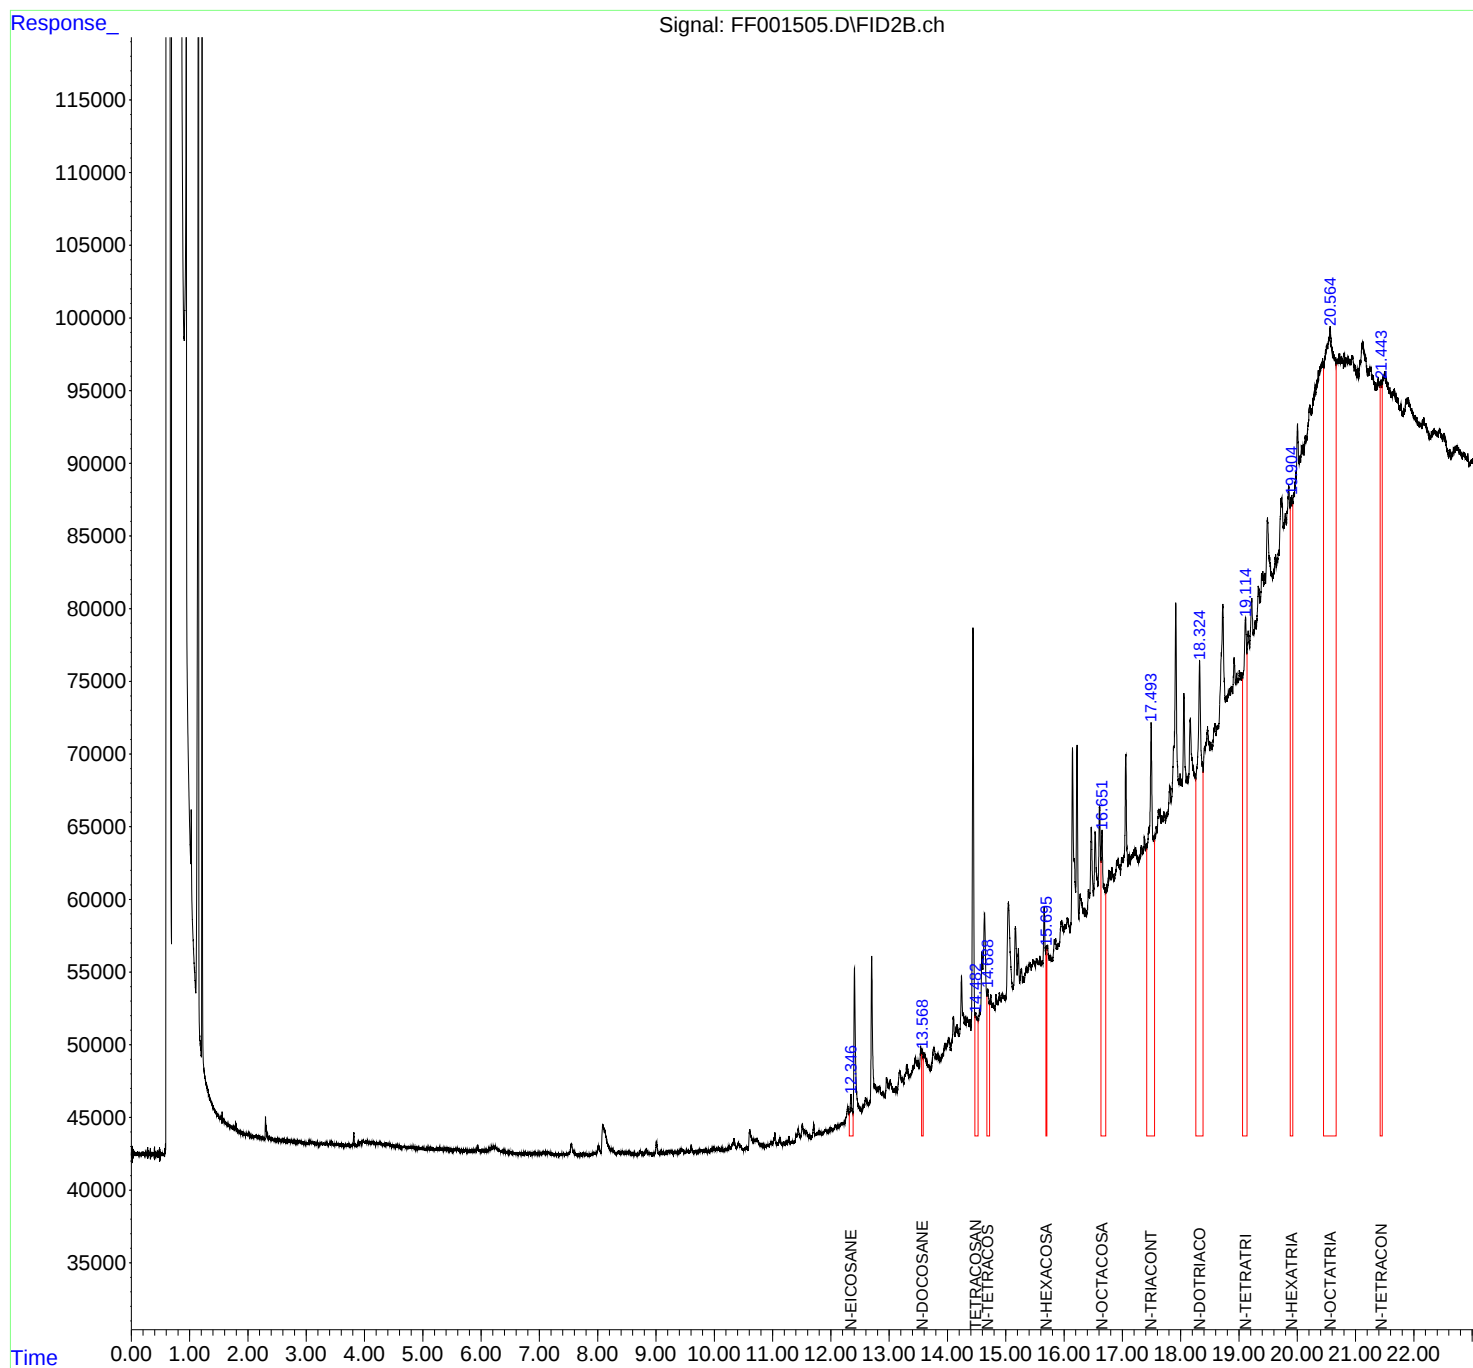


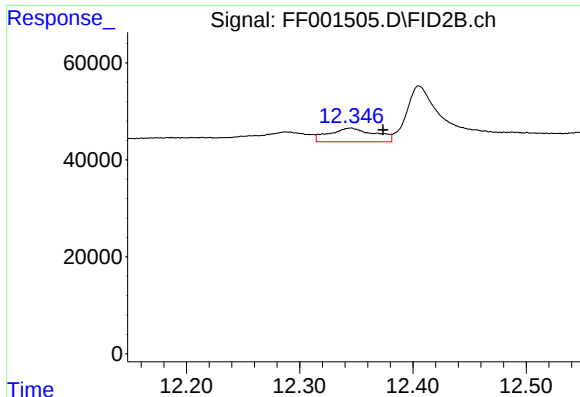

#7 N-EICOSANE


R.T.: 12.345 min
Delta R.T.: -0.029 min
Response: 79659
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

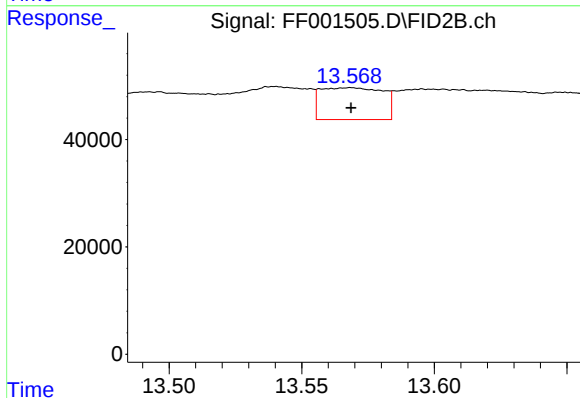


#8 N-DOCOSANE

R.T.: 13.568 min
Delta R.T.: -0.001 min
Response: 97048
Conc: 0.79 ug/ml

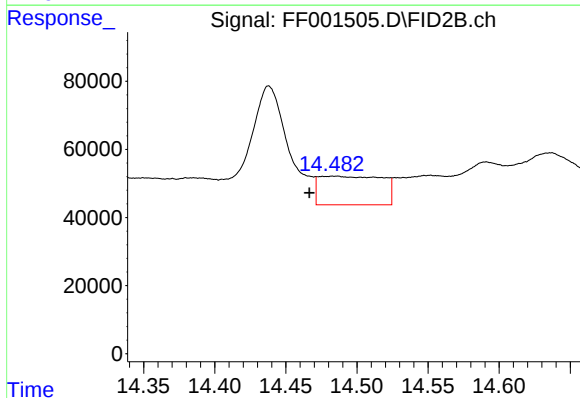


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.484 min
Delta R.T.: 0.017 min
Response: 260365
Conc: 2.42 ug/ml

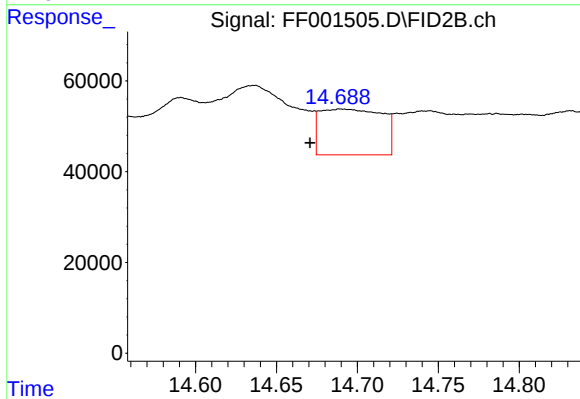

#10 N-TETRACOSANE


R.T.: 14.691 min
Delta R.T.: 0.020 min
Response: 269897
Conc: 2.21 ug/ml

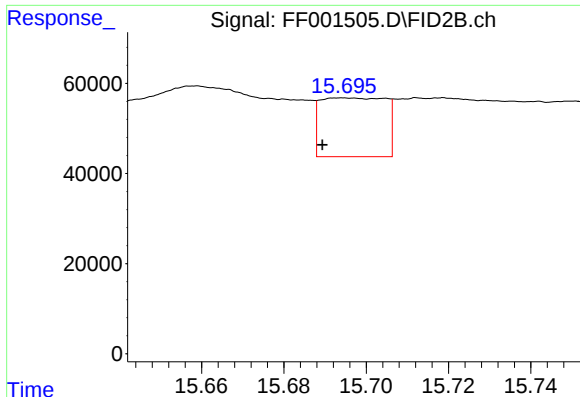

#11 N-HEXACOSANE


R.T.: 15.696 min
Delta R.T.: 0.006 min
Response: 142420
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :

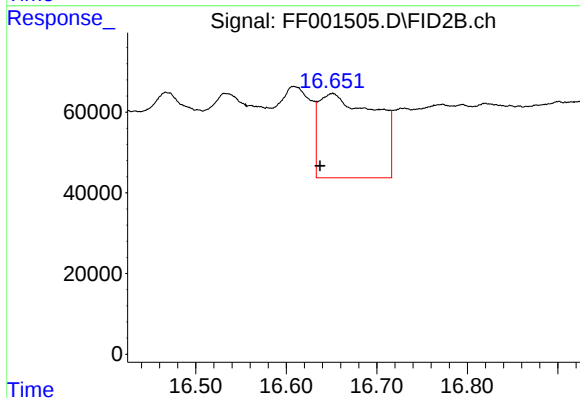


#12 N-OCTACOSANE

R.T.: 16.651 min
Delta R.T.: 0.014 min
Response: 907714
Conc: 7.53 ug/ml

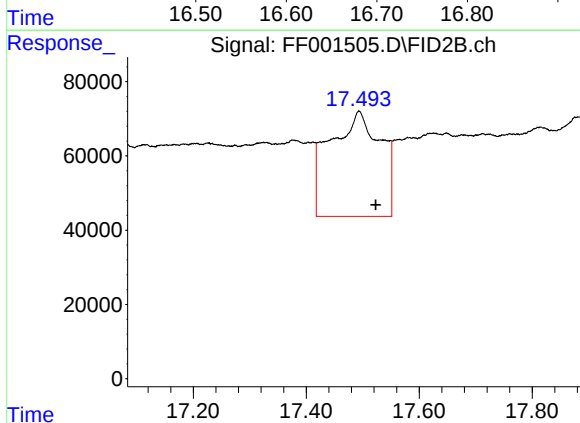


#13 N-TRIACONTANE

R.T.: 17.494 min
Delta R.T.: -0.029 min
Response: 1761091
Conc: 14.65 ug/ml

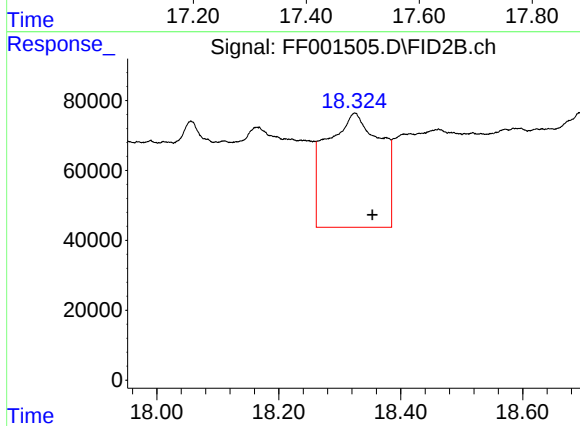

#14 N-DOTRIACONTANE


R.T.: 18.325 min
Delta R.T.: -0.029 min
Response: 2024218
Conc: 17.17 ug/ml

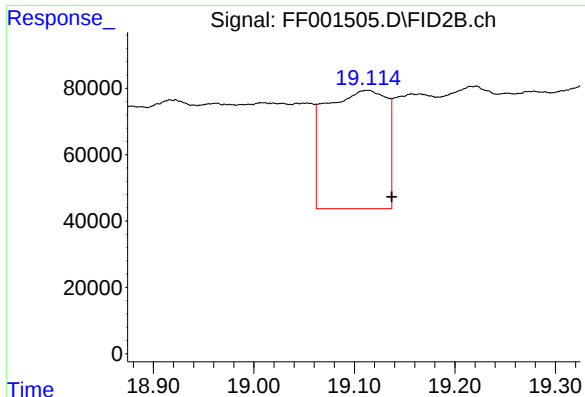

#15 N-TETRATRIACONTANE


R.T.: 19.113 min
Delta R.T.: -0.025 min
Response: 1508168
Conc: 12.83 ug/ml

Instrument :
FID_F
ClientSampleId :

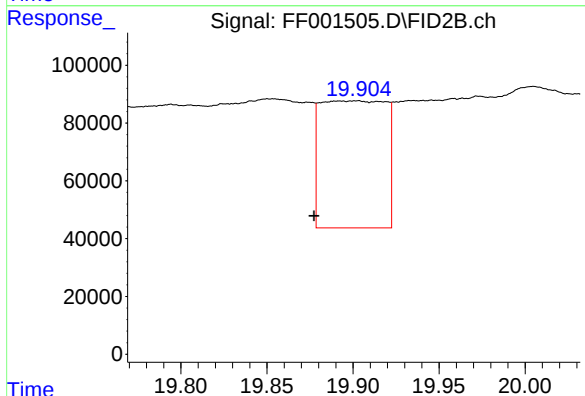


#16 N-HEXATRIACONTANE

R.T.: 19.901 min
Delta R.T.: 0.023 min
Response: 1150655
Conc: 10.13 ug/ml

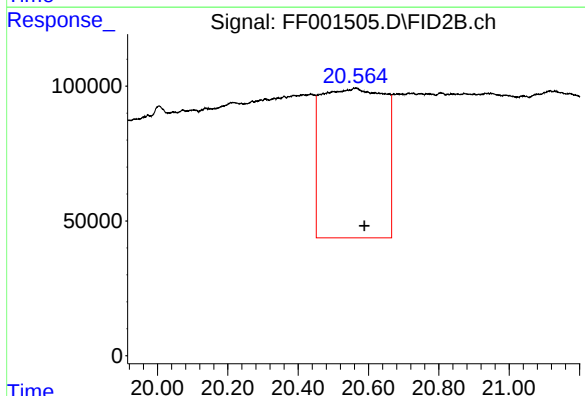

#17 N-OCTATRIACONTANE

R.T.: 20.563 min
Delta R.T.: -0.025 min
Response: 6958841
Conc: 67.39 ug/ml

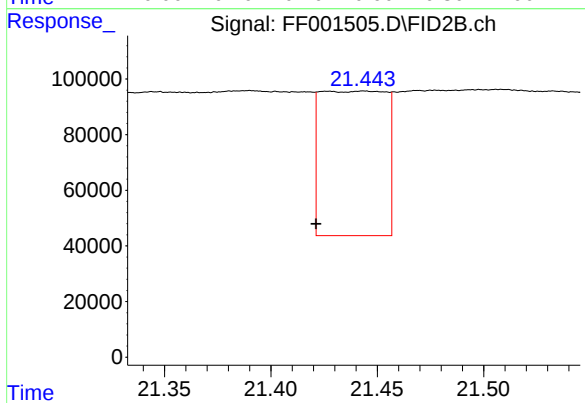

#18 N-TETRACONTANE

R.T.: 21.444 min
Delta R.T.: 0.023 min
Response: 1102259
Conc: 10.76 ug/ml