

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
 Data File : FF001507.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jul 2018 14:40
 Operator : AJ\SJ
 Sample : J4126-01 25X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jul 27 05:02:37 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.440	556727	5.168 ug/ml
Target Compounds			
6) N-OCTADECANE	11.036	26014	0.208 ug/ml
7) N-EICOSANE	12.397	2124223	17.077 ug/ml
8) N-DOCOSANE	13.564	356652	2.892 ug/ml
10) N-TETRACOSANE	14.688	540880	4.437 ug/ml
11) N-HEXACOSANE	15.670	460376	3.798 ug/ml
12) N-OCTACOSANE	16.625	891843	7.403 ug/ml
13) N-TRIACONTANE	17.494	1617236	13.453 ug/ml
14) N-DOTRIACONTANE	18.299f	2068084	17.541 ug/ml
15) N-TETRATRIACONTANE	19.112	1391440	11.839 ug/ml
16) N-HEXATRIACONTANE	19.893	1260448	11.096 ug/ml
17) N-OCTATRIACONTANE	20.558	3377163	32.707 ug/ml
18) N-TETRACONTANE	21.396	2760362	26.957 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
Data File : FF001507.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2018 14:40
Operator : AJ\SJ
Sample : J4126-01 25X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jul 27 05:02:37 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

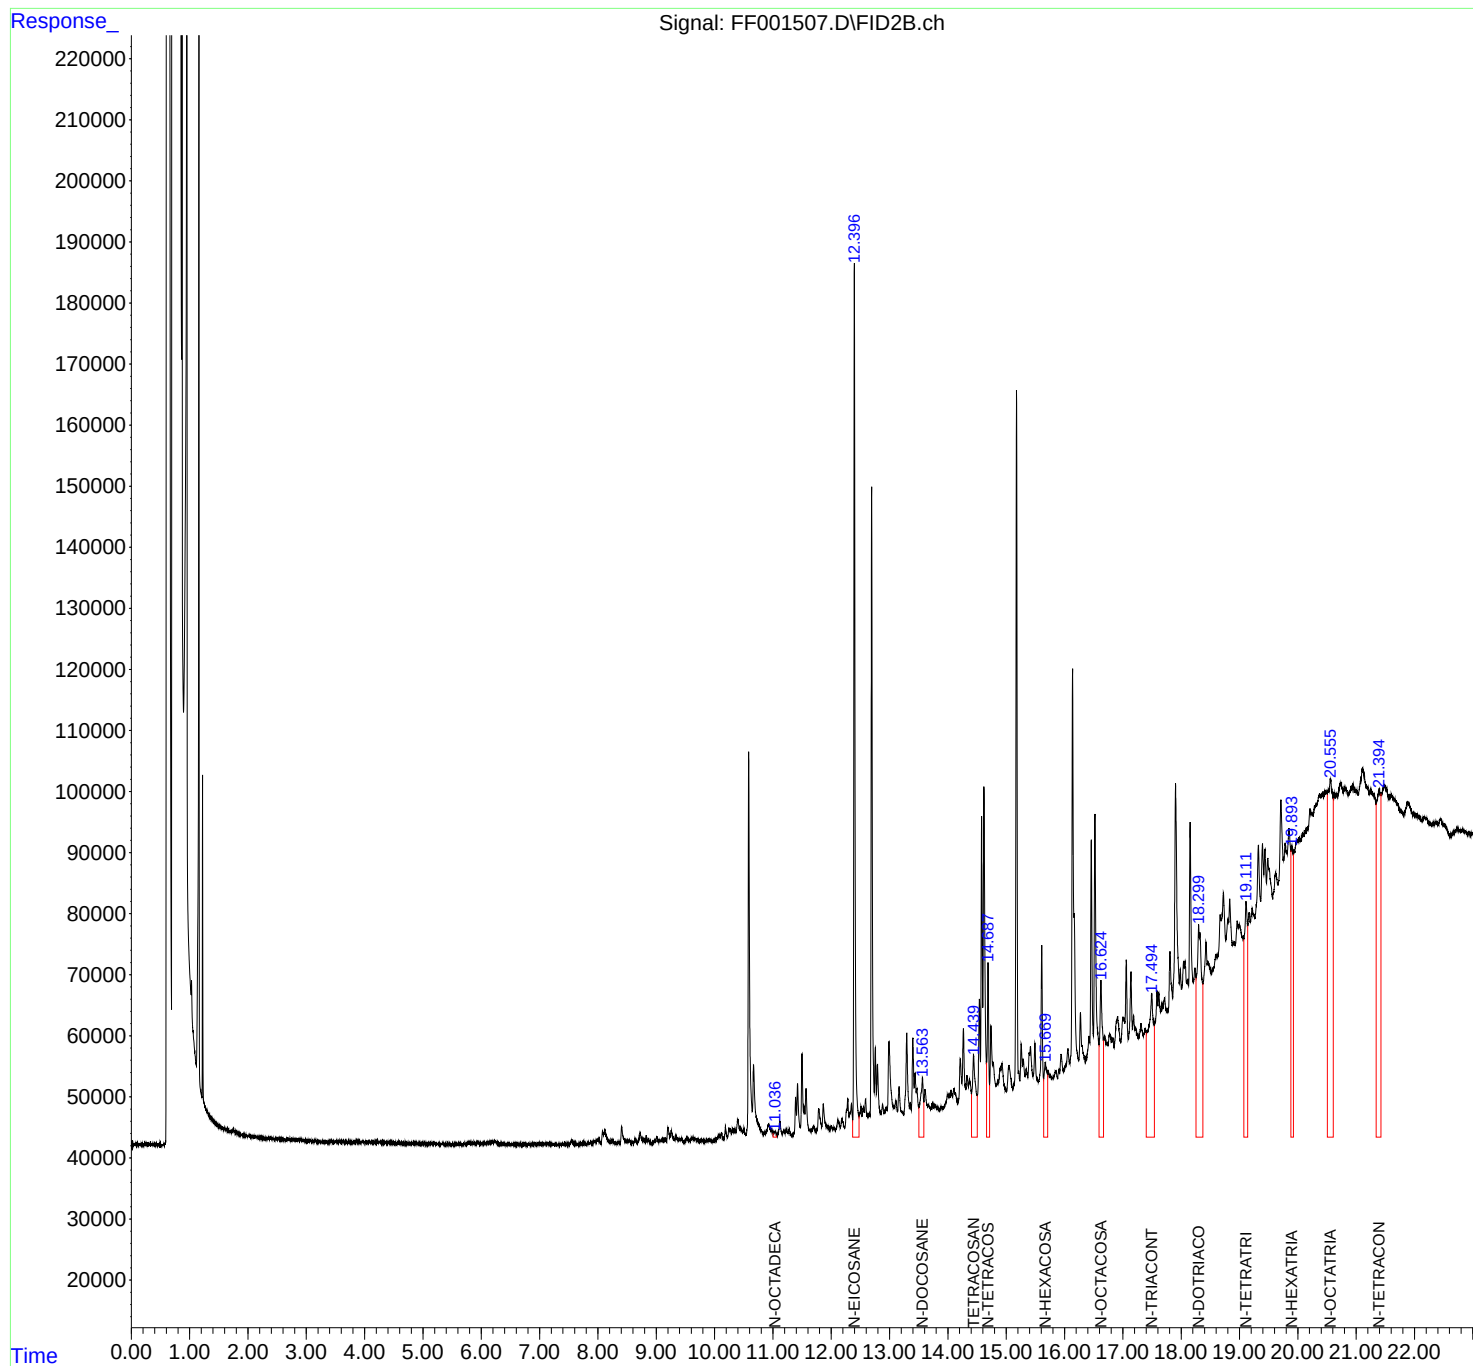


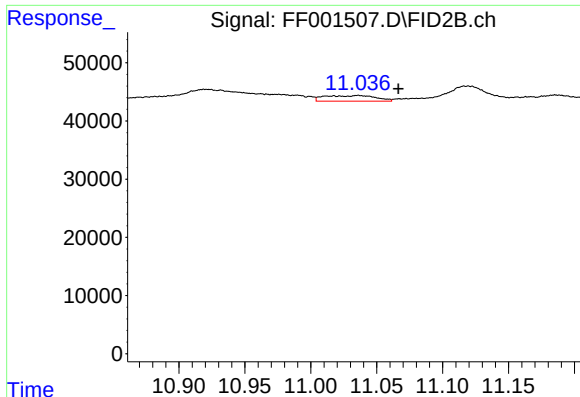

#6 N-OCTADECANE


R.T.: 11.036 min
Delta R.T.: -0.030 min
Response: 26014
Conc: 0.21 ug/ml

Instrument :
FID_F
ClientSampleId :

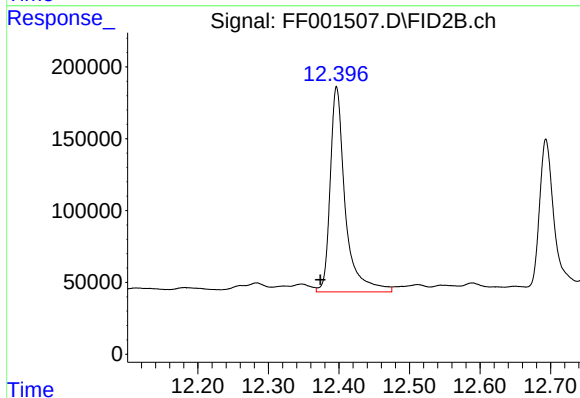


#7 N-EICOSANE

R.T.: 12.397 min
Delta R.T.: 0.023 min
Response: 2124223
Conc: 17.08 ug/ml

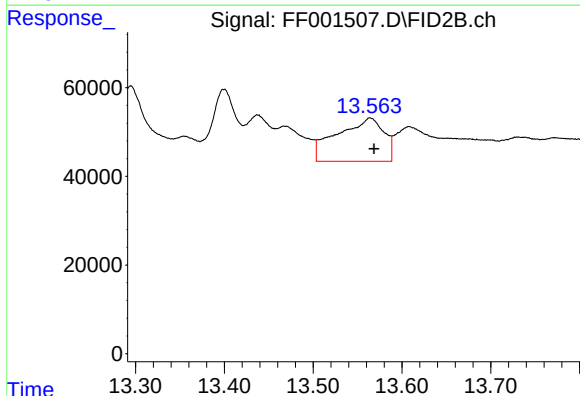


#8 N-DOCOSANE

R.T.: 13.564 min
Delta R.T.: -0.004 min
Response: 356652
Conc: 2.89 ug/ml

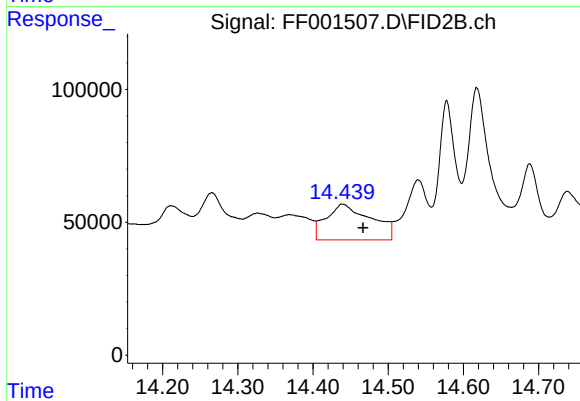

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.440 min
Delta R.T.: -0.027 min
Response: 556727
Conc: 5.17 ug/ml

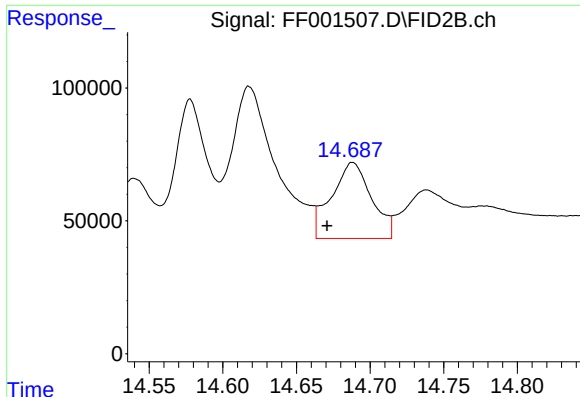

#10 N-TETRACOSANE


R.T.: 14.688 min
Delta R.T.: 0.018 min
Response: 540880
Conc: 4.44 ug/ml

Instrument :
FID_F
ClientSampleId :

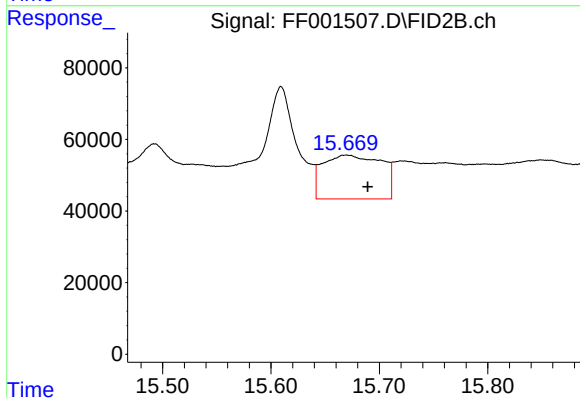


#11 N-HEXACOSANE

R.T.: 15.670 min
Delta R.T.: -0.020 min
Response: 460376
Conc: 3.80 ug/ml

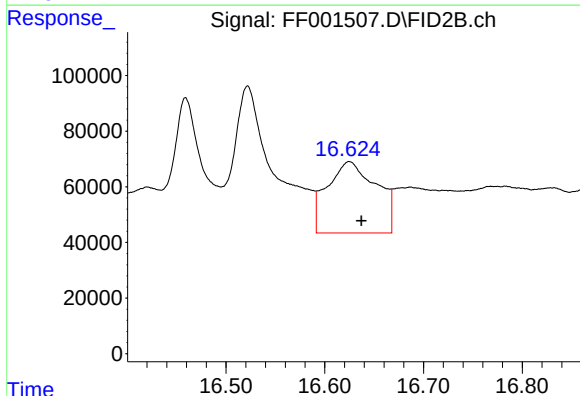


#12 N-OCTACOSANE

R.T.: 16.625 min
Delta R.T.: -0.012 min
Response: 891843
Conc: 7.40 ug/ml

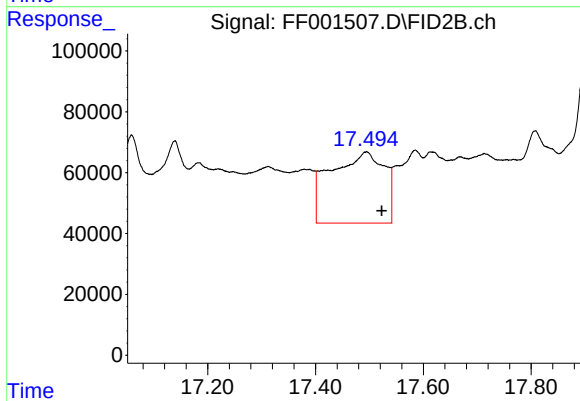

#13 N-TRIACONTANE


R.T.: 17.494 min
Delta R.T.: -0.029 min
Response: 1617236
Conc: 13.45 ug/ml

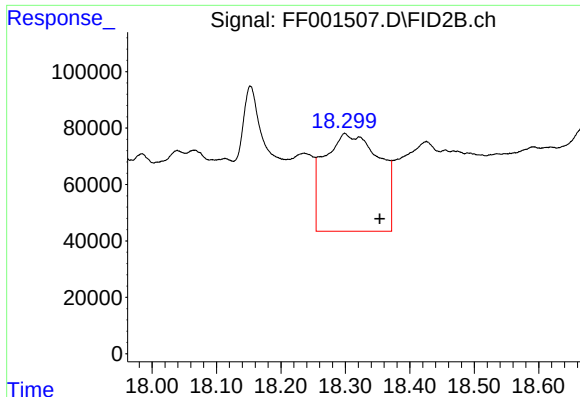

#14 N-DOTRIACONTANE


R.T.: 18.299 min
Delta R.T.: -0.054 min
Response: 2068084
Conc: 17.54 ug/ml

Instrument :
FID_F
ClientSampleId :

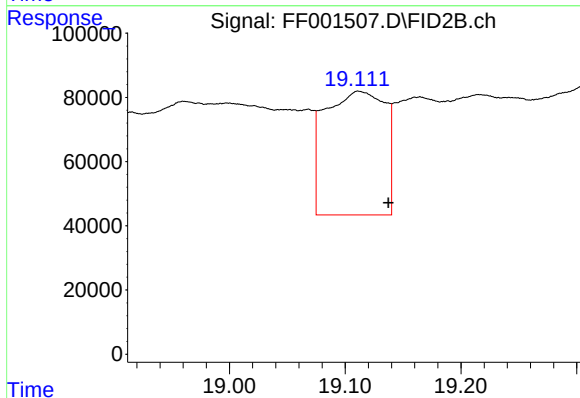


#15 N-TETRATRIACONTANE

R.T.: 19.112 min
Delta R.T.: -0.025 min
Response: 1391440
Conc: 11.84 ug/ml

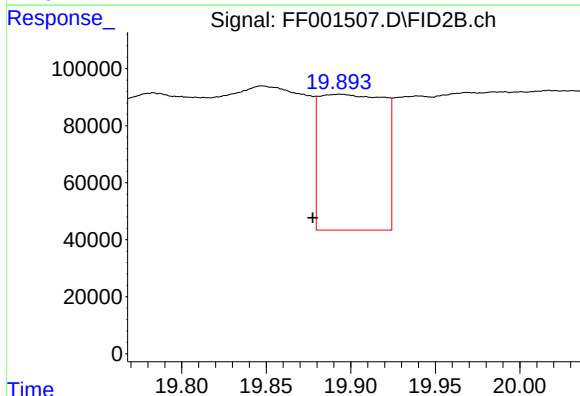


#16 N-HEXATRIACONTANE

R.T.: 19.893 min
Delta R.T.: 0.016 min
Response: 1260448
Conc: 11.10 ug/ml

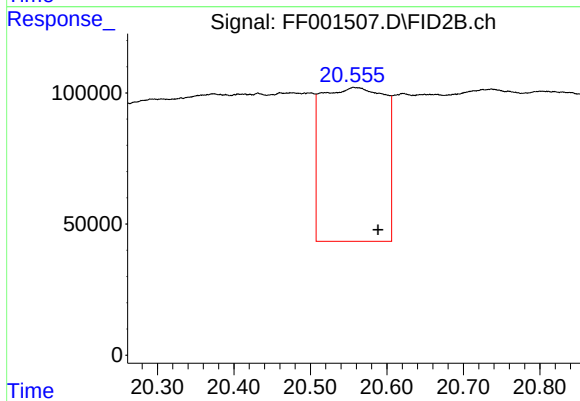

#17 N-OCTATRIACONTANE

R.T.: 20.558 min
Delta R.T.: -0.030 min
Response: 3377163
Conc: 32.71 ug/ml

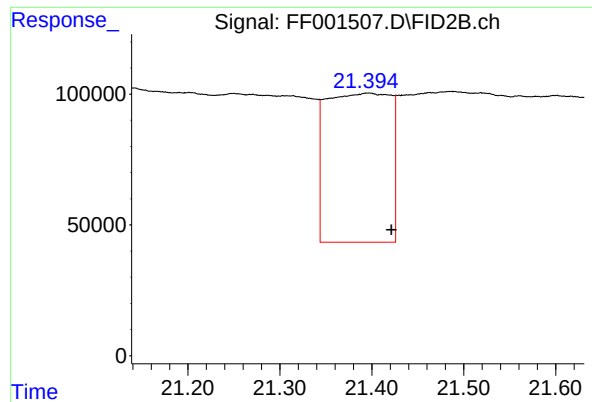

#18 N-TETRACONTANE

R.T.: 21.396 min
Delta R.T.: -0.025 min
Response: 2760362
Conc: 26.96 ug/ml

Instrument :
FID_F
ClientSampleId :