

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
 Data File : FF001508.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jul 2018 15:11
 Operator : AJ\SJ
 Sample : J4126-03 25X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jul 27 05:02:45 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.479	75457	0.700 ug/ml
Target Compounds			
1) N-OCTANE	2.146	1063	0.009 ug/ml
7) N-EICOSANE	12.351	52599	0.423 ug/ml
8) N-DOCOSANE	13.568	106299	0.862 ug/ml
10) N-TETRACOSANE	14.688	197186	1.617 ug/ml
11) N-HEXACOSANE	15.660	202675	1.672 ug/ml
12) N-OCTACOSANE	16.647	386031	3.204 ug/ml
13) N-TRIACONTANE	17.494	873605	7.267 ug/ml
14) N-DOTRIACONTANE	18.325	1396043	11.841 ug/ml
15) N-TETRATRIACONTANE	19.109	1554699	13.228 ug/ml
16) N-HEXATRIACONTANE	19.849	2800979	24.658 ug/ml
17) N-OCTATRIACONTANE	20.559	3588366	34.752 ug/ml
18) N-TETRACONTANE	21.383	3239364	31.634 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
Data File : FF001508.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2018 15:11
Operator : AJ\SJ
Sample : J4126-03 25X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jul 27 05:02:45 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

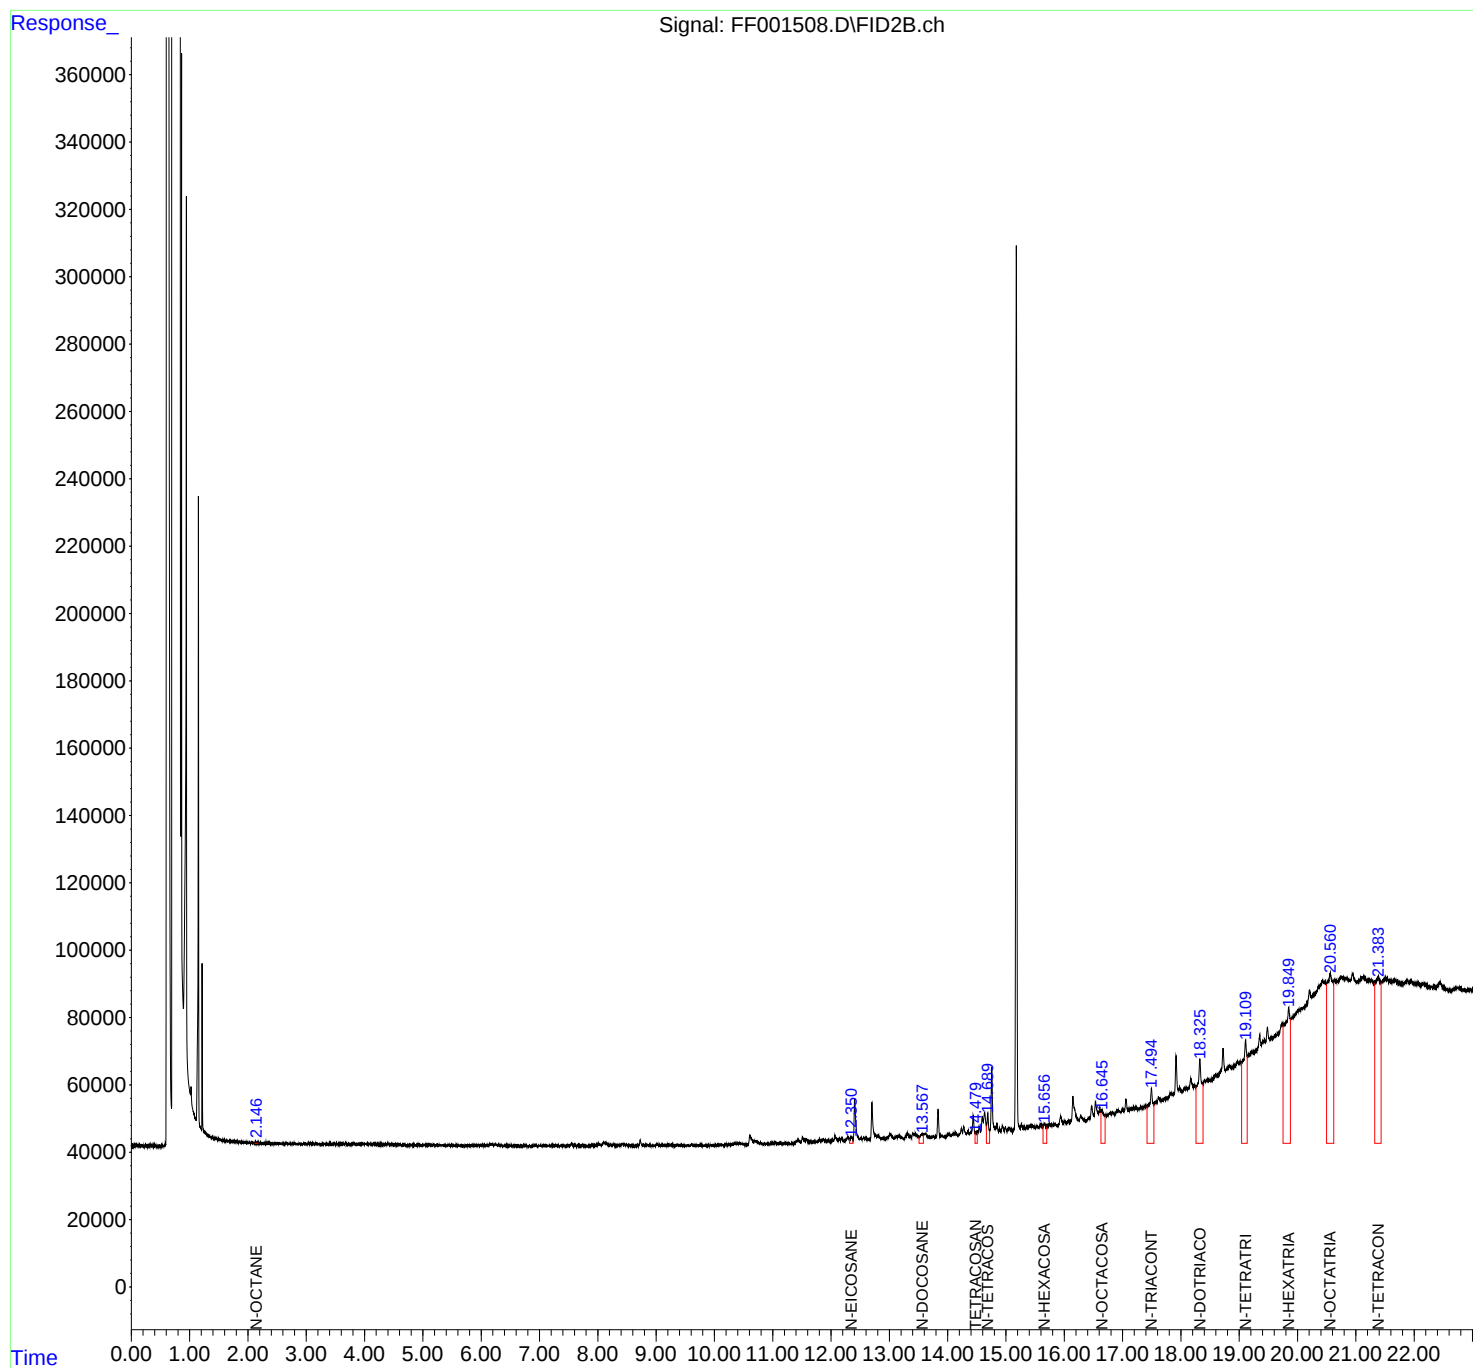


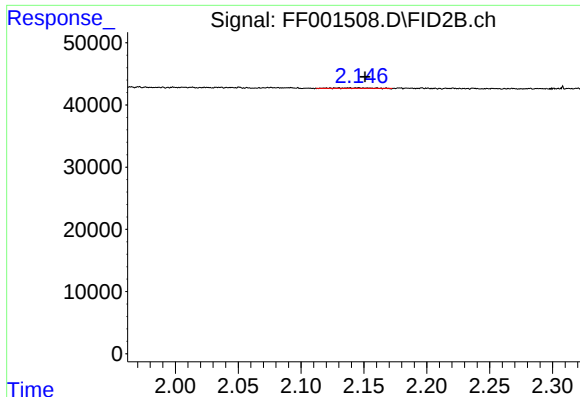

#1 N-OCTANE


R.T.: 2.146 min
Delta R.T.: -0.005 min
Response: 1063
Conc: 0.01 ug/ml

Instrument :
FID_F
ClientSampleId :

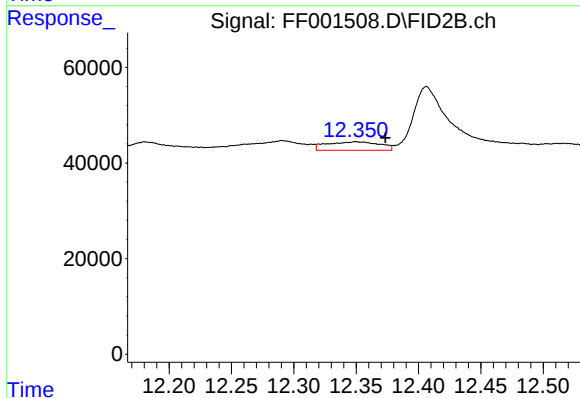


#7 N-EICOSANE

R.T.: 12.351 min
Delta R.T.: -0.023 min
Response: 52599
Conc: 0.42 ug/ml

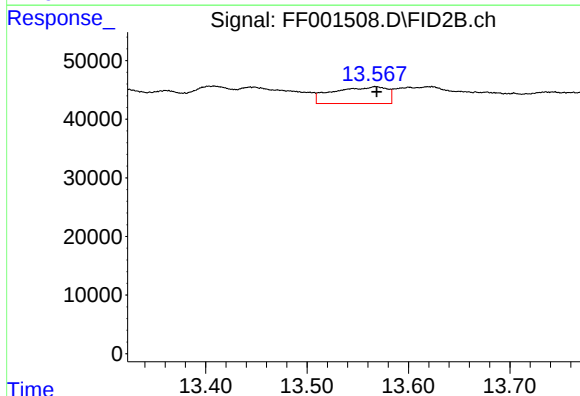


#8 N-DOCOSANE

R.T.: 13.568 min
Delta R.T.: 0.000 min
Response: 106299
Conc: 0.86 ug/ml

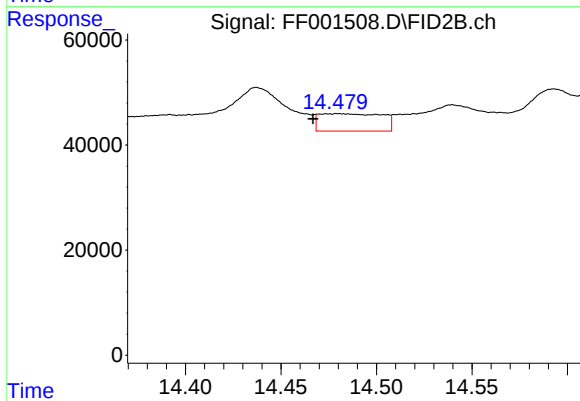

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.479 min
Delta R.T.: 0.012 min
Response: 75457
Conc: 0.70 ug/ml

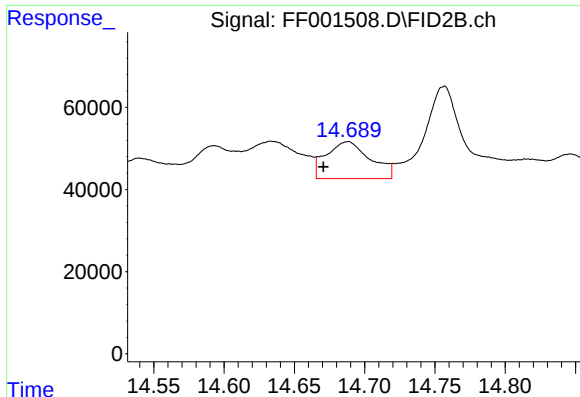

#10 N-TETRACOSANE


R.T.: 14.688 min
Delta R.T.: 0.017 min
Response: 197186
Conc: 1.62 ug/ml

Instrument :
FID_F
ClientSampleId :

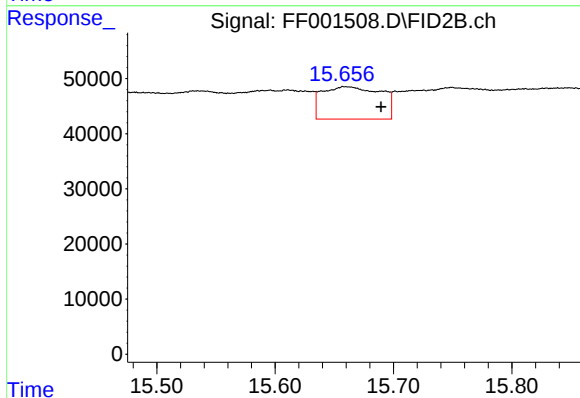


#11 N-HEXACOSANE

R.T.: 15.660 min
Delta R.T.: -0.029 min
Response: 202675
Conc: 1.67 ug/ml

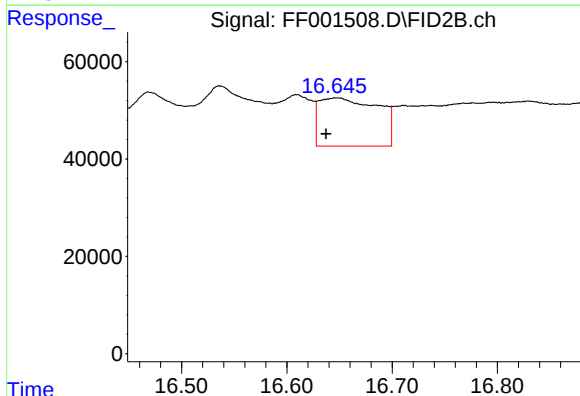


#12 N-OCTACOSANE

R.T.: 16.647 min
Delta R.T.: 0.010 min
Response: 386031
Conc: 3.20 ug/ml

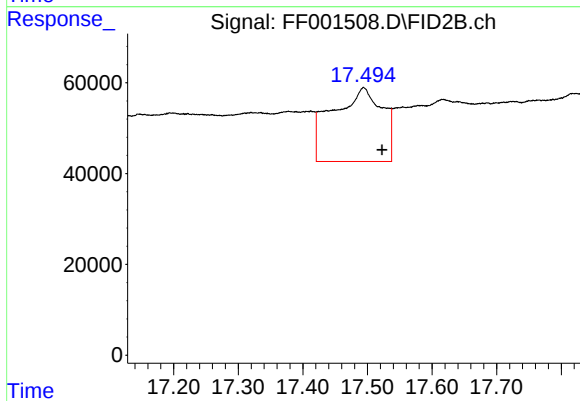

#13 N-TRIACONTANE


R.T.: 17.494 min
Delta R.T.: -0.029 min
Response: 873605
Conc: 7.27 ug/ml

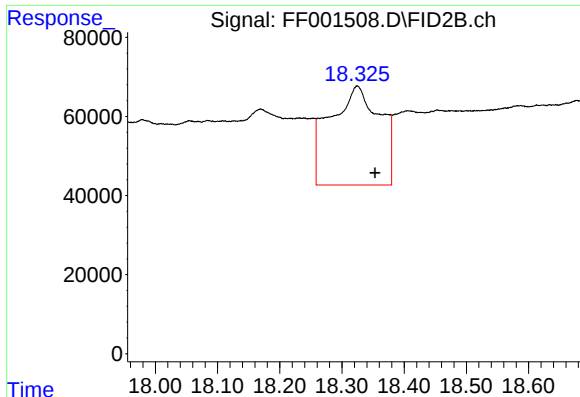

#14 N-DOTRIACONTANE


R.T.: 18.325 min
Delta R.T.: -0.029 min
Response: 1396043
Conc: 11.84 ug/ml

Instrument :
FID_F
ClientSampleId :

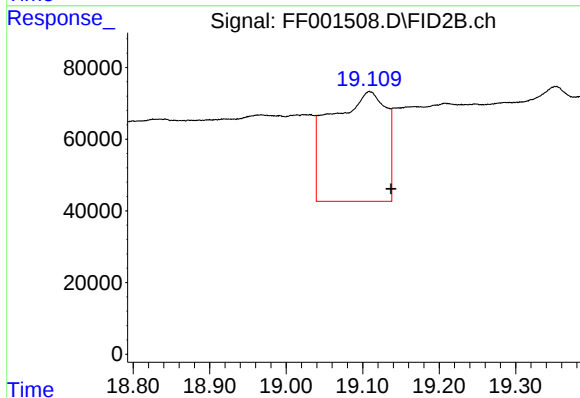


#15 N-TETRATRIACONTANE

R.T.: 19.109 min
Delta R.T.: -0.028 min
Response: 1554699
Conc: 13.23 ug/ml

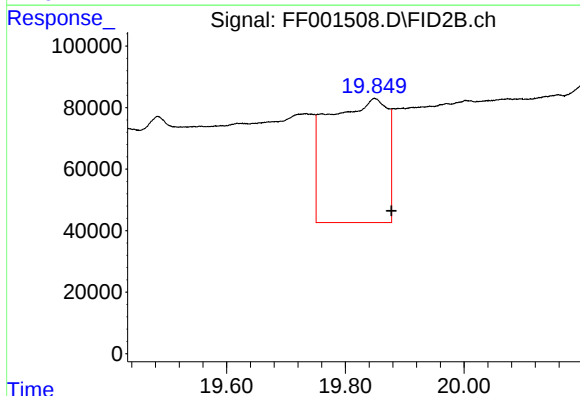


#16 N-HEXATRIACONTANE

R.T.: 19.849 min
Delta R.T.: -0.028 min
Response: 2800979
Conc: 24.66 ug/ml

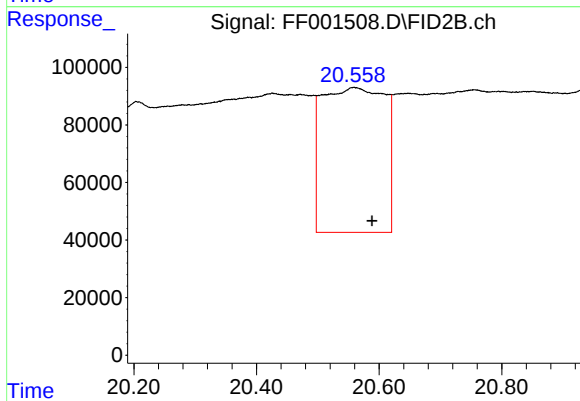

#17 N-OCTATRIACONTANE

R.T.: 20.559 min
Delta R.T.: -0.030 min
Response: 3588366
Conc: 34.75 ug/ml

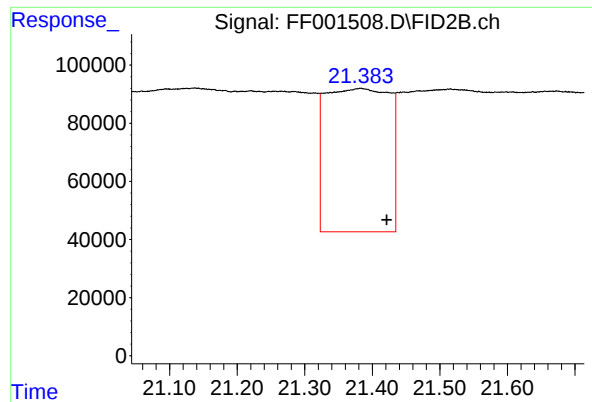

#18 N-TETRACONTANE

R.T.: 21.383 min
Delta R.T.: -0.038 min
Response: 3239364
Conc: 31.63 ug/ml

Instrument :
FID_F
ClientSampleId :