

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
 Data File : FF001512.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jul 2018 17:11
 Operator : AJ\SJ
 Sample : J4126-11 25X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jul 27 05:03:18 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.438	257584	2.391 ug/ml
Target Compounds			
3) N-DODECANE	6.223	6909	0.055 ug/ml
4) N-TETRADECANE	8.002	81011	0.644 ug/ml
5) N-HEXADECANE	9.621	74265	0.594 ug/ml
6) N-OCTADECANE	11.080	48366	0.386 ug/ml
7) N-EICOSANE	12.398	1800751	14.477 ug/ml
8) N-DOCOSANE	13.563	233145	1.891 ug/ml
10) N-TETRACOSANE	14.621	881924	7.234 ug/ml
11) N-HEXACOSANE	15.662	321153	2.649 ug/ml
12) N-OCTACOSANE	16.629	391207	3.247 ug/ml
13) N-TRIACONTANE	17.495	755452	6.284 ug/ml
14) N-DOTRIACONTANE	18.321	1481358	12.564 ug/ml
15) N-TETRATRIACONTANE	19.109	981048	8.347 ug/ml
16) N-HEXATRIACONTANE	19.893	812596	7.154 ug/ml
17) N-OCTATRIACONTANE	20.617	1716642	16.625 ug/ml
18) N-TETRACONTANE	21.428	2232474	21.801 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
Data File : FF001512.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2018 17:11
Operator : AJ\SJ
Sample : J4126-11 25X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jul 27 05:03:18 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

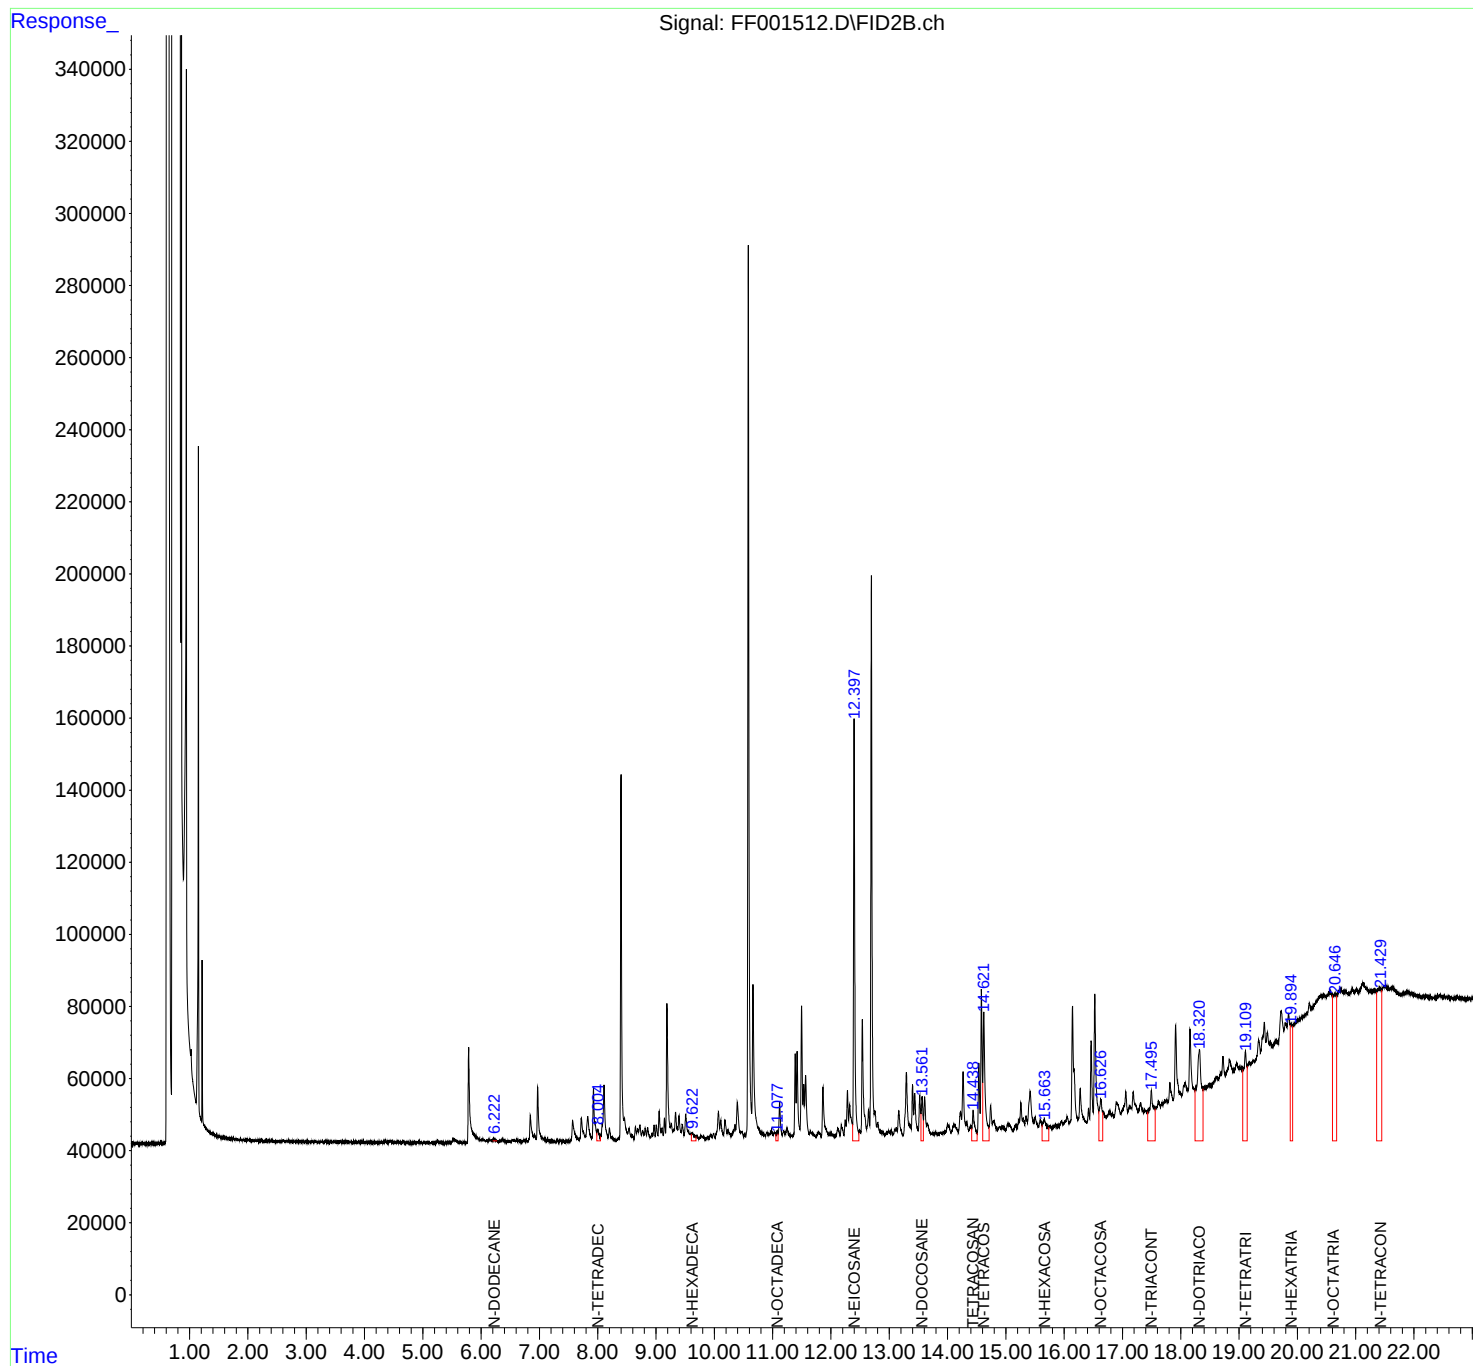


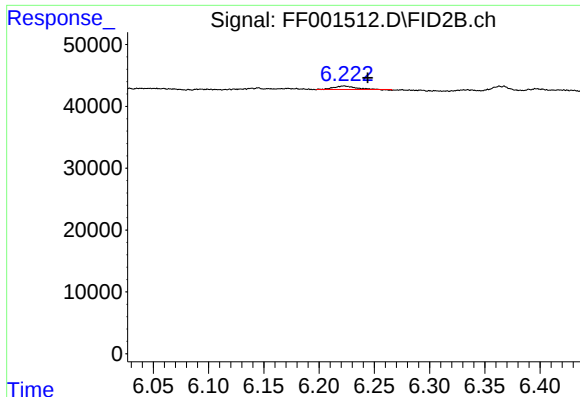

#3 N-DODECANE


R.T.: 6.223 min
Delta R.T.: -0.022 min
Response: 6909
Conc: 0.06 ug/ml

Instrument :
FID_F
ClientSampleId :

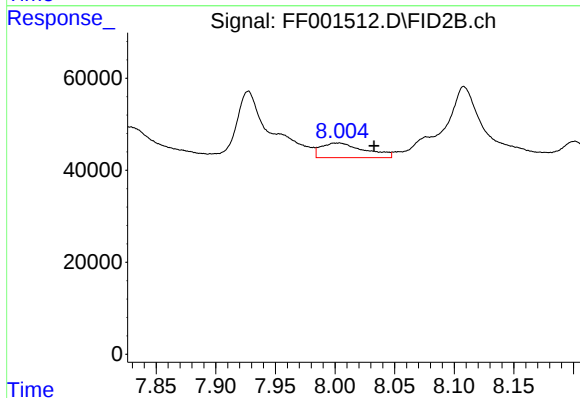


#4 N-TETRADECANE

R.T.: 8.002 min
Delta R.T.: -0.031 min
Response: 81011
Conc: 0.64 ug/ml

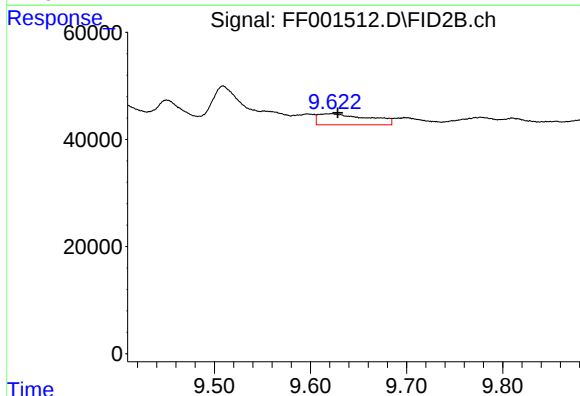


#5 N-HEXADECANE

R.T.: 9.621 min
Delta R.T.: -0.007 min
Response: 74265
Conc: 0.59 ug/ml

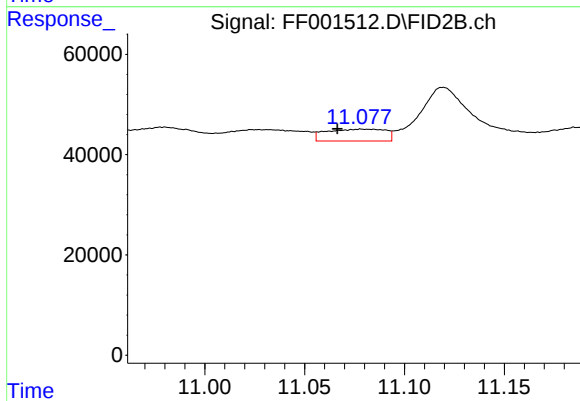

#6 N-OCTADECANE


R.T.: 11.080 min
Delta R.T.: 0.013 min
Response: 48366
Conc: 0.39 ug/ml

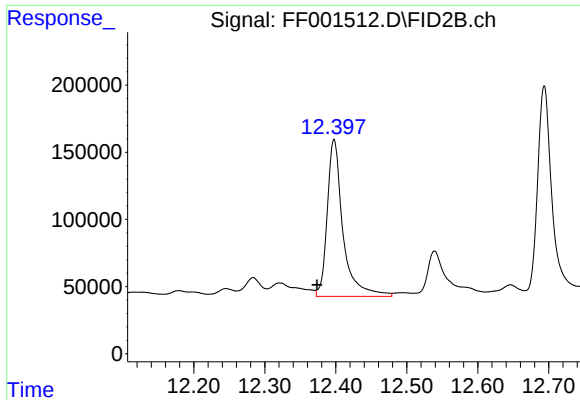

#7 N-EICOSANE


R.T.: 12.398 min
Delta R.T.: 0.024 min
Response: 1800751
Conc: 14.48 ug/ml

Instrument :
FID_F
ClientSampleId :

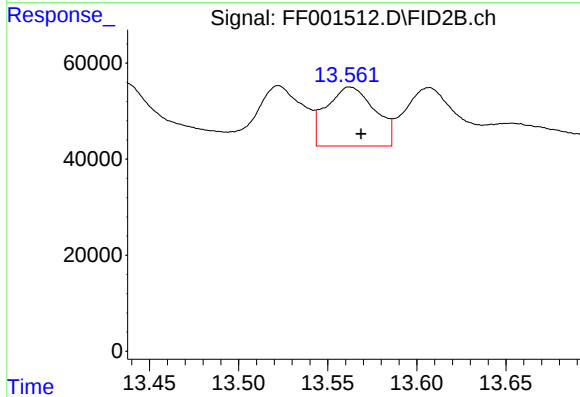


#8 N-DOCOSANE

R.T.: 13.563 min
Delta R.T.: -0.006 min
Response: 233145
Conc: 1.89 ug/ml

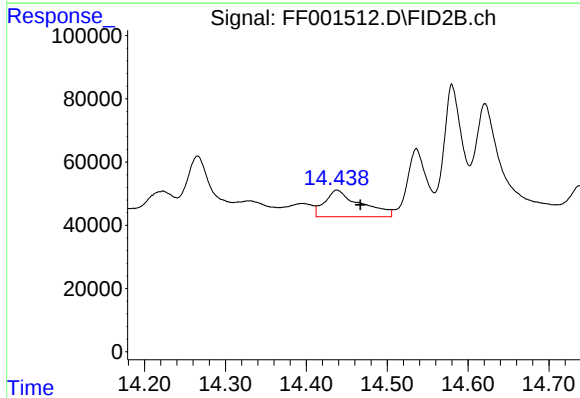


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.438 min
Delta R.T.: -0.029 min
Response: 257584
Conc: 2.39 ug/ml

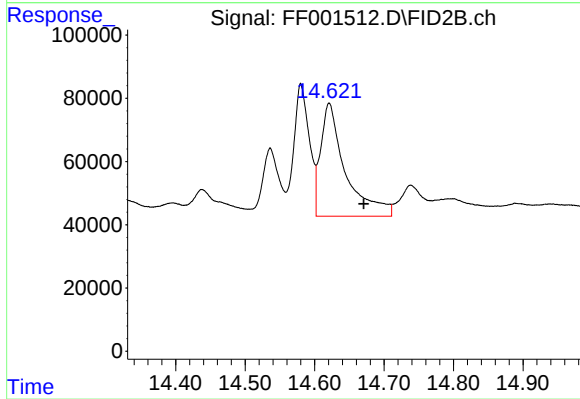

#10 N-TETRACOSANE


R.T.: 14.621 min
Delta R.T.: -0.050 min
Response: 881924
Conc: 7.23 ug/ml

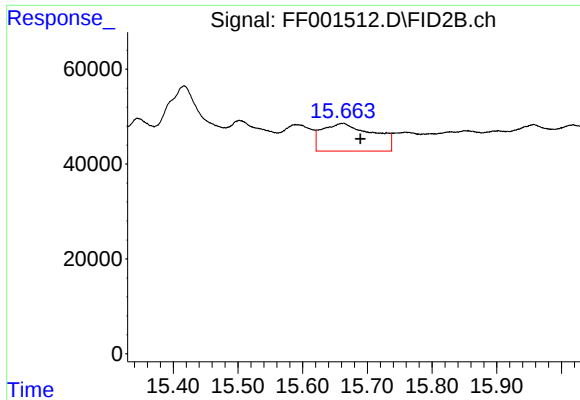

#11 N-HEXACOSANE


R.T.: 15.662 min
Delta R.T.: -0.028 min
Response: 321153
Conc: 2.65 ug/ml

Instrument :
FID_F
ClientSampleId :

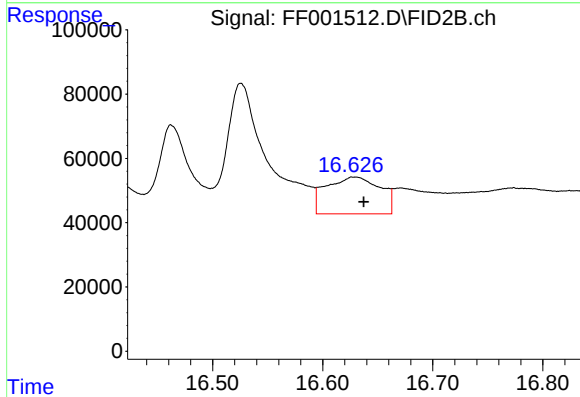


#12 N-OCTACOSANE

R.T.: 16.629 min
Delta R.T.: -0.008 min
Response: 391207
Conc: 3.25 ug/ml

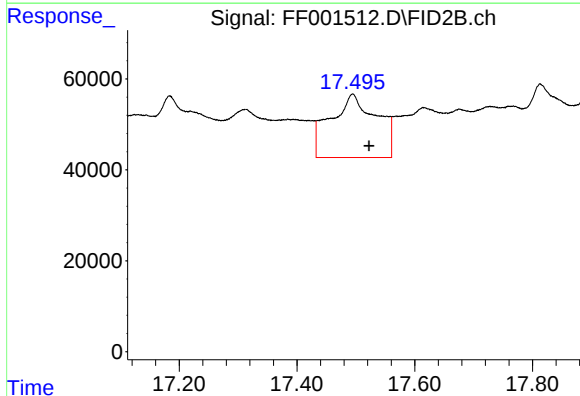


#13 N-TRIACONTANE

R.T.: 17.495 min
Delta R.T.: -0.028 min
Response: 755452
Conc: 6.28 ug/ml

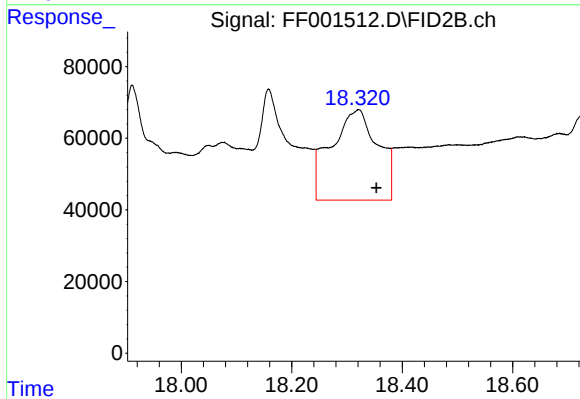

#14 N-DOTRIACONTANE


R.T.: 18.321 min
Delta R.T.: -0.033 min
Response: 1481358
Conc: 12.56 ug/ml

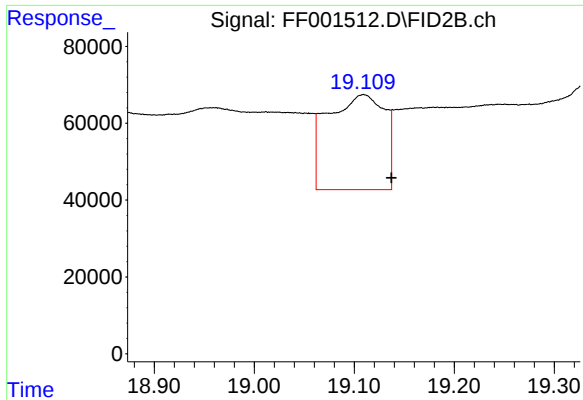

#15 N-TETRATRIACONTANE


R.T.: 19.109 min
Delta R.T.: -0.028 min
Response: 981048
Conc: 8.35 ug/ml

Instrument :
FID_F
ClientSampleId :

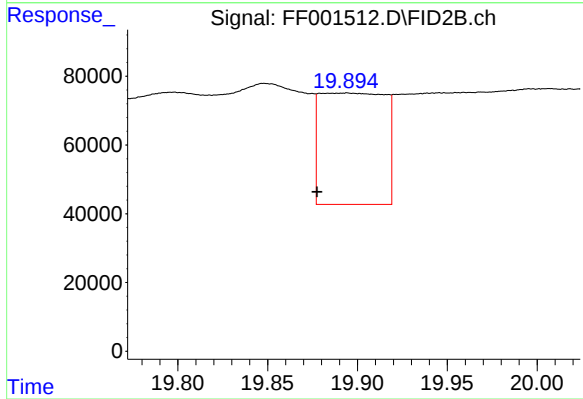


#16 N-HEXATRIACONTANE

R.T.: 19.893 min
Delta R.T.: 0.016 min
Response: 812596
Conc: 7.15 ug/ml

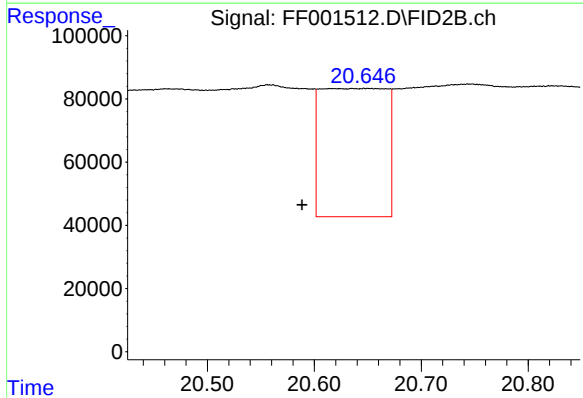

#17 N-OCTATRIACONTANE

R.T.: 20.617 min
Delta R.T.: 0.028 min
Response: 1716642
Conc: 16.63 ug/ml

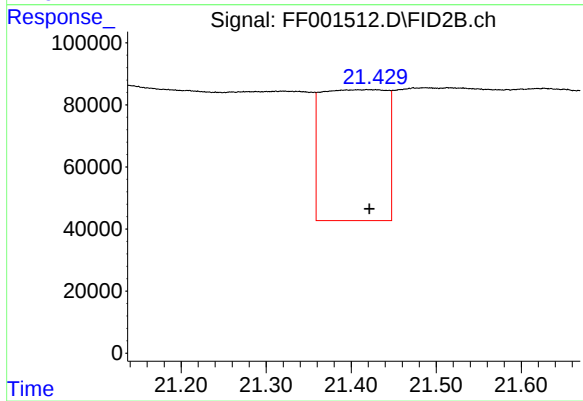

#18 N-TETRACONTANE

R.T.: 21.428 min
Delta R.T.: 0.007 min
Response: 2232474
Conc: 21.80 ug/ml