

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
 Data File : FF001513.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jul 2018 17:42
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jul 27 05:03:26 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.441	2250897	20.895 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.668	38065	0.314 ug/ml
12) N-OCTACOSANE	16.612	167243	1.388 ug/ml
13) N-TRIACONTANE	17.497	1043261	8.679 ug/ml
14) N-DOTRIACONTANE	18.327	2034932	17.259 ug/ml
15) N-TETRATRIACONTANE	19.110	1392331	11.846 ug/ml
16) N-HEXATRIACONTANE	19.851	4891465	43.061 ug/ml
17) N-OCTATRIACONTANE	20.560	7210846	69.835 ug/ml
18) N-TETRACONTANE	21.382	3328367	32.503 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072618\
Data File : FF001513.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2018 17:42
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jul 27 05:03:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

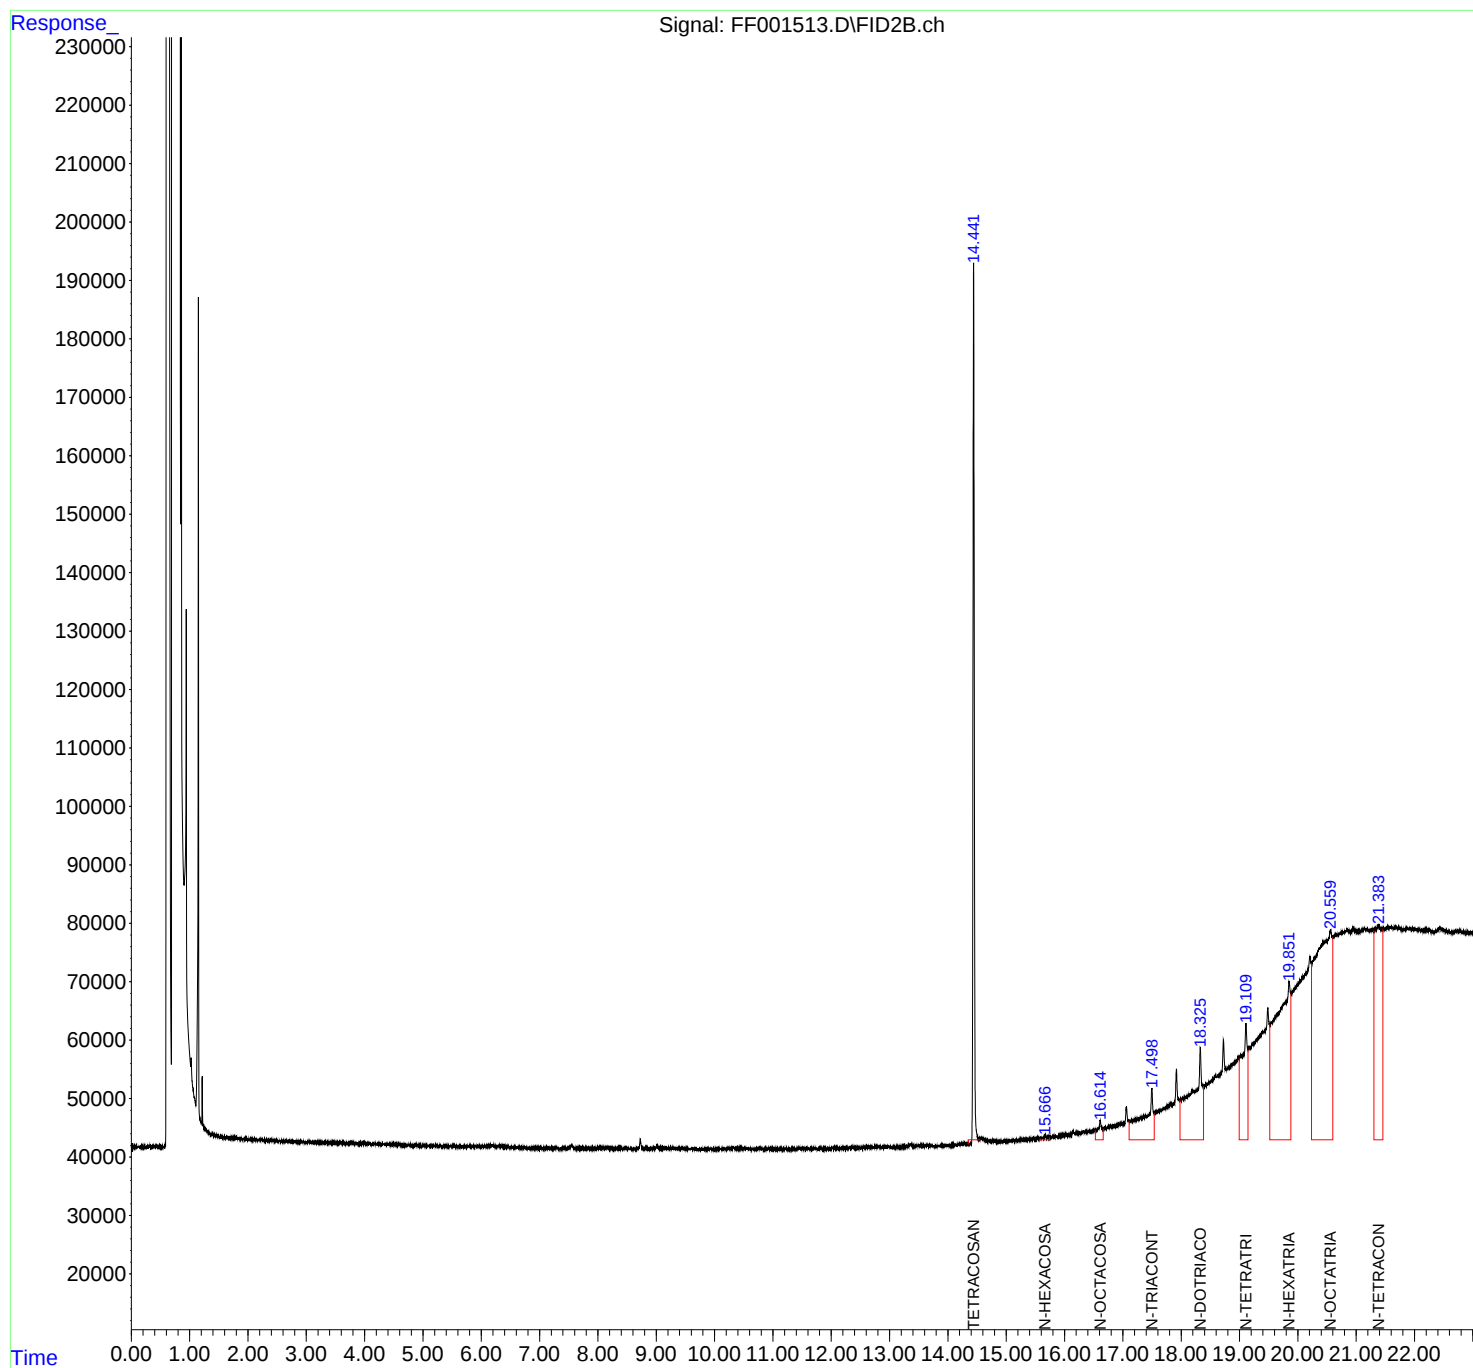


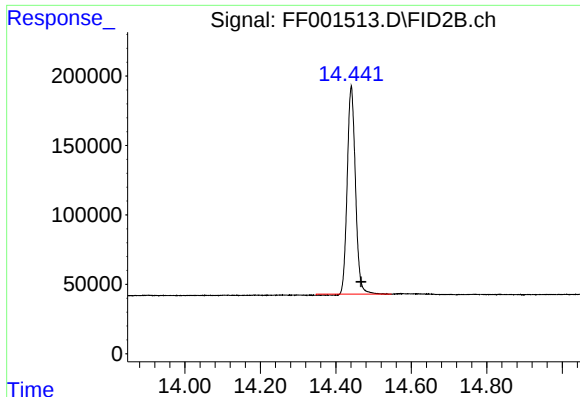

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.441 min
Delta R.T.: -0.026 min
Response: 2250897
Conc: 20.90 ug/ml

Instrument :
FID_F
ClientSampleId :

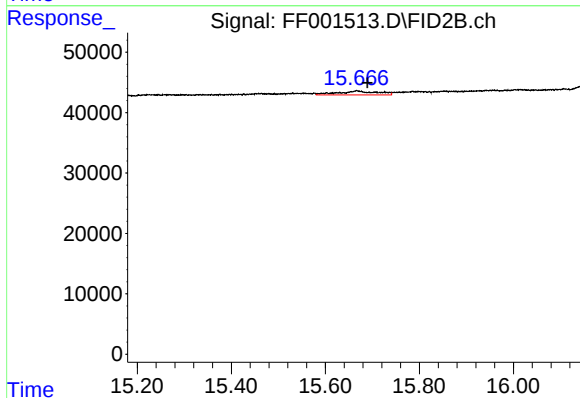


#11 N-HEXACOSANE

R.T.: 15.668 min
Delta R.T.: -0.022 min
Response: 38065
Conc: 0.31 ug/ml

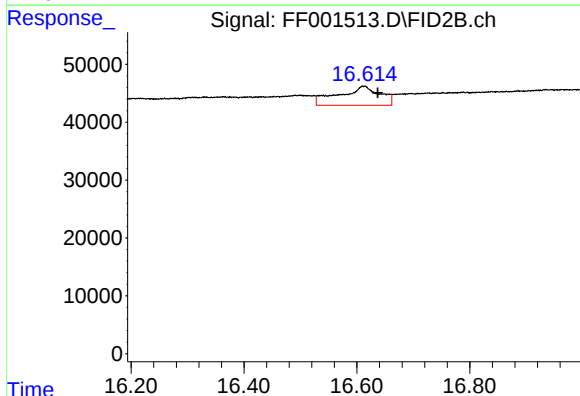


#12 N-OCTACOSANE

R.T.: 16.612 min
Delta R.T.: -0.025 min
Response: 167243
Conc: 1.39 ug/ml

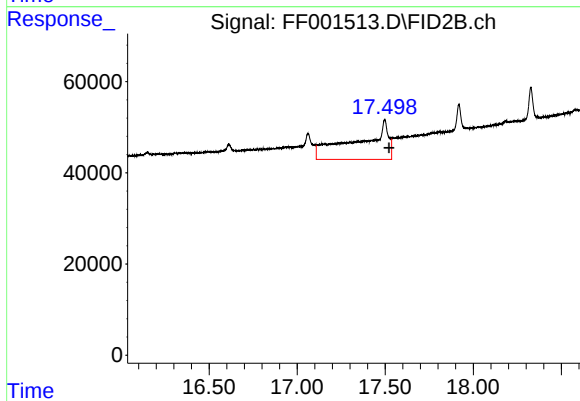

#13 N-TRIACONTANE


R.T.: 17.497 min
Delta R.T.: -0.026 min
Response: 1043261
Conc: 8.68 ug/ml

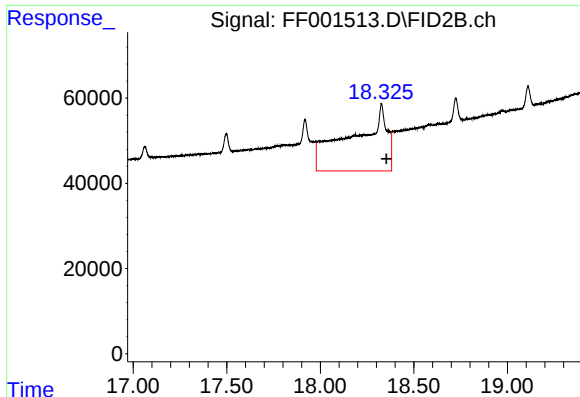

#14 N-DOTRIACONTANE


R.T.: 18.327 min
Delta R.T.: -0.026 min
Response: 2034932
Conc: 17.26 ug/ml

Instrument :
FID_F
ClientSampleId :

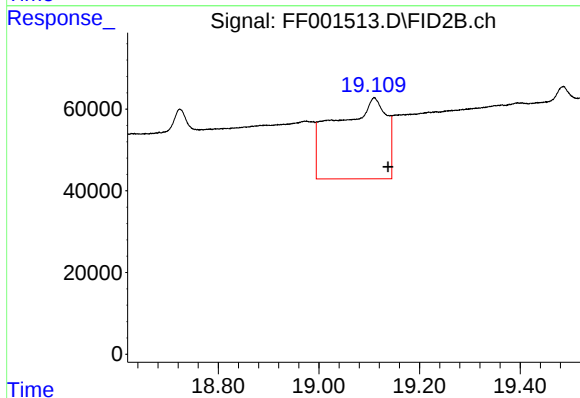


#15 N-TETRATRIACONTANE

R.T.: 19.110 min
Delta R.T.: -0.027 min
Response: 1392331
Conc: 11.85 ug/ml

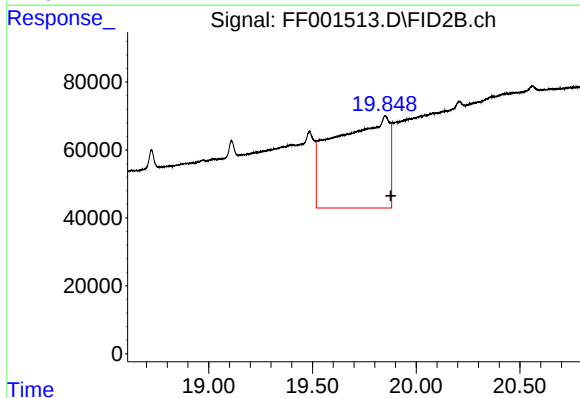


#16 N-HEXATRIACONTANE

R.T.: 19.851 min
Delta R.T.: -0.026 min
Response: 4891465
Conc: 43.06 ug/ml

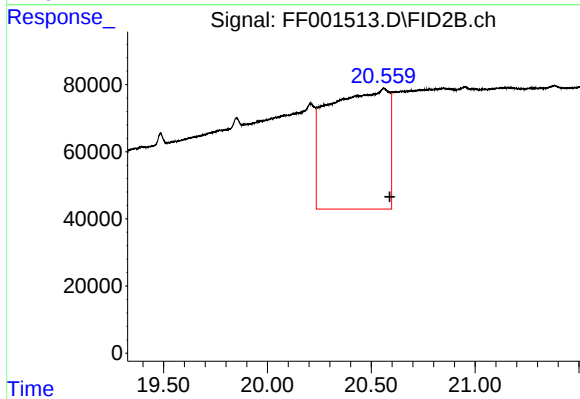

#17 N-OCTATRIACONTANE

R.T.: 20.560 min
Delta R.T.: -0.028 min
Response: 7210846
Conc: 69.84 ug/ml

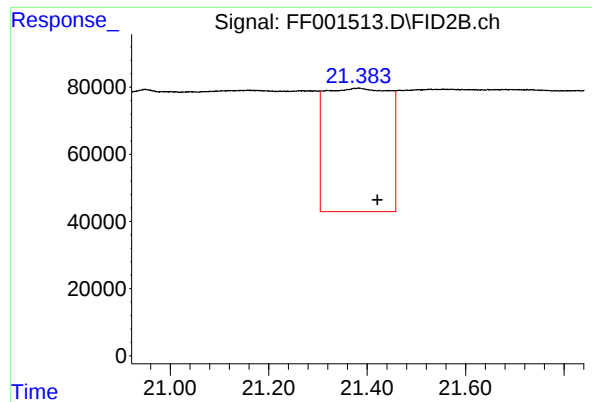

#18 N-TETRACONTANE

R.T.: 21.382 min
Delta R.T.: -0.040 min
Response: 3328367
Conc: 32.50 ug/ml

Instrument :
FID_F
ClientSampleId :