

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072621\
Data File : FF008872.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2021 11:01
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 01:18:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.516	2736341	20.623 ug/ml
12)	N-OCTACOSANE	16.915	2933702	21.930 ug/ml
13)	N-TRIACONTANE	17.799	241961	1.851 ug/ml
14)	N-DOTRIACONTANE	18.629	316097	2.555 ug/ml
15)	N-TETRATRIACONTANE	19.408	259611	2.229 ug/ml
16)	N-HEXATRIACONTANE	20.145	174454	1.642 ug/ml
17)	N-OCTATRIACONTANE	20.890	118546	1.215 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072621\
Data File : FF008872.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2021 11:01
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 01:18:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

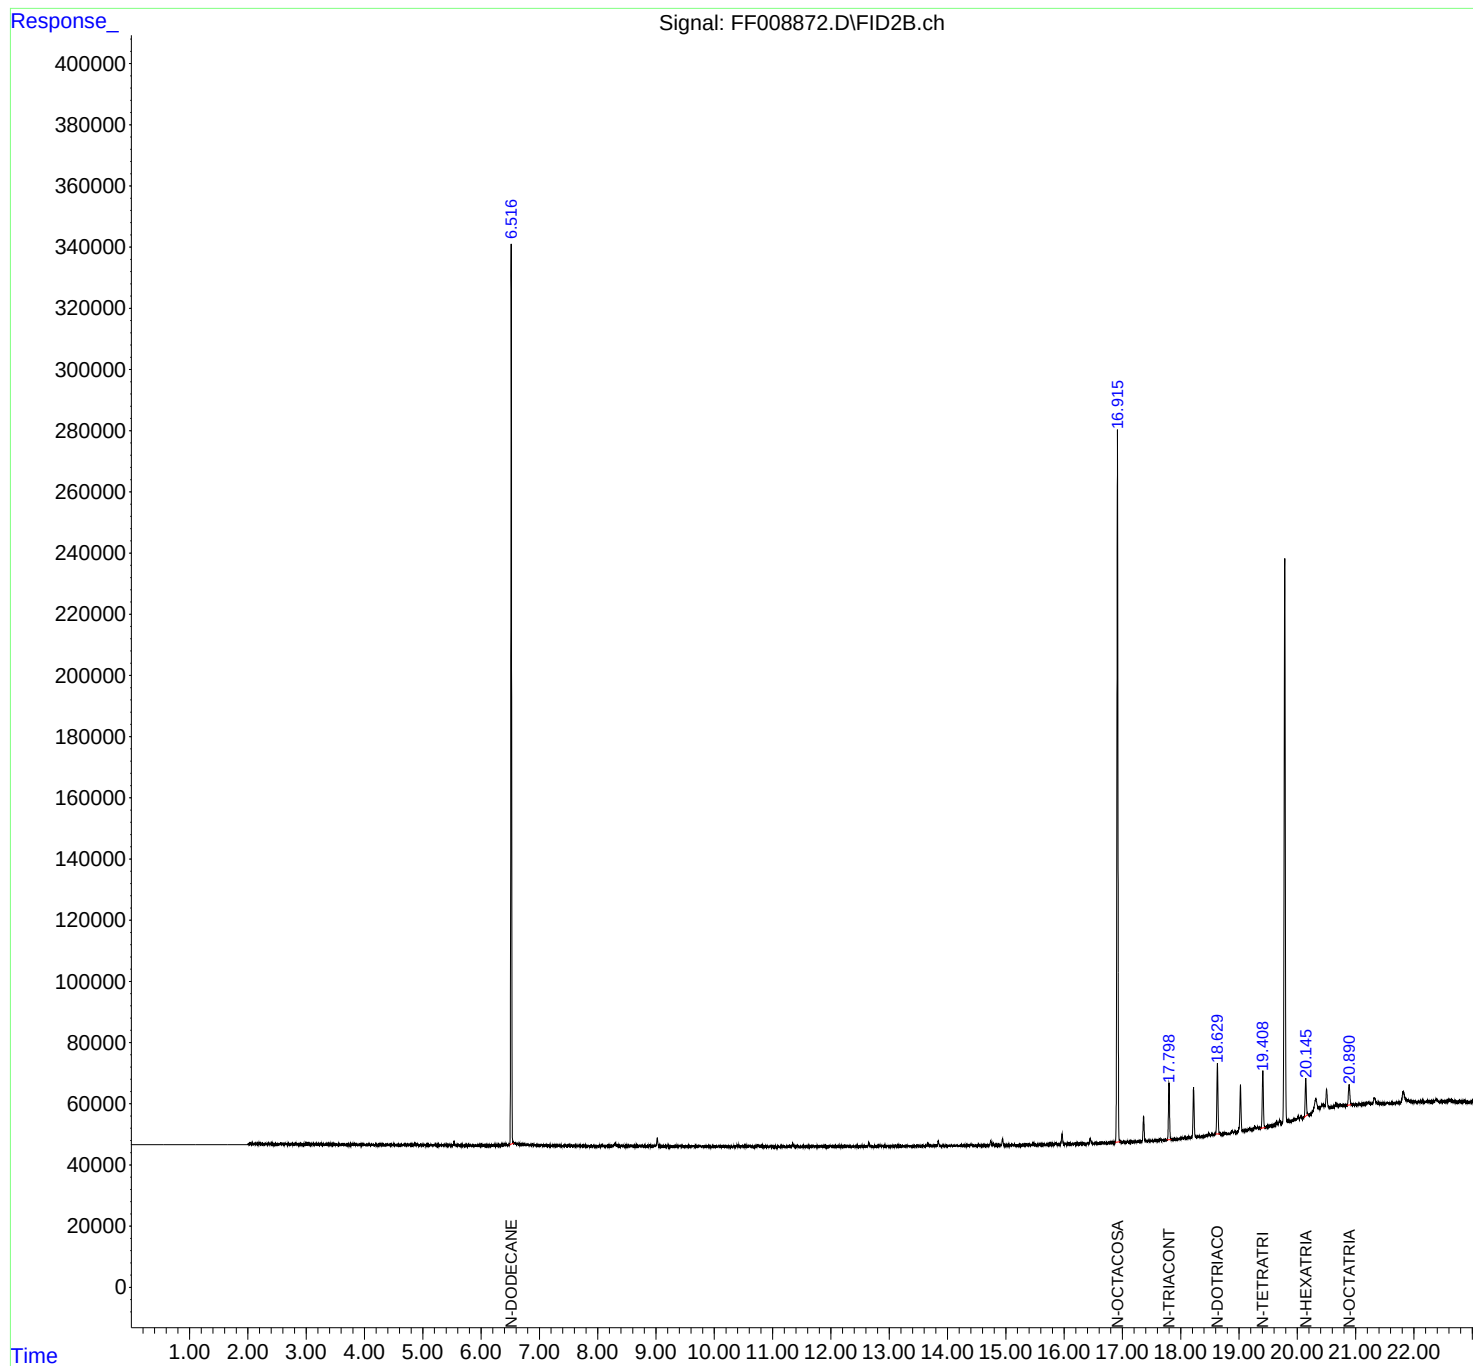


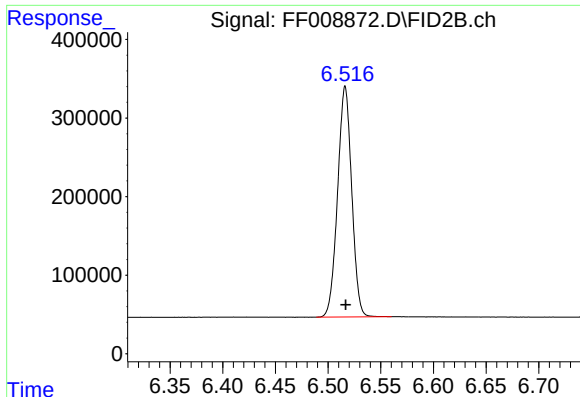

#3 N-DODECANE


R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 2736341
Conc: 20.62 ug/ml

Instrument :
FID_F
ClientSampleId :

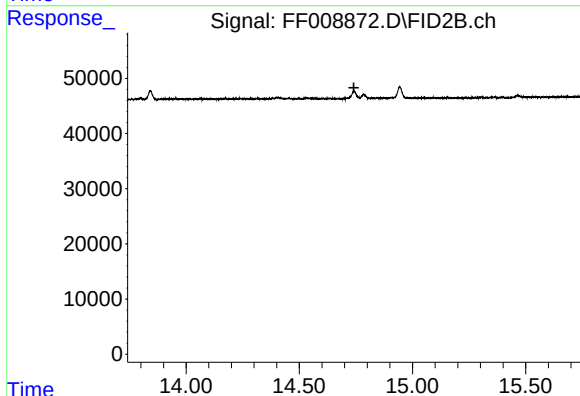


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.741 min
Response: 0
Conc: N.D.

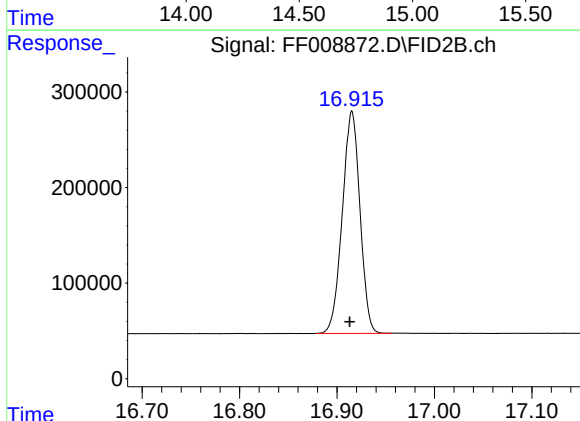


#12 N-OCTACOSANE

R.T.: 16.915 min
Delta R.T.: 0.002 min
Response: 2933702
Conc: 21.93 ug/ml

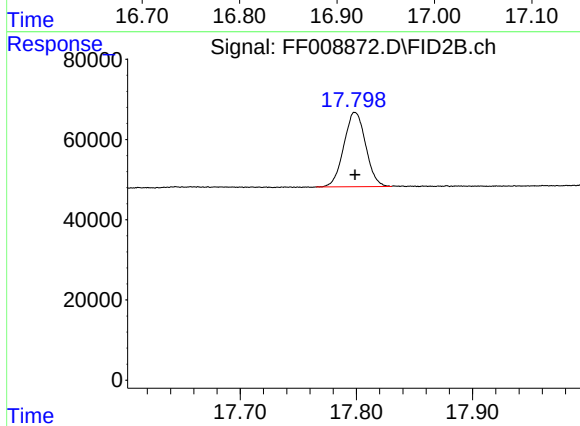

#13 N-TRIACONTANE


R.T.: 17.799 min
Delta R.T.: 0.000 min
Response: 241961
Conc: 1.85 ug/ml

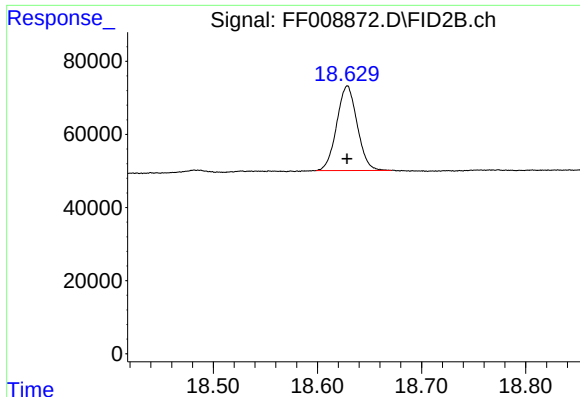

#14 N-DOTRIACONTANE


R.T.: 18.629 min
Delta R.T.: 0.000 min
Response: 316097
Conc: 2.56 ug/ml

Instrument :
FID_F
ClientSampleId :

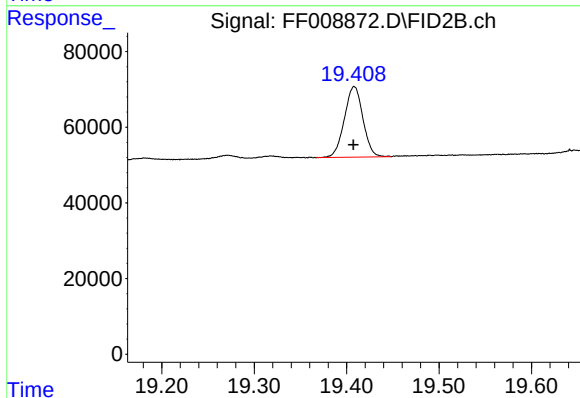


#15 N-TETRATRIACONTANE

R.T.: 19.408 min
Delta R.T.: 0.000 min
Response: 259611
Conc: 2.23 ug/ml

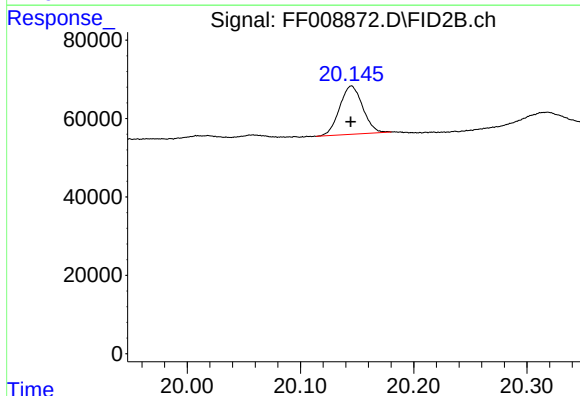

#16 N-HEXATRIACONTANE

R.T.: 20.145 min
Delta R.T.: 0.000 min
Response: 174454
Conc: 1.64 ug/ml

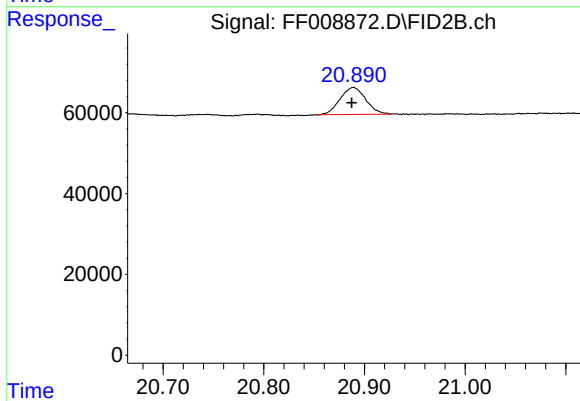

#17 N-OCTATRIACONTANE

R.T.: 20.890 min
Delta R.T.: 0.002 min
Response: 118546
Conc: 1.21 ug/ml