

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072621\
Data File : FF008887.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2021 19:30
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 01:19:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.743	1831904	15.290 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.632	95530	0.772 ug/ml
15) N-TETRATRIACONTANE	19.412	170827	1.466 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072621\
Data File : FF008887.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2021 19:30
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 01:19:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

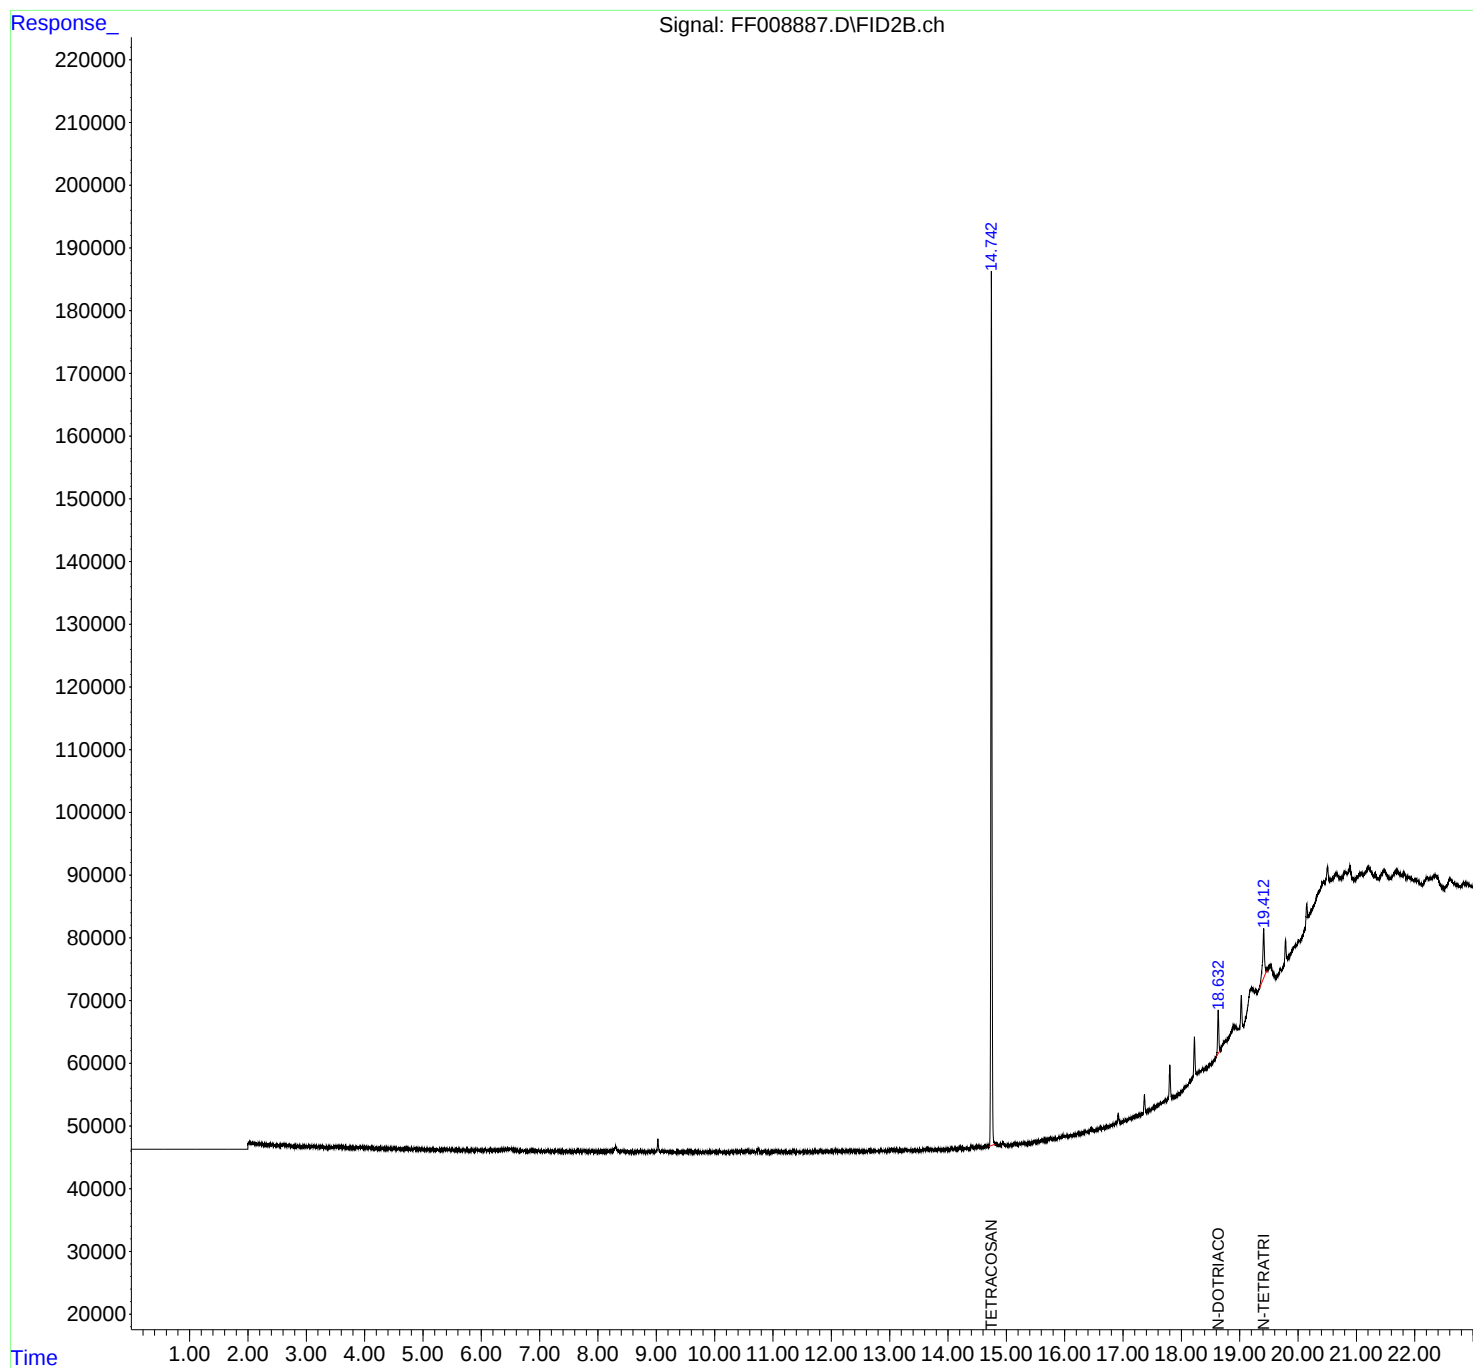


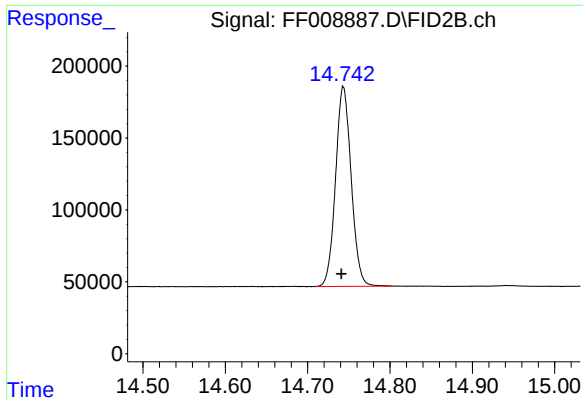

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.743 min
Delta R.T.: 0.002 min
Response: 1831904
Conc: 15.29 ug/ml

Instrument :
FID_F
ClientSampleId :

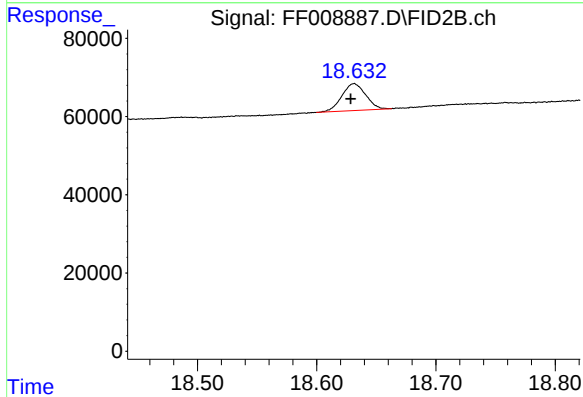

#14 N-DOTRIACONTANE

R.T.: 18.632 min
Delta R.T.: 0.003 min
Response: 95530
Conc: 0.77 ug/ml

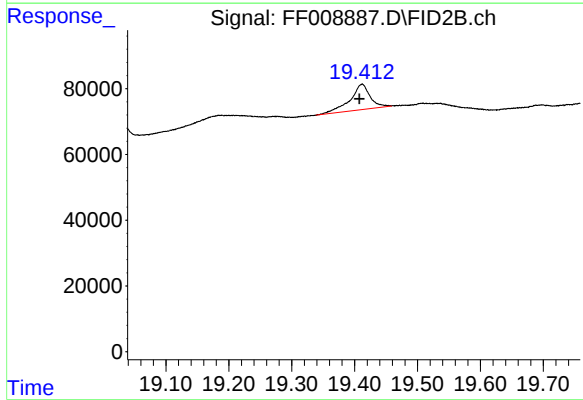

#15 N-TETRATRIACONTANE

R.T.: 19.412 min
Delta R.T.: 0.005 min
Response: 170827
Conc: 1.47 ug/ml