

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072622\
Data File : FF011098.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2022 15:44
Operator : YP\AJ
Sample : N3839-04
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FIELD-DUPLICATE-01

Integration File: autoint1.e
Quant Time: Jul 27 02:00:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.806	1213467	12.935 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072622\
Data File : FF011098.D
Signal(s) : FID2B.ch
Acq On : 26 Jul 2022 15:44
Operator : YP\AJ
Sample : N3839-04
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FIELD-DUPLICATE-01

Integration File: autoint1.e
Quant Time: Jul 27 02:00:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

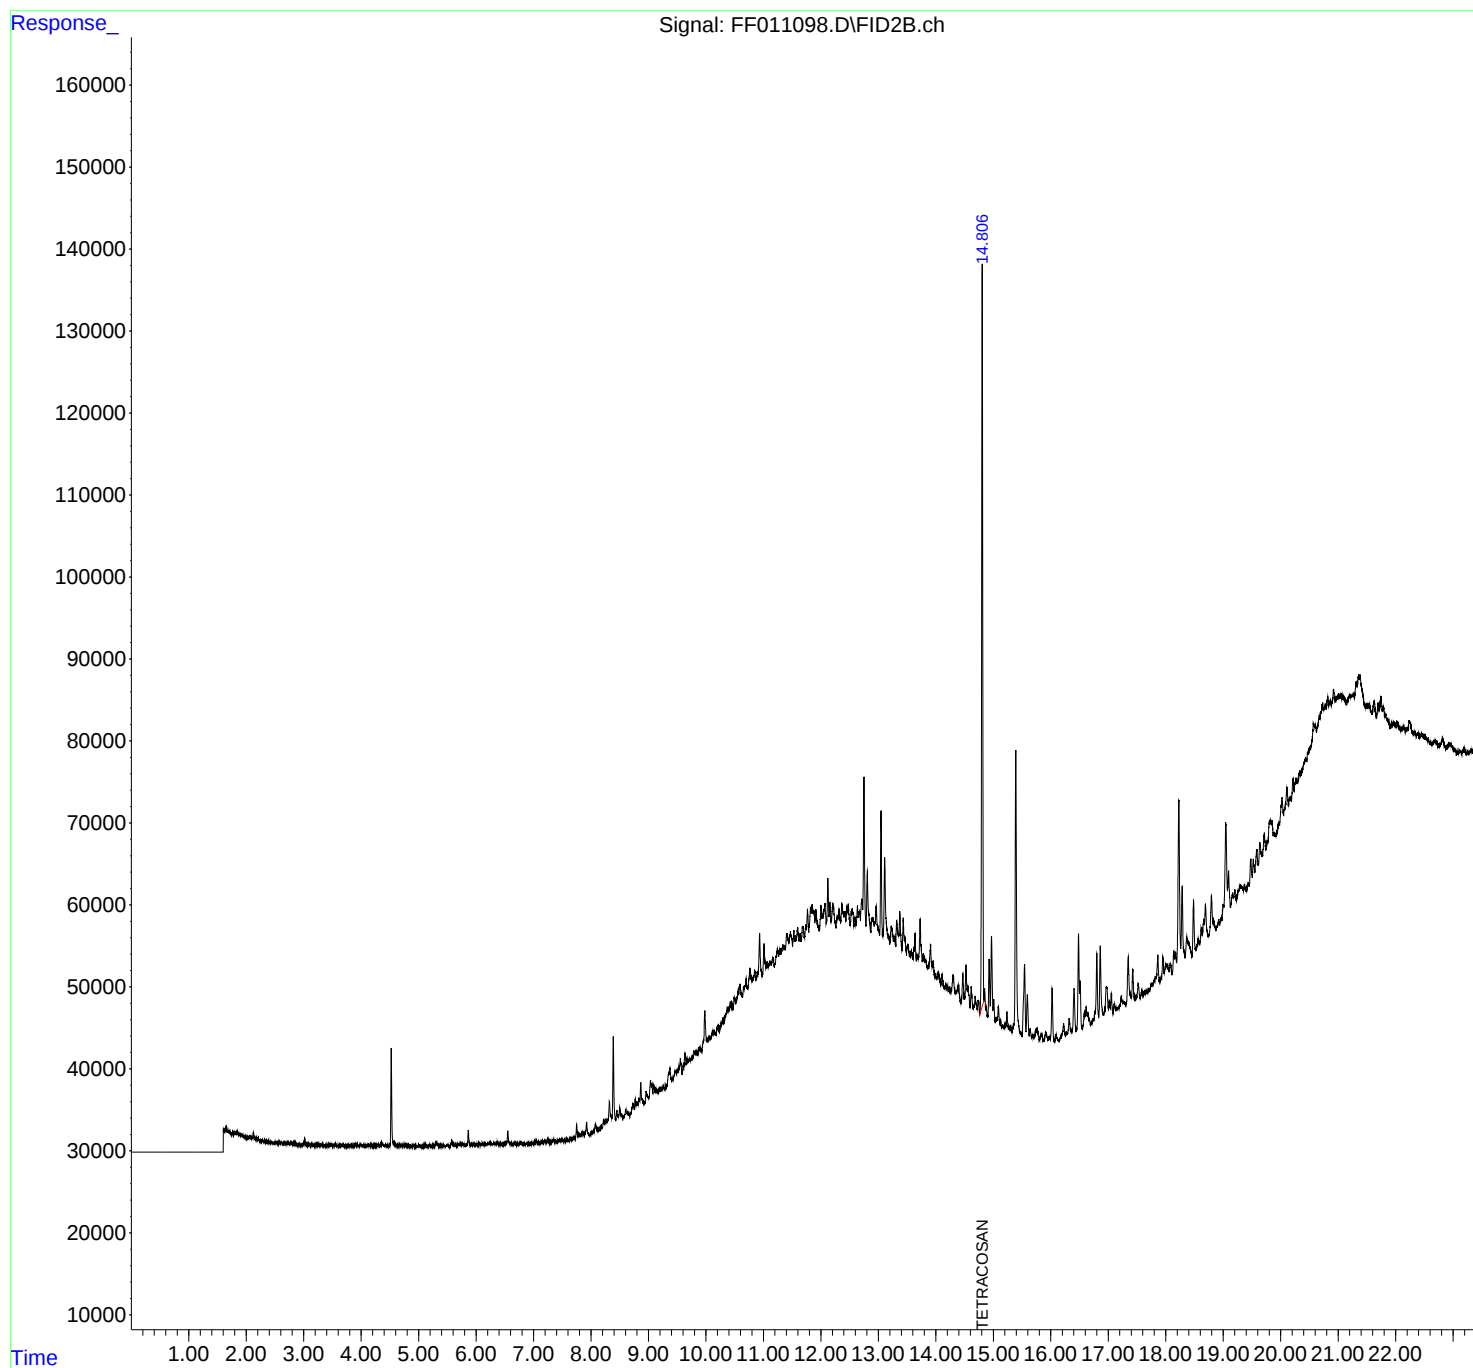

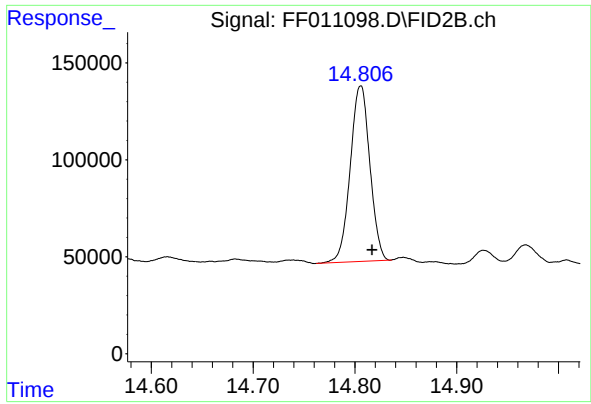

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.806 min
Delta R.T.: -0.011 min
Response: 1213467
Conc: 12.94 ug/ml

Instrument :
FID_F
ClientSampleId :
FIELD-DUPLICATE-01